

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022775.D
 Acq On : 31 Oct 2024 18:21
 Operator : RC/JU
 Sample : P4630-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	29	rBV3	3671	4108	0.13%	0.018%
2	3.175	29	32	39	rVB	13364	18287	0.60%	0.079%
3	3.599	100	104	121	rBV	43377	82151	2.68%	0.354%
4	3.905	152	156	161	rVB4	4236	6246	0.20%	0.027%
5	4.417	237	243	253	rVB	82756	125616	4.10%	0.541%
6	6.775	638	644	647	rBV	7571	11560	0.38%	0.050%
7	6.828	647	653	665	rVV	75280	139712	4.56%	0.602%
8	6.975	671	678	692	rBV	237459	368002	12.01%	1.584%
9	7.175	704	712	723	rBV	292980	471921	15.40%	2.032%
10	7.628	780	789	799	rBV	279463	451482	14.73%	1.944%
11	8.334	901	909	924	rBV	245575	419415	13.68%	1.806%
12	8.769	974	983	1000	rBV	309980	548148	17.89%	2.360%
13	9.175	1044	1052	1062	rBV	11730	21189	0.69%	0.091%
14	9.487	1098	1105	1119	rBV	280195	488588	15.94%	2.104%
15	10.028	1188	1197	1221	rBV	360159	746709	24.36%	3.215%
16	10.387	1250	1258	1271	rVB	346884	594756	19.41%	2.561%
17	10.534	1275	1283	1306	rBV	248199	473426	15.45%	2.038%
18	10.752	1316	1320	1324	rVB6	3060	4422	0.14%	0.019%
19	11.228	1395	1401	1403	rBV6	4326	7512	0.25%	0.032%
20	11.657	1468	1474	1479	rBV	6641	9375	0.31%	0.040%
21	11.987	1523	1530	1536	rBV2	6157	12897	0.42%	0.056%
22	13.140	1717	1726	1730	rBV7	2214	3570	0.12%	0.015%
23	13.663	1808	1815	1826	rBV	749633	1134198	37.01%	4.883%
24	13.940	1854	1862	1875	rBV	831311	1275574	41.62%	5.492%
25	14.251	1908	1915	1928	rBV	548878	899075	29.34%	3.871%
26	14.522	1956	1961	1980	rBV2	39311	120084	3.92%	0.517%
27	15.263	2080	2087	2095	rBV	1207694	1715629	55.98%	7.387%
28	15.340	2095	2100	2107	rVV4	18556	34487	1.13%	0.148%
29	15.422	2107	2114	2128	rVV	339703	510111	16.64%	2.196%
30	15.522	2128	2131	2137	rVB3	8031	11355	0.37%	0.049%
31	16.481	2287	2294	2296	rBV8	2821	4515	0.15%	0.019%
32	17.063	2386	2393	2404	rBV	742206	1214807	39.64%	5.230%
33	17.175	2404	2412	2425	rBV2	1316922	2087930	68.13%	8.989%
34	17.486	2461	2465	2471	rBV9	2161	4734	0.15%	0.020%
35	17.769	2507	2513	2517	rBV7	4295	8950	0.29%	0.039%
36	17.998	2547	2552	2559	rBV3	23987	40649	1.33%	0.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022775.D
Acq On : 31 Oct 2024 18:21
Operator : RC/JU
Sample : P4630-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	19.092	2734	2738	2743	rBV3	19501	26692	0.87%	0.115%
38	19.169	2747	2751	2754	rVV	19429	30439	0.99%	0.131%
39	19.210	2754	2758	2767	rVB4	59068	90425	2.95%	0.389%
40	19.333	2775	2779	2785	rVB5	22445	35955	1.17%	0.155%
41	19.545	2809	2815	2824	rBV	1981496	2661834	86.85%	11.460%
42	21.510	3143	3149	3161	rBV2	989870	1543225	50.35%	6.644%
43	24.539	3654	3664	3679	rVB	1309640	3064816	100.00%	13.195%
44	24.774	3695	3704	3720	rVB	617234	1701869	55.53%	7.327%


Sum of corrected areas: 23226445

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022775.D
Acq On : 31 Oct 2024 18:21
Operator : RC/JU
Sample : P4630-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

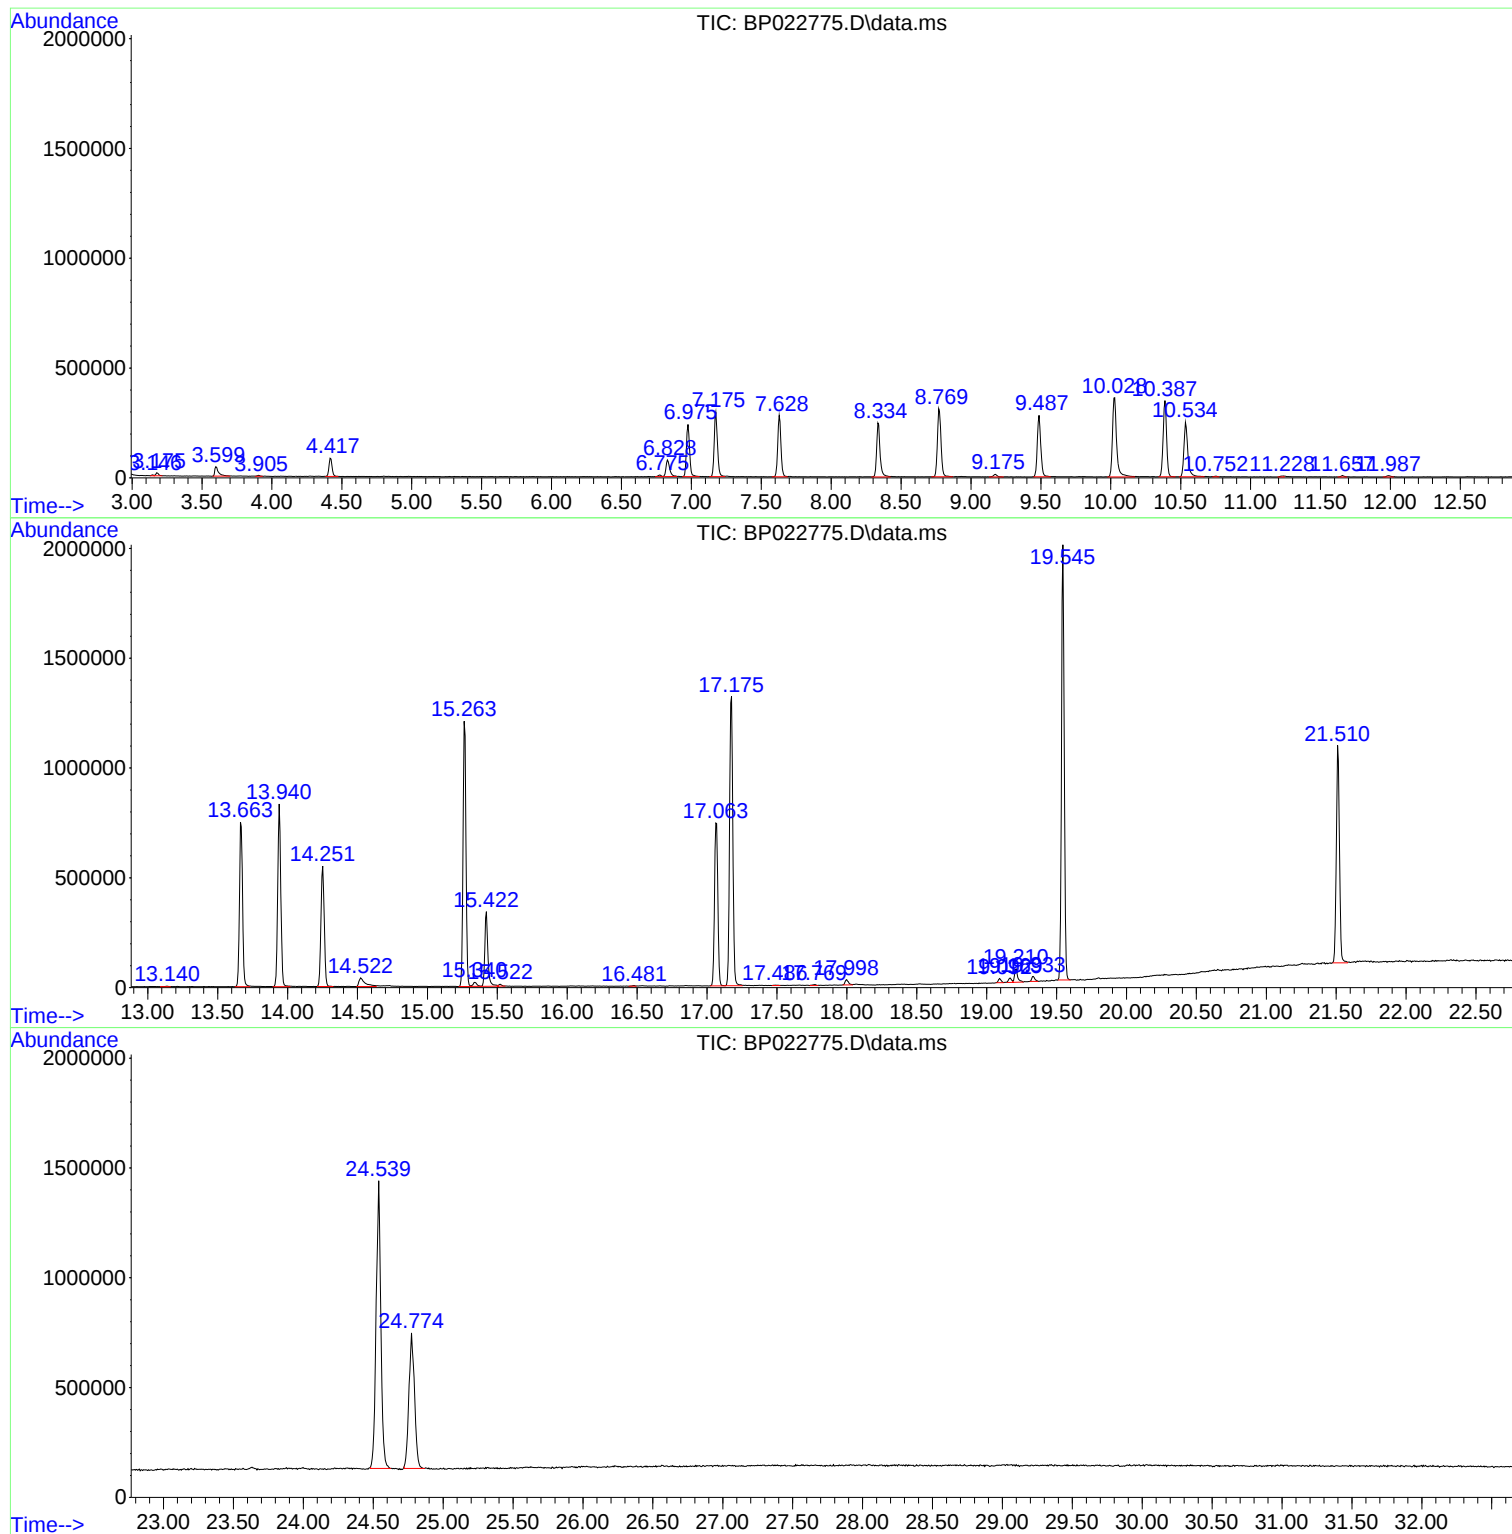

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022775.D
Acq On : 31 Oct 2024 18:21
Operator : RC/JU
Sample : P4630-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP02









Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.417	5.56 ng/ul	125616	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	16

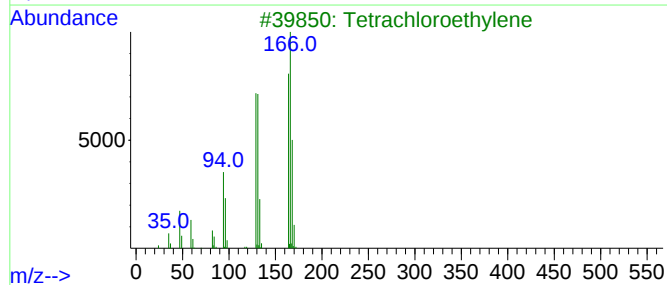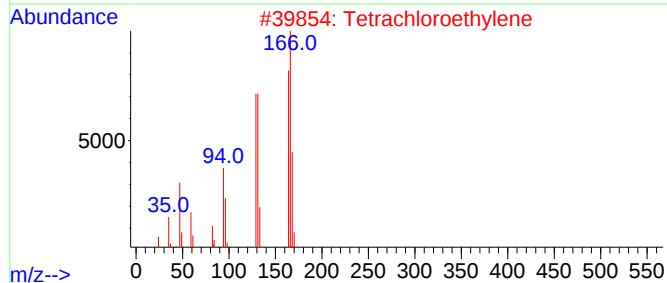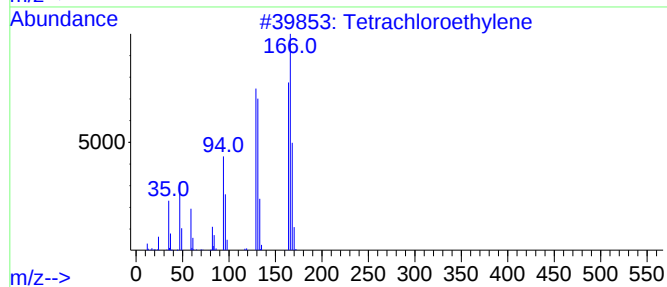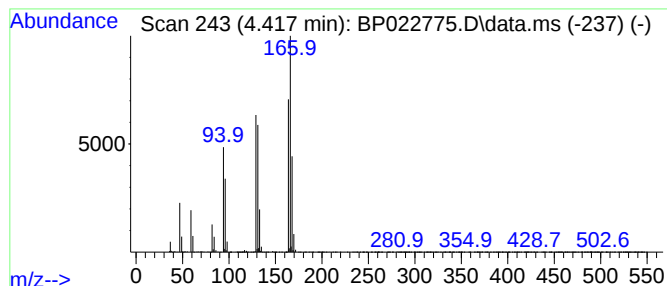

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022775.D
Acq On : 31 Oct 2024 18:21
Operator : RC/JU
Sample : P4630-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.417	5.6	ng/ul	125616	1	7.628	451482	20.0