

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022789.D
 Acq On : 01 Nov 2024 04:33
 Operator : RC/JU
 Sample : P4630-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	34	rBV	14890	16950	0.46%	0.058%
2	3.211	34	38	45	rVB	54524	71873	1.96%	0.247%
3	3.599	100	104	114	rBV	40549	74522	2.03%	0.256%
4	3.752	127	130	137	rVB2	4451	7042	0.19%	0.024%
5	3.899	152	155	160	rVB2	5261	6798	0.18%	0.023%
6	4.328	225	228	234	rBV6	4620	7927	0.22%	0.027%
7	4.417	239	243	251	rVB7	4422	7291	0.20%	0.025%
8	6.393	574	579	581	rBV6	2372	3912	0.11%	0.013%
9	6.769	640	643	648	rVV2	4419	5993	0.16%	0.021%
10	6.828	648	653	666	rVB	96158	177717	4.84%	0.610%
11	6.975	672	678	692	rVB	284603	442682	12.04%	1.520%
12	7.175	704	712	723	rBV	327962	563543	15.33%	1.936%
13	7.628	782	789	800	rBV	340527	570548	15.52%	1.960%
14	8.340	903	910	932	rBV	283077	539728	14.68%	1.854%
15	8.593	947	953	959	rVB	28720	46227	1.26%	0.159%
16	8.687	964	969	975	rBV2	3357	5558	0.15%	0.019%
17	8.769	975	983	997	rBV	370561	647924	17.63%	2.225%
18	9.175	1046	1052	1060	rVB	8734	13612	0.37%	0.047%
19	9.481	1097	1104	1119	rBV	351274	584910	15.91%	2.009%
20	10.022	1186	1196	1219	rBV	445865	901566	24.53%	3.097%
21	10.387	1249	1258	1266	rBV	464093	762783	20.75%	2.620%
22	10.534	1275	1283	1299	rBV	288717	567994	15.45%	1.951%
23	11.216	1389	1399	1401	rBV8	5871	11468	0.31%	0.039%
24	11.534	1447	1453	1461	rBV5	3000	6383	0.17%	0.022%
25	11.646	1467	1472	1477	rBV2	7712	11096	0.30%	0.038%
26	11.981	1523	1529	1537	rVB3	6818	13794	0.38%	0.047%
27	12.593	1627	1633	1641	rBV3	1621	4760	0.13%	0.016%
28	12.840	1671	1675	1682	rBV9	2380	4369	0.12%	0.015%
29	13.216	1732	1739	1747	rBV9	6682	16901	0.46%	0.058%
30	13.551	1794	1796	1806	rBV9	1898	3841	0.10%	0.013%
31	13.657	1806	1814	1830	rVV	1146789	1483084	40.35%	5.094%
32	13.757	1830	1831	1840	rVB8	1919	4050	0.11%	0.014%
33	13.945	1854	1863	1872	rBV	950905	1548802	42.14%	5.320%
34	14.251	1908	1915	1926	rBV	755403	1161614	31.60%	3.990%
35	14.528	1956	1962	1985	rBV2	37601	141300	3.84%	0.485%
36	14.692	1985	1990	1991	rBV5	3010	4038	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022789.D
 Acq On : 01 Nov 2024 04:33
 Operator : RC/JU
 Sample : P4630-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.063	2048	2053	2057	rBV	9797	14385	0.39%	0.049%
38	15.269	2080	2088	2098	rBV	1259047	2140362	58.23%	7.352%
39	15.340	2098	2100	2106	rVV7	5515	7515	0.20%	0.026%
40	15.404	2106	2111	2123	rVV	537120	736585	20.04%	2.530%
41	15.510	2126	2129	2134	rVB6	7048	10673	0.29%	0.037%
42	16.022	2209	2216	2220	rBV9	4327	9099	0.25%	0.031%
43	16.081	2221	2226	2230	rVB5	4787	7206	0.20%	0.025%
44	16.534	2299	2303	2306	rVB5	3969	5202	0.14%	0.018%
45	16.657	2319	2324	2326	rBV6	4738	6646	0.18%	0.023%
46	16.739	2335	2338	2343	rVB7	3019	3973	0.11%	0.014%
47	17.069	2387	2394	2402	rBV	1074267	1586375	43.16%	5.449%
48	17.163	2404	2410	2423	rVV	1871245	2620246	71.29%	9.000%
49	17.369	2441	2445	2450	rVB5	3814	5545	0.15%	0.019%
50	17.763	2509	2512	2517	rVB7	4779	7253	0.20%	0.025%
51	18.004	2547	2553	2561	rBV4	45835	78927	2.15%	0.271%
52	18.081	2562	2566	2568	rBV2	4666	6470	0.18%	0.022%
53	18.475	2631	2633	2635	rBV3	3379	4266	0.12%	0.015%
54	18.528	2638	2642	2645	rBV6	4862	8484	0.23%	0.029%
55	19.086	2733	2737	2743	rVB3	22329	36150	0.98%	0.124%
56	19.175	2747	2752	2754	rBV2	24767	38916	1.06%	0.134%
57	19.210	2754	2758	2766	rVB2	70870	100237	2.73%	0.344%
58	19.339	2775	2780	2788	rBV3	57082	98888	2.69%	0.340%
59	19.551	2809	2816	2825	rBV	2349112	3260318	88.71%	11.198%
60	21.504	3142	3148	3156	rBV	1449818	2031861	55.28%	6.979%
61	24.533	3653	3663	3675	rVB	1355532	3675445	100.00%	12.624%
62	24.757	3692	3701	3713	rVB	873453	2170941	59.07%	7.457%




Sum of corrected areas: 29114568

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022789.D
Acq On : 01 Nov 2024 04:33
Operator : RC/JU
Sample : P4630-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

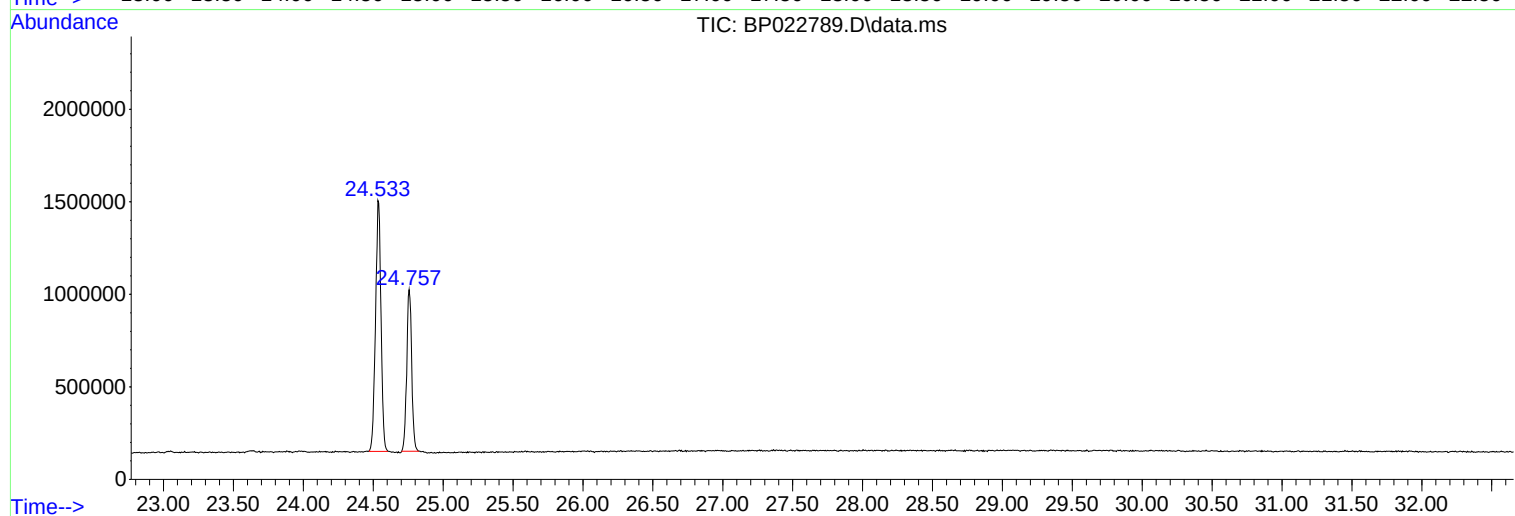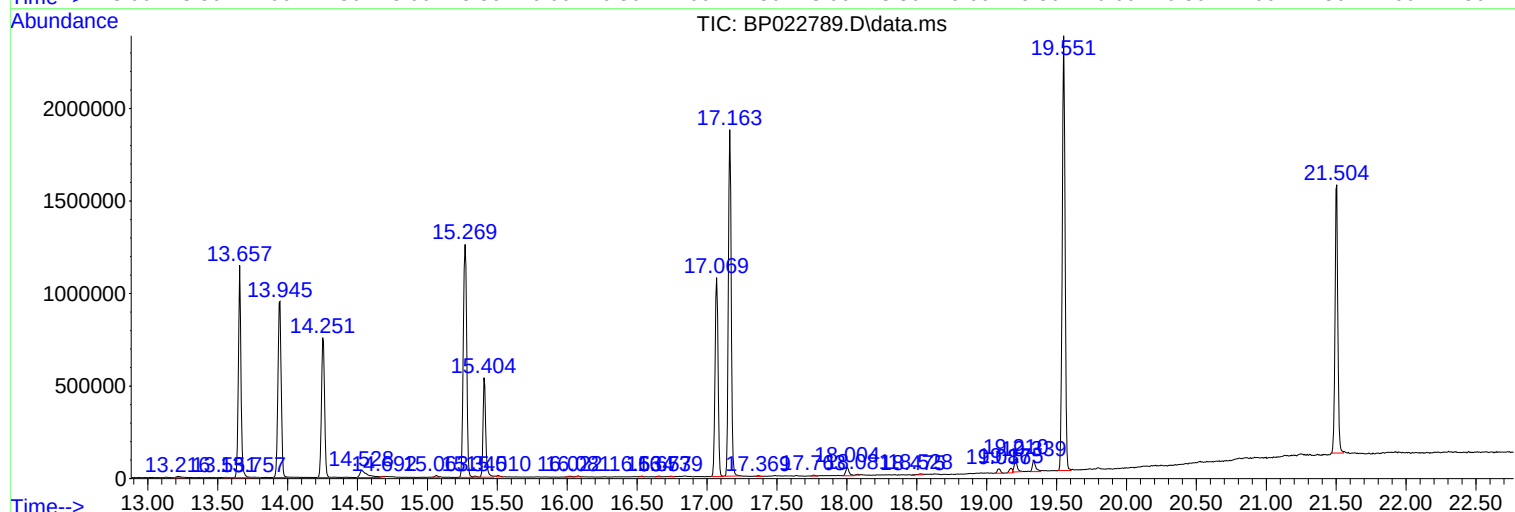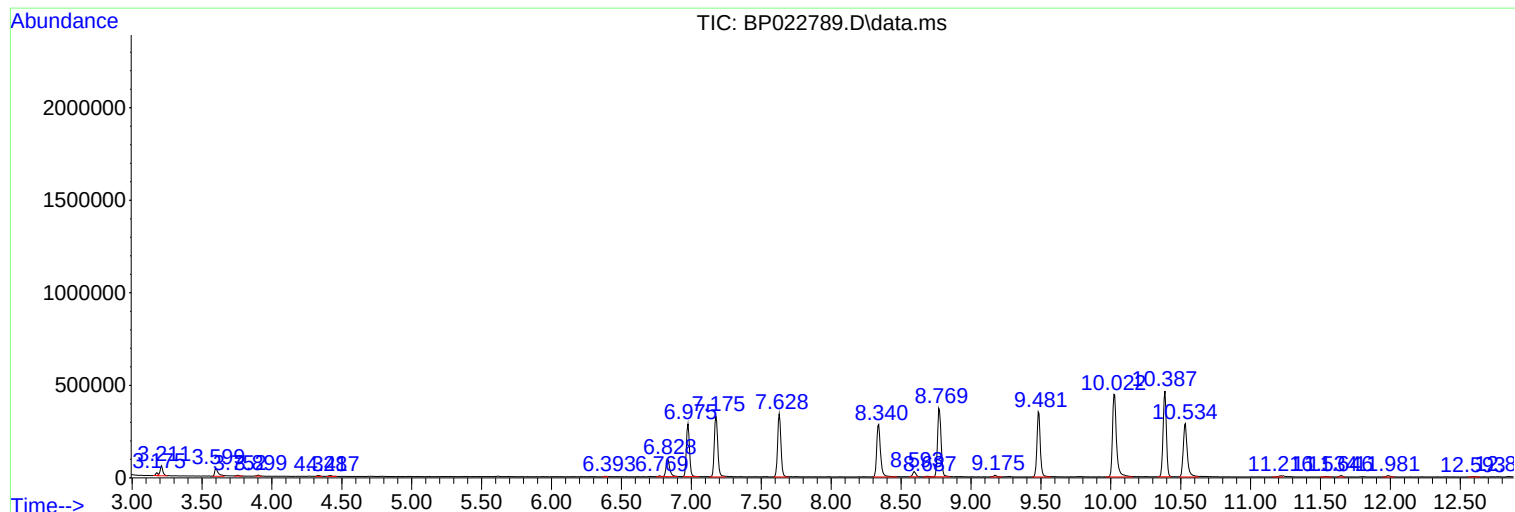

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022789.D
Acq On : 01 Nov 2024 04:33
Operator : RC/JU
Sample : P4630-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022789.D
Acq On : 01 Nov 2024 04:33
Operator : RC/JU
Sample : P4630-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc