

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022791.D
 Acq On : 01 Nov 2024 05:54
 Operator : RC/JU
 Sample : PB164516BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK516

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	43	rVB2	14660	23569	0.69%	0.091%
2	3.599	100	104	120	rBV	75691	130929	3.84%	0.508%
3	3.905	152	156	159	rBV2	4585	5803	0.17%	0.023%
4	6.775	639	644	648	rVB	5095	7386	0.22%	0.029%
5	6.828	648	653	666	rBV	77846	149555	4.39%	0.580%
6	6.975	672	678	689	rBV	260120	399386	11.72%	1.549%
7	7.175	703	712	729	rBV	298674	505709	14.84%	1.961%
8	7.628	782	789	800	rBV	322329	526093	15.44%	2.040%
9	8.340	903	910	926	rBV	264725	454530	13.34%	1.763%
10	8.775	974	984	1002	rBV	358793	604530	17.74%	2.344%
11	9.175	1045	1052	1060	rBV3	10754	17700	0.52%	0.069%
12	9.352	1076	1082	1084	rBV5	2224	3459	0.10%	0.013%
13	9.487	1097	1105	1117	rBV	294809	533538	15.65%	2.069%
14	10.022	1189	1196	1214	rBV	416642	807859	23.70%	3.133%
15	10.387	1248	1258	1266	rBV	413866	699177	20.52%	2.711%
16	10.534	1275	1283	1302	rBV	280395	562539	16.51%	2.181%
17	11.216	1393	1399	1411	rBV	3552	11240	0.33%	0.044%
18	11.657	1469	1474	1478	rVB2	6845	9989	0.29%	0.039%
19	11.987	1524	1530	1539	rBV3	7442	13683	0.40%	0.053%
20	13.140	1719	1726	1732	rBV	57270	85320	2.50%	0.331%
21	13.663	1807	1815	1830	rBV	768245	1238778	36.35%	4.804%
22	13.934	1851	1861	1875	rBV2	812328	1359914	39.90%	5.273%
23	14.246	1907	1914	1928	rVB	622498	1005415	29.50%	3.899%
24	14.522	1953	1961	1971	rBV	40288	99538	2.92%	0.386%
25	15.075	2050	2055	2059	rBV2	4219	6203	0.18%	0.024%
26	15.263	2080	2087	2095	rBV	1342525	1815003	53.26%	7.038%
27	15.416	2106	2113	2127	rBV	361988	576257	16.91%	2.235%
28	15.522	2127	2131	2135	rVB5	6828	10796	0.32%	0.042%
29	15.640	2145	2151	2159	rVB	66514	95246	2.79%	0.369%
30	15.798	2172	2178	2179	rBV5	2669	4250	0.12%	0.016%
31	16.004	2210	2213	2217	rBV5	2391	3435	0.10%	0.013%
32	16.475	2288	2293	2294	rBV4	2347	3632	0.11%	0.014%
33	16.534	2298	2303	2309	rVB10	4787	8665	0.25%	0.034%
34	16.640	2315	2321	2329	rVV4	25487	51396	1.51%	0.199%
35	16.728	2333	2336	2342	rVB7	2274	4022	0.12%	0.016%
36	16.828	2350	2353	2356	rBV5	5469	7568	0.22%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022791.D
 Acq On : 01 Nov 2024 05:54
 Operator : RC/JU
 Sample : PB164516BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK516

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	17.057	2386	2392	2400	rBV	933678	1347217	39.53%	5.224%
38	17.169	2403	2411	2422	rBV	1380336	2226361	65.33%	8.633%
39	17.357	2440	2443	2448	rVB4	6815	9045	0.27%	0.035%
40	17.563	2473	2478	2488	rBV	14863	26562	0.78%	0.103%
41	17.645	2488	2492	2499	rVV10	4042	6290	0.18%	0.024%
42	17.751	2508	2510	2513	rBV4	3028	3420	0.10%	0.013%
43	17.945	2539	2543	2546	rBV6	2439	4052	0.12%	0.016%
44	17.987	2546	2550	2555	rBV3	48220	82222	2.41%	0.319%
45	18.557	2643	2647	2652	rBV4	11445	15074	0.44%	0.058%
46	19.086	2733	2737	2743	rVB2	21631	31121	0.91%	0.121%
47	19.169	2747	2751	2754	rVV	18120	25163	0.74%	0.098%
48	19.210	2755	2758	2766	rVB	42157	56400	1.65%	0.219%
49	19.328	2774	2778	2786	rBV6	31040	51511	1.51%	0.200%
50	19.551	2809	2816	2828	rBV	1856912	2884598	84.64%	11.185%
51	21.498	3142	3147	3157	rVB	1242298	1781747	52.28%	6.909%
52	24.533	3653	3663	3677	rVB	1262684	3408104	100.00%	13.215%
53	24.769	3694	3703	3715	rVB	715224	1987843	58.33%	7.708%


Sum of corrected areas: 25788842

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022791.D
Acq On : 01 Nov 2024 05:54
Operator : RC/JU
Sample : PB164516BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

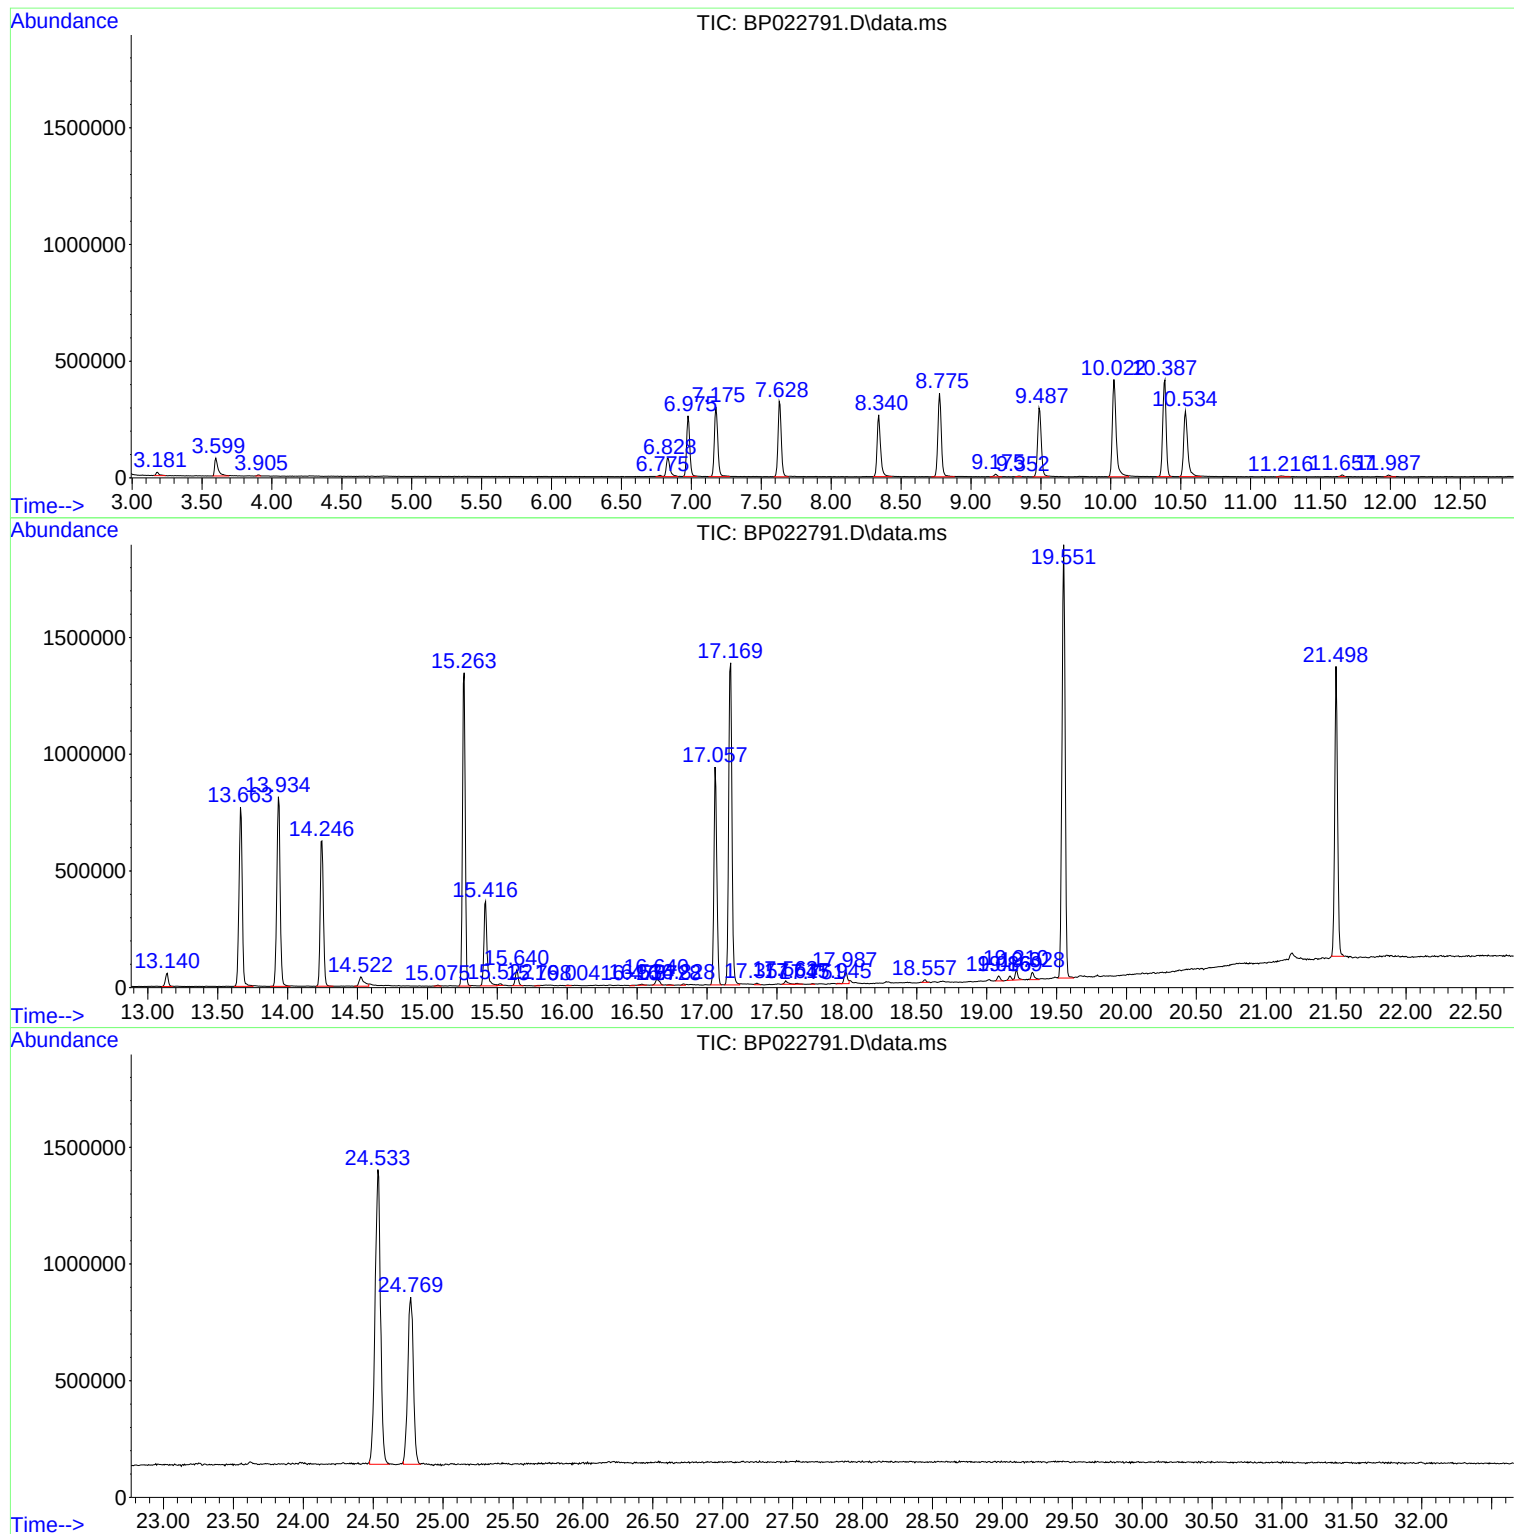

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022791.D
Acq On : 01 Nov 2024 05:54
Operator : RC/JU
Sample : PB164516BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022791.D
Acq On : 01 Nov 2024 05:54
Operator : RC/JU
Sample : PB164516BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc