

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022792.D
 Acq On : 01 Nov 2024 06:35
 Operator : RC/JU
 Sample : PB164546BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK546

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rBV	13446	18590	0.58%	0.077%
2	3.599	100	104	120	rBV	80129	140659	4.38%	0.584%
3	3.905	152	156	162	rVB3	4825	6858	0.21%	0.028%
4	4.805	302	309	311	rBV7	2405	3801	0.12%	0.016%
5	6.775	640	644	648	rBV3	3562	5219	0.16%	0.022%
6	6.834	648	654	670	rVV	87857	164505	5.12%	0.683%
7	6.975	672	678	691	rVB	230831	359631	11.19%	1.493%
8	7.175	705	712	724	rBV	284255	461846	14.37%	1.917%
9	7.634	781	790	798	rBV	304170	501594	15.61%	2.082%
10	8.340	901	910	929	rBV	256005	459474	14.30%	1.907%
11	8.775	976	984	993	rBV	311457	510818	15.90%	2.120%
12	9.175	1047	1052	1058	rBV3	9170	13398	0.42%	0.056%
13	9.487	1098	1105	1119	rBV	254917	450191	14.01%	1.869%
14	10.028	1187	1197	1215	rBV	350005	704180	21.91%	2.923%
15	10.387	1250	1258	1272	rVB	425398	648948	20.19%	2.694%
16	10.534	1274	1283	1304	rBV	262463	526370	16.38%	2.185%
17	11.222	1394	1400	1404	rBV8	2273	5538	0.17%	0.023%
18	11.651	1470	1473	1480	rVB6	4113	6410	0.20%	0.027%
19	11.998	1526	1532	1540	rVV5	4724	10219	0.32%	0.042%
20	13.145	1720	1727	1735	rBV	41287	75392	2.35%	0.313%
21	13.663	1806	1815	1826	rBV	669478	1081388	33.65%	4.489%
22	13.945	1856	1863	1873	rBV	782472	1175794	36.59%	4.881%
23	14.251	1907	1915	1925	rBV	755717	964703	30.02%	4.004%
24	14.534	1956	1963	1974	rBV4	37753	112889	3.51%	0.469%
25	15.075	2051	2055	2060	rVB	5089	6693	0.21%	0.028%
26	15.269	2081	2088	2097	rBV	1187327	1632433	50.80%	6.776%
27	15.422	2107	2114	2126	rBV	325029	510502	15.89%	2.119%
28	15.522	2127	2131	2138	rVB3	5567	10505	0.33%	0.044%
29	15.639	2146	2151	2159	rVB2	21088	33942	1.06%	0.141%
30	15.804	2170	2179	2180	rBV8	3047	5304	0.17%	0.022%
31	16.004	2209	2213	2217	rBV6	3113	4865	0.15%	0.020%
32	16.539	2300	2304	2307	rBV6	3635	5027	0.16%	0.021%
33	16.651	2317	2323	2330	rBV3	26291	50590	1.57%	0.210%
34	16.733	2335	2337	2341	rVB5	3636	3675	0.11%	0.015%
35	16.833	2348	2354	2355	rBV6	5238	7840	0.24%	0.033%
36	17.063	2386	2393	2403	rVV	991302	1321046	41.11%	5.483%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022792.D
Acq On : 01 Nov 2024 06:35
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.163	2403	2410	2423	rBV	1331664	1970983	61.33%	8.181%
38	17.357	2441	2443	2450	rVB5	6178	9005	0.28%	0.037%
39	17.569	2474	2479	2485	rBV2	11031	20769	0.65%	0.086%
40	17.645	2490	2492	2494	rBV2	3151	3827	0.12%	0.016%
41	17.998	2548	2552	2557	rBV	53992	82157	2.56%	0.341%
42	18.292	2597	2602	2606	rBV2	10357	15433	0.48%	0.064%
43	18.551	2643	2646	2653	rBV5	8746	15645	0.49%	0.065%
44	19.098	2734	2739	2745	rBV3	19470	33542	1.04%	0.139%
45	19.169	2748	2751	2755	rVV	25310	33972	1.06%	0.141%
46	19.210	2755	2758	2768	rVB3	46058	77933	2.43%	0.323%
47	19.333	2775	2779	2784	rBV2	50258	67526	2.10%	0.280%
48	19.545	2809	2815	2826	rBV	2038786	2680695	83.41%	11.127%
49	21.504	3142	3148	3163	rVB2	943828	1855335	57.73%	7.701%
50	24.539	3655	3664	3678	rVB	1296606	3213687	100.00%	13.339%
51	24.762	3693	3702	3716	rVB	660717	2010278	62.55%	8.344%


Sum of corrected areas: 24091624

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022792.D
Acq On : 01 Nov 2024 06:35
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

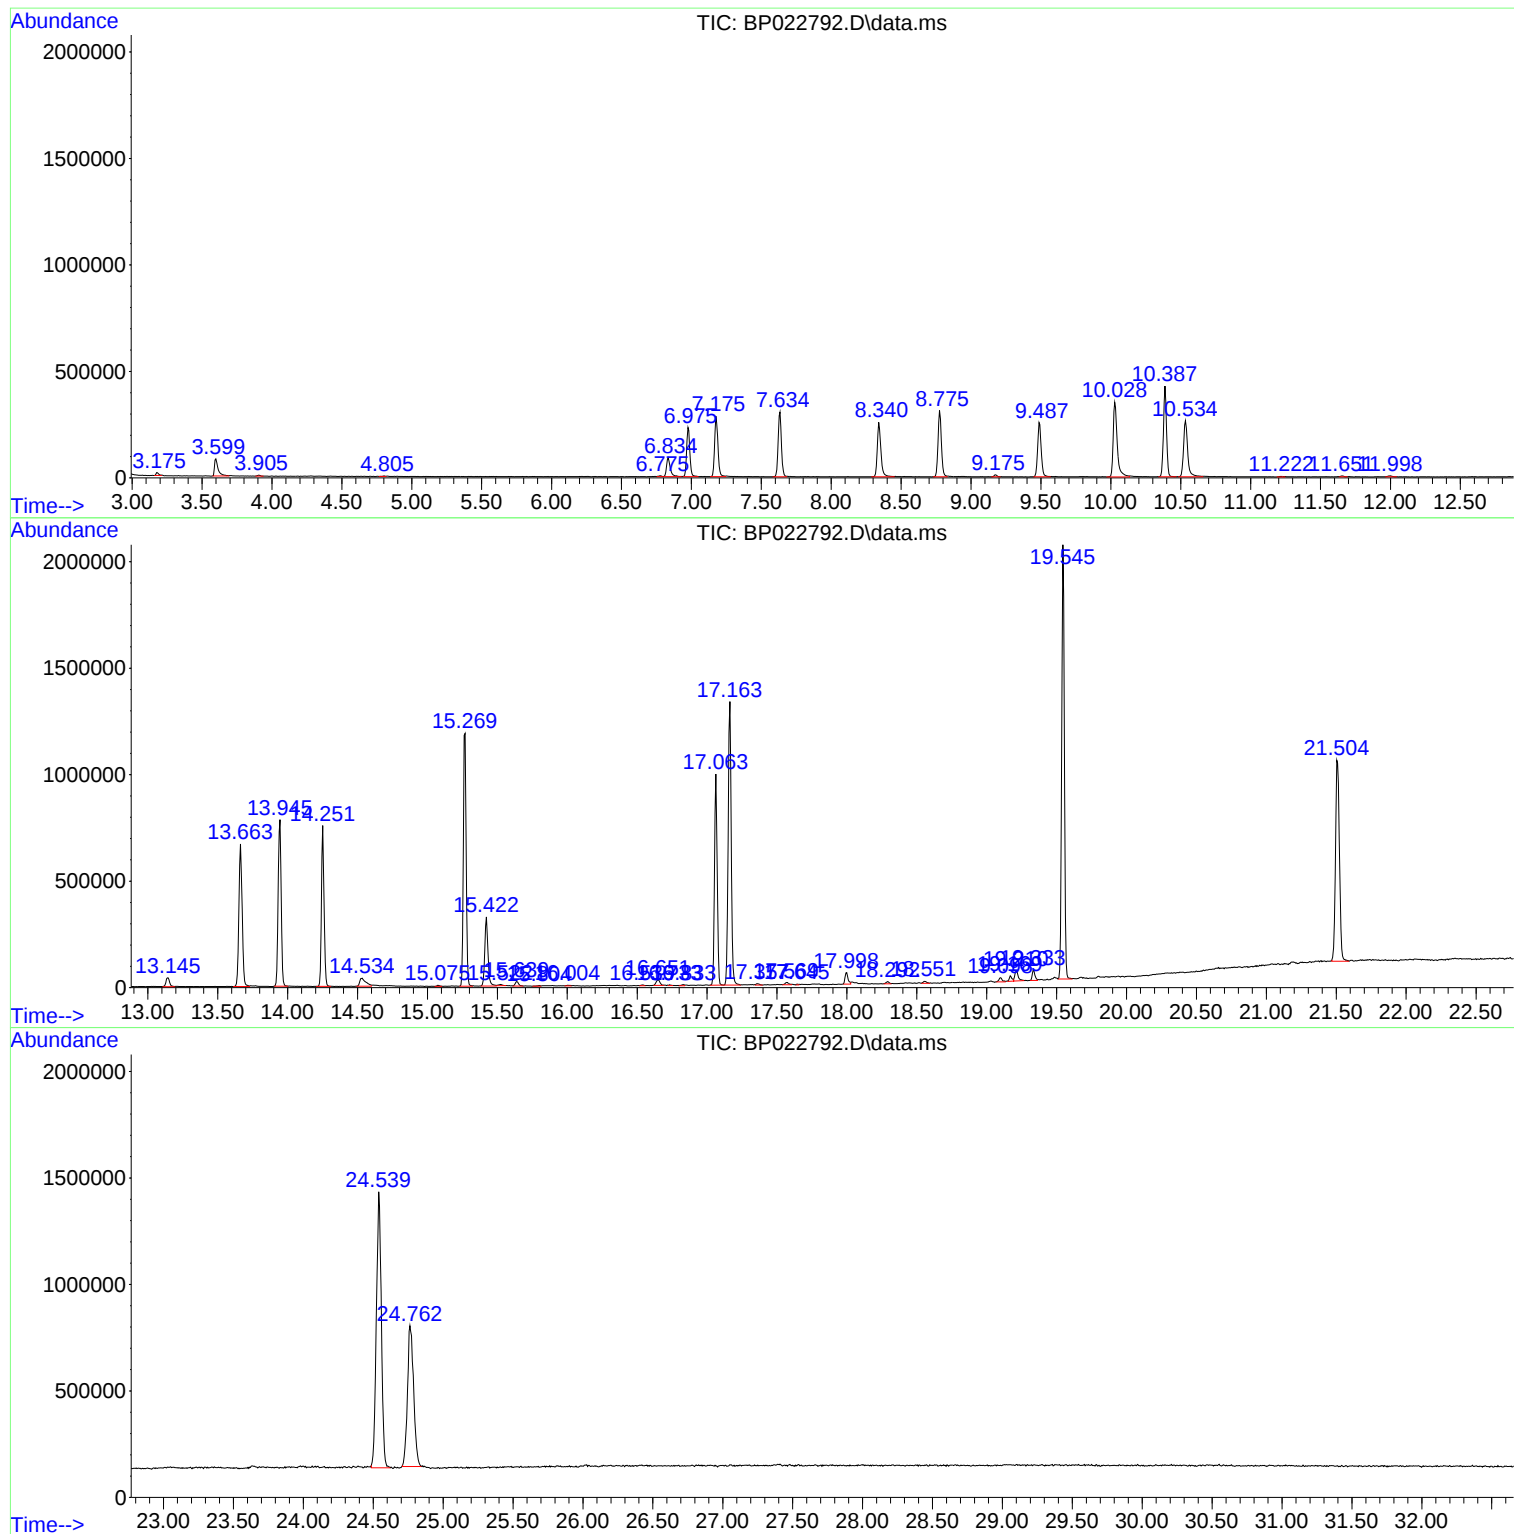

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022792.D
Acq On : 01 Nov 2024 06:35
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022792.D
Acq On : 01 Nov 2024 06:35
Operator : RC/JU
Sample : PB164546BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK546

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------