

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022793.D
 Acq On : 01 Nov 2024 07:15
 Operator : RC/JU
 Sample : P4630-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	29	rBV3	3123	4616	0.11%	0.014%
2	3.175	29	32	37	rVB	18991	23359	0.54%	0.072%
3	3.599	101	104	119	rBV	38418	71278	1.66%	0.219%
4	3.899	152	155	162	rVB	5442	7970	0.19%	0.024%
5	4.417	237	243	253	rBV	82115	122206	2.84%	0.375%
6	6.775	638	644	648	rBV2	6829	10968	0.25%	0.034%
7	6.834	648	654	666	rVV	150719	268299	6.23%	0.824%
8	6.975	672	678	691	rVB	299870	474974	11.03%	1.459%
9	7.175	705	712	729	rBV	400823	647090	15.03%	1.988%
10	7.628	782	789	798	rBV	401192	645001	14.98%	1.981%
11	8.334	902	909	926	rBV	378840	696726	16.18%	2.140%
12	8.775	977	984	997	rBV	442705	719334	16.71%	2.209%
13	8.905	1003	1006	1011	rBV6	3643	6605	0.15%	0.020%
14	9.175	1043	1052	1059	rBV	13094	21736	0.50%	0.067%
15	9.481	1097	1104	1120	rBV	370843	654764	15.21%	2.011%
16	10.022	1189	1196	1219	rBV	548663	998660	23.20%	3.067%
17	10.387	1251	1258	1266	rBV	561124	872506	20.27%	2.680%
18	10.528	1275	1282	1298	rBV	293470	560824	13.03%	1.723%
19	11.210	1391	1398	1403	rBV9	3658	8618	0.20%	0.026%
20	11.651	1467	1473	1477	rBV3	5896	9634	0.22%	0.030%
21	11.987	1523	1530	1541	rVB4	6588	15539	0.36%	0.048%
22	12.863	1672	1679	1686	rVB10	3029	7317	0.17%	0.022%
23	13.657	1805	1814	1828	rBV	937153	1492502	34.67%	4.584%
24	13.945	1853	1863	1876	rBV	1218399	1721064	39.98%	5.286%
25	14.263	1909	1917	1928	rBV	1011560	1345414	31.25%	4.132%
26	14.528	1956	1962	1982	rBV2	57999	176235	4.09%	0.541%
27	14.716	1991	1994	1999	rVB7	4660	7783	0.18%	0.024%
28	15.069	2050	2054	2061	rVB2	7434	11099	0.26%	0.034%
29	15.281	2082	2090	2099	rBV	1553927	2295677	53.32%	7.051%
30	15.410	2105	2112	2124	rBV	431038	751975	17.47%	2.310%
31	15.510	2126	2129	2136	rVB4	6850	13692	0.32%	0.042%
32	17.075	2387	2395	2404	rBV	1161956	1775178	41.23%	5.452%
33	17.163	2404	2410	2425	rVB	2298627	2922621	67.89%	8.977%
34	17.375	2440	2446	2448	rBV2	4378	5984	0.14%	0.018%
35	17.763	2509	2512	2516	rVB6	4129	4987	0.12%	0.015%
36	17.998	2547	2552	2561	rBV3	42465	58173	1.35%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022793.D
 Acq On : 01 Nov 2024 07:15
 Operator : RC/JU
 Sample : P4630-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	18.075	2562	2565	2570	rVV2	5541	8089	0.19%	0.025%
38	18.522	2637	2641	2647	rBV9	5130	12523	0.29%	0.038%
39	19.086	2732	2737	2742	rBV2	25017	42825	0.99%	0.132%
40	19.175	2748	2752	2754	rBV	27132	38767	0.90%	0.119%
41	19.204	2754	2757	2766	rVB3	65079	105560	2.45%	0.324%
42	19.339	2775	2780	2786	rBV	56008	79486	1.85%	0.244%
43	19.551	2809	2816	2825	rBV	2363064	3719938	86.41%	11.426%
44	19.798	2855	2858	2862	rVB	14890	18537	0.43%	0.057%
45	21.504	3141	3148	3159	rBV	1424688	2291240	53.22%	7.038%
46	24.533	3654	3663	3679	rVB	1575947	4305097	100.00%	13.223%
47	24.757	3693	3701	3714	rVB	1105402	2504815	58.18%	7.694%


Sum of corrected areas: 32557285

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022793.D
Acq On : 01 Nov 2024 07:15
Operator : RC/JU
Sample : P4630-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

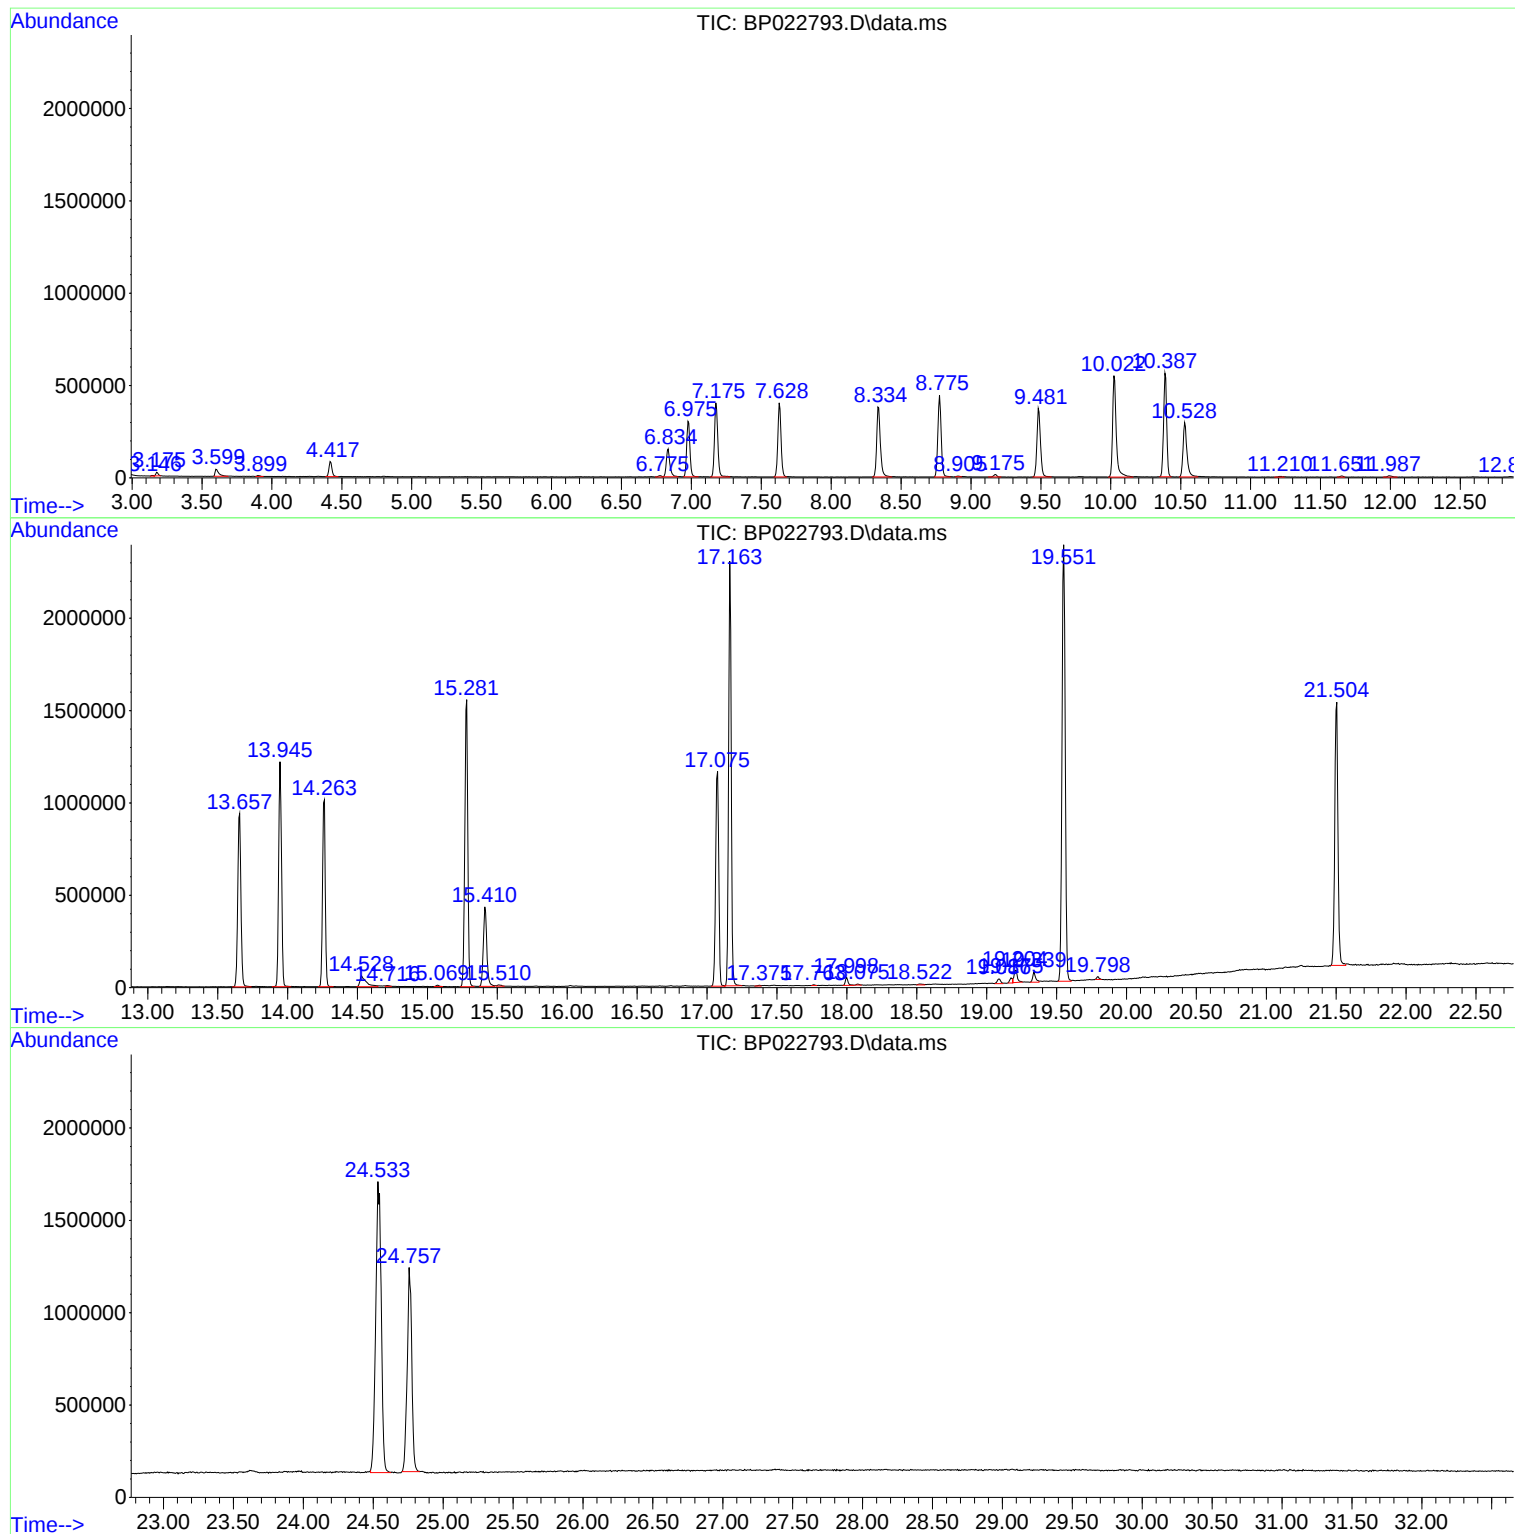

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022793.D
Acq On : 01 Nov 2024 07:15
Operator : RC/JU
Sample : P4630-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP07










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.417	3.79 ng/ul	122206	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	87
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

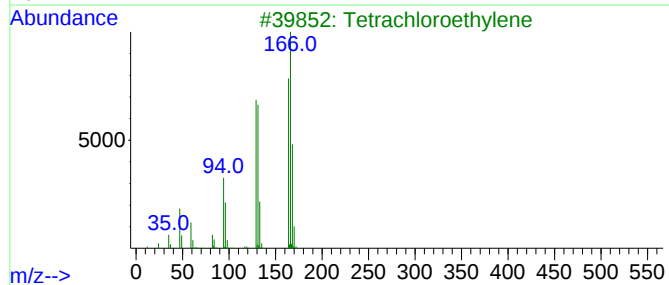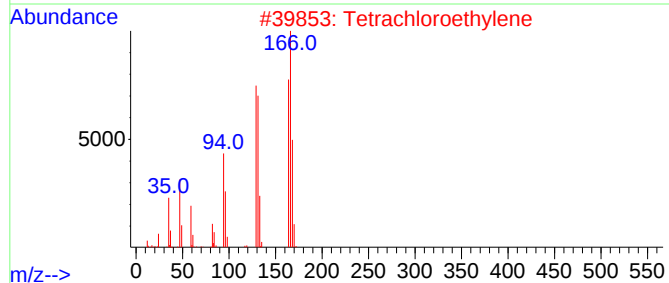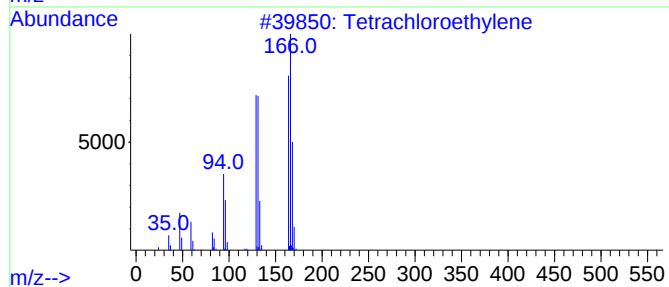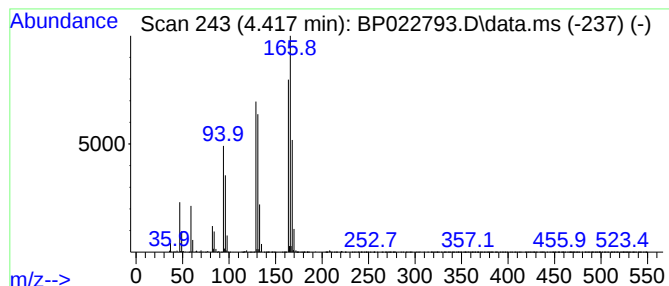

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022793.D
Acq On : 01 Nov 2024 07:15
Operator : RC/JU
Sample : P4630-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.417	3.8	ng/u1	122206	1	7.628	645001	20.0