

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022796.D
 Acq On : 01 Nov 2024 09:18
 Operator : RC/JU
 Sample : P4630-14
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP08

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	29	rBV3	3781	3744	0.10%	0.013%
2	3.181	29	33	44	rVB	19106	29771	0.80%	0.102%
3	3.599	100	104	119	rBV	59019	110363	2.98%	0.380%
4	3.905	151	156	162	rVB	6055	9362	0.25%	0.032%
5	4.417	238	243	252	rVB	53028	79708	2.15%	0.274%
6	6.775	639	644	648	rBV3	3913	6251	0.17%	0.022%
7	6.834	648	654	669	rVV	82378	155914	4.21%	0.537%
8	6.975	671	678	694	rVB	277707	446215	12.06%	1.536%
9	7.175	705	712	723	rBV	335013	560541	15.14%	1.929%
10	7.634	780	790	802	rBV	364273	590529	15.95%	2.032%
11	8.340	902	910	926	rBV	266884	480755	12.99%	1.655%
12	8.775	976	984	997	rBV	376091	647463	17.49%	2.228%
13	9.175	1046	1052	1058	rVB2	12492	21207	0.57%	0.073%
14	9.487	1097	1105	1122	rBV	330250	570390	15.41%	1.963%
15	10.028	1189	1197	1219	rBV	461949	887422	23.97%	3.054%
16	10.387	1251	1258	1266	rBV	476234	778733	21.04%	2.680%
17	10.534	1274	1283	1305	rBV	295736	636271	17.19%	2.190%
18	11.652	1469	1473	1479	rVB4	5564	10056	0.27%	0.035%
19	11.993	1527	1531	1538	rBV3	6054	12318	0.33%	0.042%
20	12.846	1671	1676	1681	rBV7	2053	4516	0.12%	0.016%
21	13.657	1804	1814	1827	rBV	1043226	1470329	39.72%	5.060%
22	13.940	1855	1862	1875	rBV2	1101434	1593722	43.06%	5.485%
23	14.251	1908	1915	1927	rBV	862704	1181250	31.91%	4.065%
24	14.540	1956	1964	1984	rBV3	43837	156283	4.22%	0.538%
25	15.063	2048	2053	2058	rBV	8937	12170	0.33%	0.042%
26	15.263	2080	2087	2101	rBV	1576226	2194490	59.29%	7.553%
27	15.404	2104	2111	2126	rBV	370363	636416	17.19%	2.190%
28	15.510	2126	2129	2136	rVB6	8135	14933	0.40%	0.051%
29	16.722	2333	2335	2341	rVB7	3062	4567	0.12%	0.016%
30	16.839	2350	2355	2357	rBV5	2351	3820	0.10%	0.013%
31	17.057	2386	2392	2401	rBV	1279831	1620743	43.79%	5.578%
32	17.151	2401	2408	2425	rVV	1699514	2694087	72.78%	9.272%
33	17.357	2441	2443	2448	rVB5	3446	4663	0.13%	0.016%
34	17.751	2507	2510	2515	rVB7	3876	4985	0.13%	0.017%
35	17.998	2547	2552	2557	rBV2	32600	48258	1.30%	0.166%
36	18.069	2561	2564	2567	rVB2	6448	7759	0.21%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022796.D
Acq On : 01 Nov 2024 09:18
Operator : RC/JU
Sample : P4630-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP08

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	19.098	2734	2739	2745	rBV2	27214	43932	1.19%	0.151%
38	19.169	2747	2751	2754	rBV	27457	36955	1.00%	0.127%
39	19.210	2754	2758	2764	rVV3	42728	62244	1.68%	0.214%
40	19.339	2776	2780	2785	rBV3	39726	49007	1.32%	0.169%
41	19.539	2809	2814	2825	rBV	2578183	3399253	91.84%	11.699%
42	21.510	3143	3149	3160	rVB	1049110	1991875	53.81%	6.855%
43	24.551	3656	3666	3682	rVB	1448220	3701453	100.00%	12.739%
44	24.780	3695	3705	3720	rVB	705343	2081704	56.24%	7.164%




Sum of corrected areas: 29056427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022796.D
Acq On : 01 Nov 2024 09:18
Operator : RC/JU
Sample : P4630-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

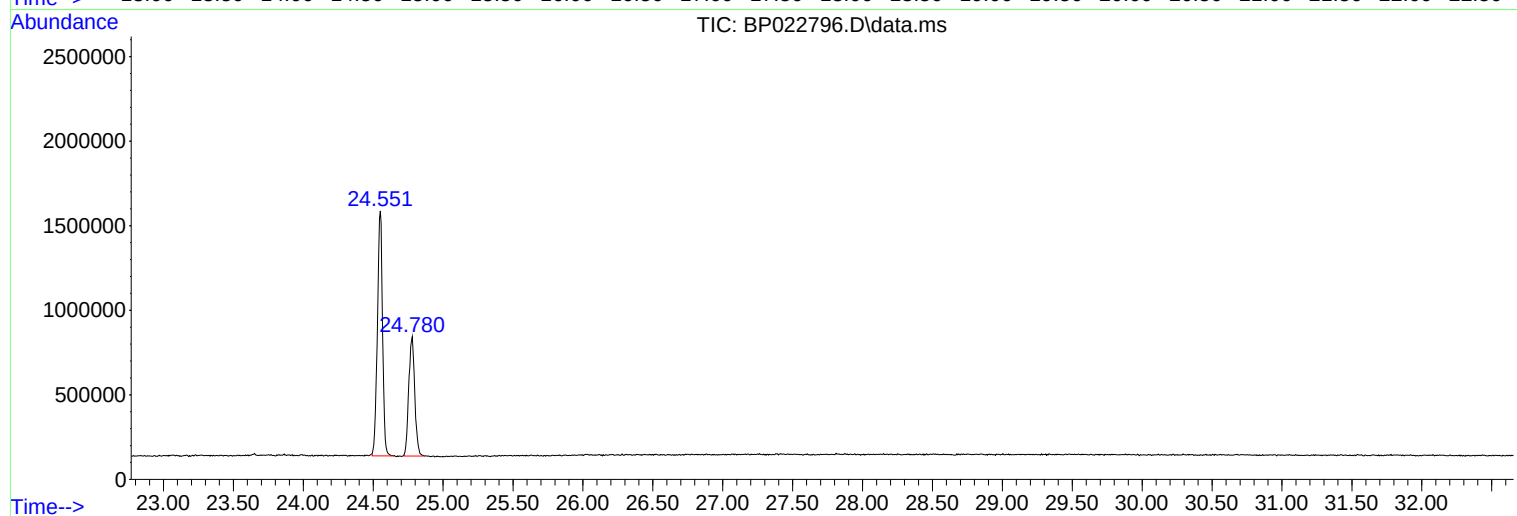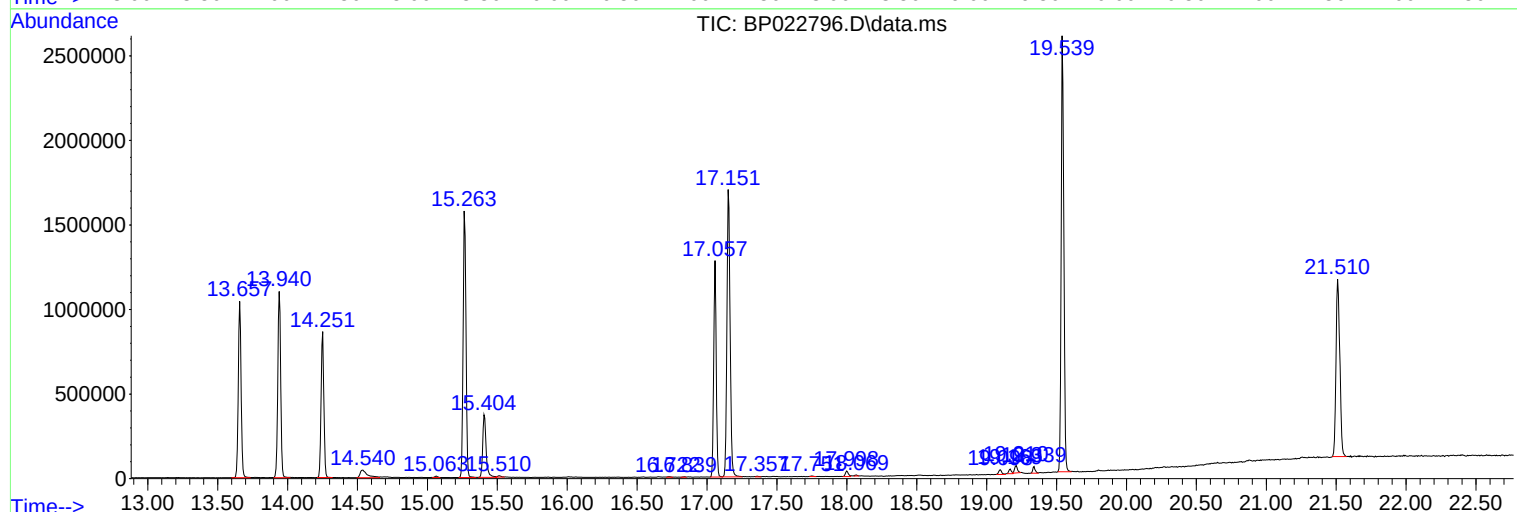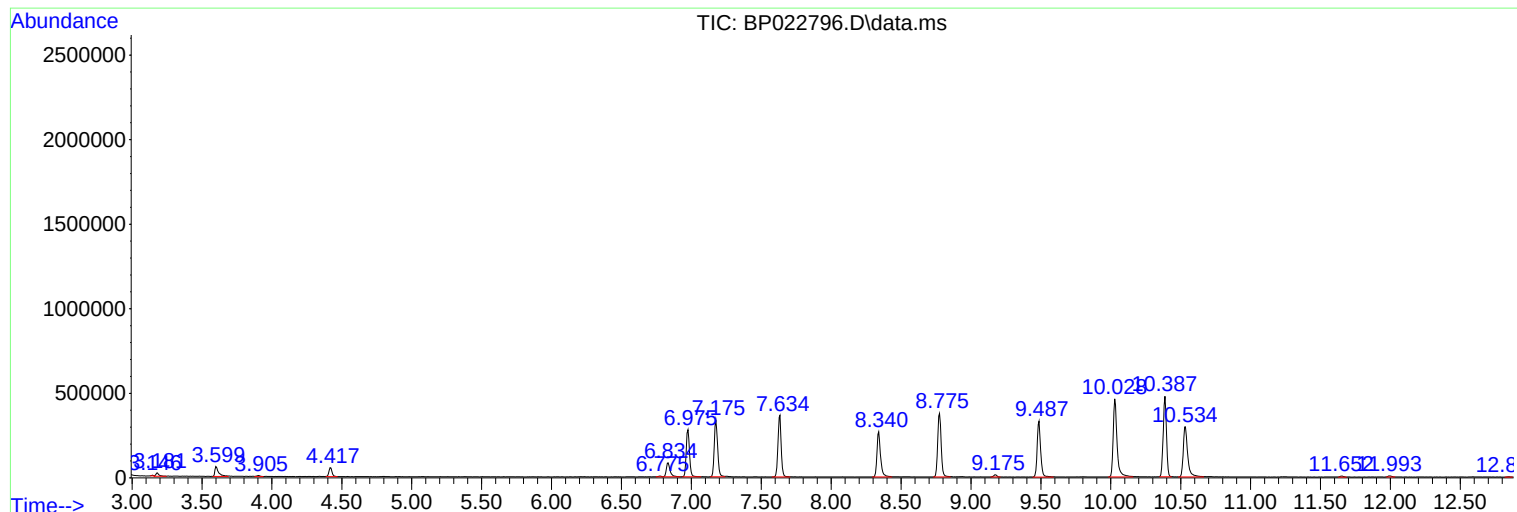

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022796.D
Acq On : 01 Nov 2024 09:18
Operator : RC/JU
Sample : P4630-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP08










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.417	2.70 ng/ul	79708	1,4-Dichlorobenzene-d4	7.634

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	90
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	27

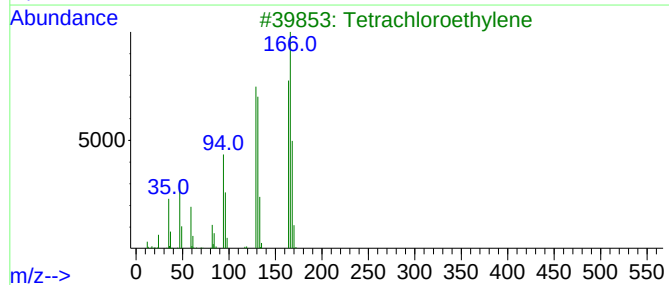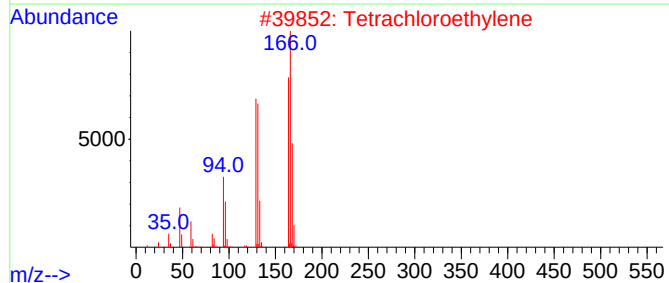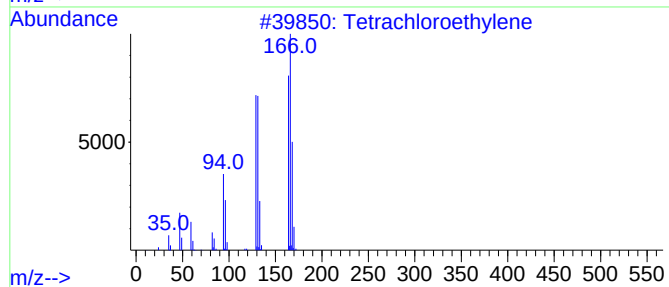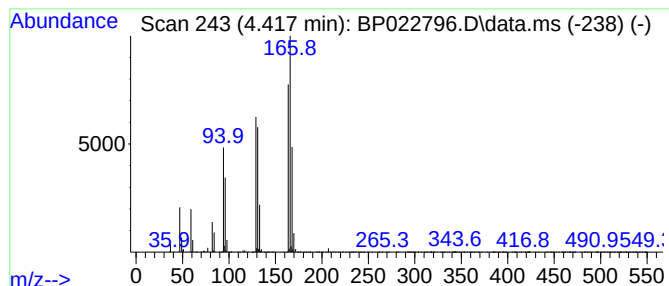

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022796.D
Acq On : 01 Nov 2024 09:18
Operator : RC/JU
Sample : P4630-14
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.417	2.7	ng/ul	79708	1	7.634	590529	20.0