

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022808.D
 Acq On : 01 Nov 2024 17:28
 Operator : RC/JU
 Sample : P4583-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0P11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	29	32	41	rVB	18505	24696	0.74%	0.085%
2	3.517	87	90	94	rVB3	3536	4832	0.15%	0.017%
3	3.899	152	155	159	rBV	5236	6848	0.21%	0.024%
4	4.264	215	217	223	rVB6	2721	3979	0.12%	0.014%
5	4.328	225	228	234	rVB4	3123	4196	0.13%	0.014%
6	5.193	370	375	378	rBV6	3778	6585	0.20%	0.023%
7	5.722	461	465	471	rVB7	2977	4634	0.14%	0.016%
8	6.311	559	565	568	rBV7	2275	4665	0.14%	0.016%
9	6.693	625	630	637	rBV3	9012	18331	0.55%	0.063%
10	6.769	639	643	647	rVV	9050	13632	0.41%	0.047%
11	6.828	647	653	668	rVB	150578	263190	7.91%	0.905%
12	6.975	671	678	686	rBV	291197	462289	13.89%	1.590%
13	7.175	703	712	722	rBV	396179	656334	19.72%	2.257%
14	7.240	722	723	732	rVB8	3447	7123	0.21%	0.024%
15	7.628	781	789	796	rBV	369896	585566	17.59%	2.013%
16	7.693	796	800	808	rVV2	22198	44925	1.35%	0.154%
17	7.752	808	810	815	rVB6	2729	3977	0.12%	0.014%
18	7.928	836	840	845	rVB8	3219	5745	0.17%	0.020%
19	8.234	887	892	897	rBV7	5014	11254	0.34%	0.039%
20	8.334	903	909	924	rBV	375131	670558	20.14%	2.306%
21	8.446	924	928	935	rVB3	10326	17872	0.54%	0.061%
22	8.705	967	972	977	rBV	52942	88984	2.67%	0.306%
23	8.769	977	983	992	rVV	434962	687514	20.65%	2.364%
24	8.852	995	997	1001	rVB5	2845	3578	0.11%	0.012%
25	8.916	1004	1008	1009	rBV4	3250	4040	0.12%	0.014%
26	9.169	1043	1051	1058	rBV2	18148	29171	0.88%	0.100%
27	9.340	1072	1080	1083	rBV4	3285	5855	0.18%	0.020%
28	9.481	1094	1104	1120	rBV	358855	636789	19.13%	2.190%
29	9.722	1139	1145	1146	rBV6	3789	6131	0.18%	0.021%
30	9.746	1146	1149	1159	rVB9	6490	15018	0.45%	0.052%
31	10.022	1189	1196	1214	rBV	484119	974544	29.28%	3.351%
32	10.157	1217	1219	1228	rVB10	2180	5096	0.15%	0.018%
33	10.246	1228	1234	1240	rBV9	2599	4643	0.14%	0.016%
34	10.305	1240	1244	1250	rBV5	6600	15230	0.46%	0.052%
35	10.381	1250	1257	1264	rVV	479353	796377	23.92%	2.738%
36	10.446	1264	1268	1272	rVB5	7303	11708	0.35%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022808.D
 Acq On : 01 Nov 2024 17:28
 Operator : RC/JU
 Sample : P4583-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0P11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	10.563	1282	1288	1290	rBV4	5224	8584	0.26%	0.030%
38	10.693	1305	1310	1318	rVB10	2712	5980	0.18%	0.021%
39	11.052	1364	1371	1380	rBV2	7522	17386	0.52%	0.060%
40	11.210	1392	1398	1407	rBV9	7529	18191	0.55%	0.063%
41	11.575	1453	1460	1465	rBV8	3730	7140	0.21%	0.025%
42	11.646	1466	1472	1478	rVB	28438	41907	1.26%	0.144%
43	11.981	1520	1529	1536	rBV	9475	17186	0.52%	0.059%
44	12.840	1667	1675	1679	rBV7	3785	6488	0.19%	0.022%
45	13.187	1728	1734	1744	rBV3	25221	60389	1.81%	0.208%
46	13.669	1808	1816	1829	rBV	1162461	1530314	45.97%	5.262%
47	13.781	1831	1835	1842	rVB10	2529	4548	0.14%	0.016%
48	13.940	1855	1862	1874	rBV	964752	1539048	46.23%	5.292%
49	14.146	1894	1897	1905	rVB4	3219	6233	0.19%	0.021%
50	14.251	1908	1915	1927	rVV	760129	1236046	37.13%	4.250%
51	14.346	1927	1931	1935	rVB5	3299	4476	0.13%	0.015%
52	14.516	1952	1960	1978	rBV	86681	260209	7.82%	0.895%
53	15.081	2050	2056	2062	rBV6	4983	12430	0.37%	0.043%
54	15.263	2080	2087	2097	rBV	1497180	2240676	67.31%	7.704%
55	15.416	2107	2113	2125	rBV	490786	672374	20.20%	2.312%
56	15.510	2125	2129	2135	rVV5	14842	25633	0.77%	0.088%
57	15.593	2138	2143	2149	rVV	24817	34568	1.04%	0.119%
58	15.645	2149	2152	2157	rVB6	2529	3652	0.11%	0.013%
59	15.857	2183	2188	2191	rBV6	2230	3625	0.11%	0.012%
60	16.540	2300	2304	2308	rVB7	3280	4980	0.15%	0.017%
61	16.645	2319	2322	2328	rVB6	3256	5837	0.18%	0.020%
62	16.745	2332	2339	2344	rVB10	2906	6698	0.20%	0.023%
63	16.845	2352	2356	2362	rVB4	2678	5183	0.16%	0.018%
64	17.063	2382	2393	2404	rBV	1018452	1631121	49.00%	5.608%
65	17.169	2404	2411	2426	rBV2	1765484	2591817	77.86%	8.912%
66	17.363	2442	2444	2449	rVB5	3911	5443	0.16%	0.019%
67	17.639	2489	2491	2495	rBV5	2464	3673	0.11%	0.013%
68	17.763	2505	2512	2518	rBV	176993	259867	7.81%	0.894%
69	17.928	2538	2540	2546	rBV6	2576	3514	0.11%	0.012%
70	18.004	2547	2553	2560	rBV4	25145	51243	1.54%	0.176%
71	18.063	2561	2563	2570	rVB2	5469	8725	0.26%	0.030%
72	18.222	2587	2590	2593	rBV4	10010	13391	0.40%	0.046%
73	18.263	2593	2597	2599	rVB5	4188	6269	0.19%	0.022%
74	18.357	2609	2613	2615	rBV5	3254	4632	0.14%	0.016%
75	19.092	2733	2738	2743	rBV	25857	36672	1.10%	0.126%
76	19.163	2746	2750	2757	rVV	19474	34280	1.03%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022808.D
Acq On : 01 Nov 2024 17:28
Operator : RC/JU
Sample : P4583-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0P11

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

77	19.333	2775	2779	2786	rBV5	24775	42623	1.28%	0.147%
78	19.545	2809	2815	2825	rVB	2339369	3248682	97.59%	11.170%
79	21.510	3143	3149	3160	rVB	1277268	1959910	58.88%	6.739%
80	24.539	3654	3664	3679	rVB	1241130	3328877	100.00%	11.446%
81	24.774	3695	3704	3719	rVB	734941	1966824	59.08%	6.763%

Sum of corrected areas: 29083253




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022808.D
Acq On : 01 Nov 2024 17:28
Operator : RC/JU
Sample : P4583-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0P1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

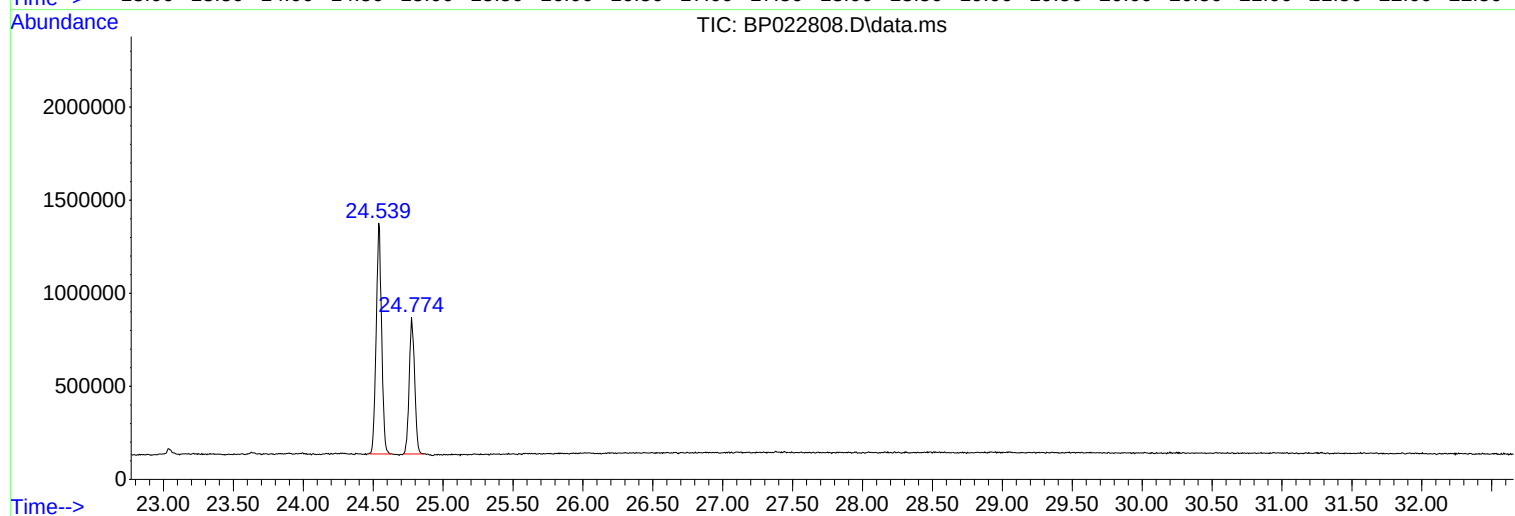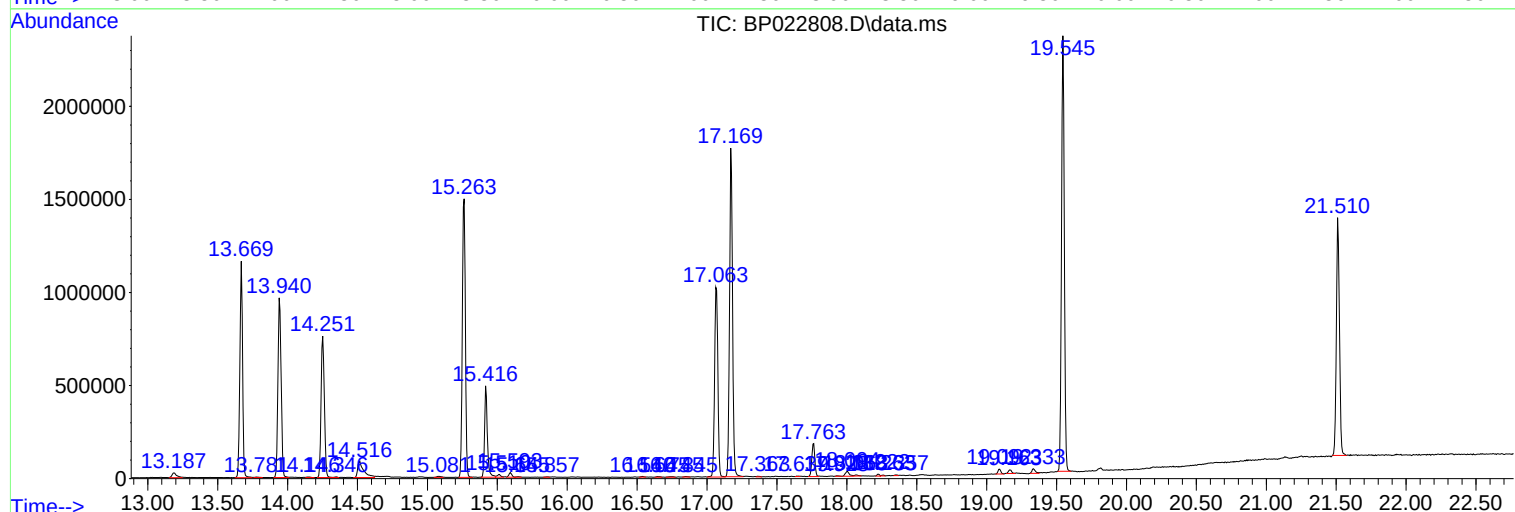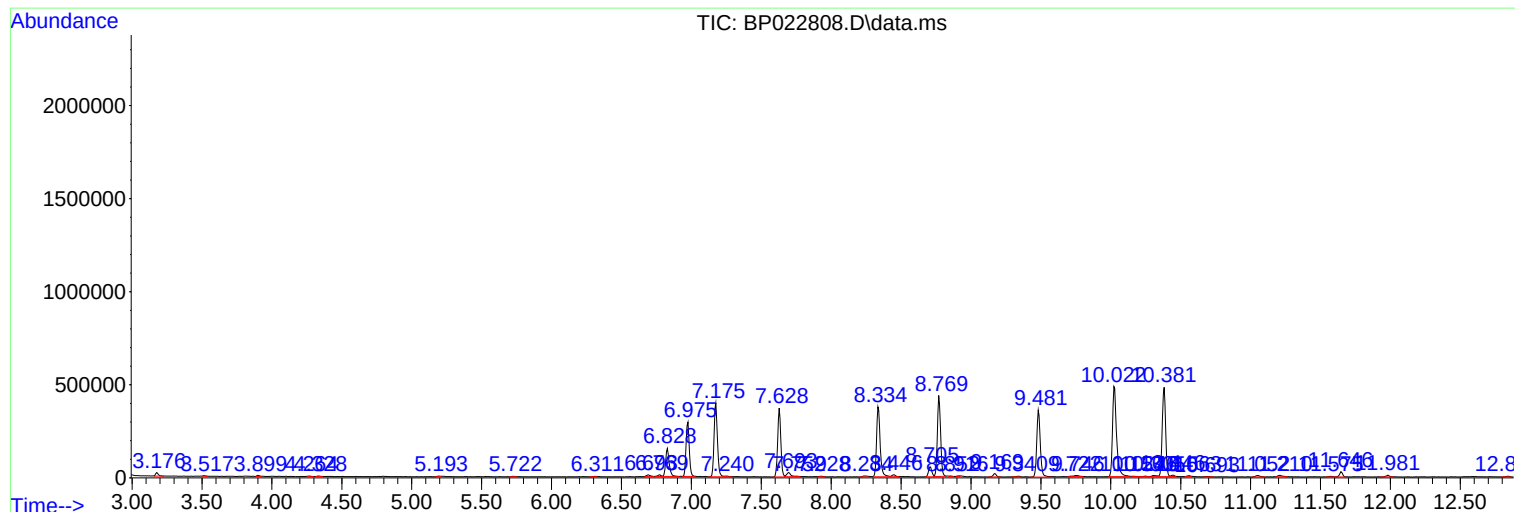

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022808.D
Acq On : 01 Nov 2024 17:28
Operator : RC/JU
Sample : P4583-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0P11










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 2-methoxy- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.705	3.04 ng/ul	88984	1,4-Dichlorobenzene-d4	7.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	95
2			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	94
3			Phenol, 2-methoxy-	124	C7H8O2	000090-05-1	91
4			Mequinol	124	C7H8O2	000150-76-5	64
5			Mequinol	124	C7H8O2	000150-76-5	64

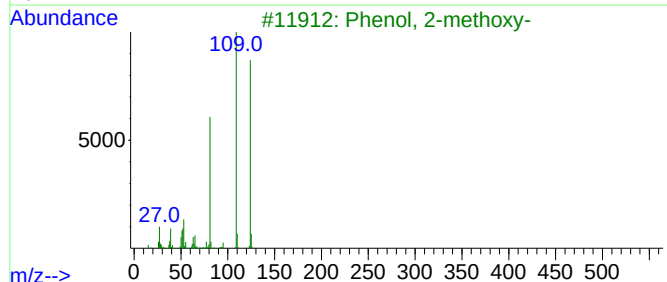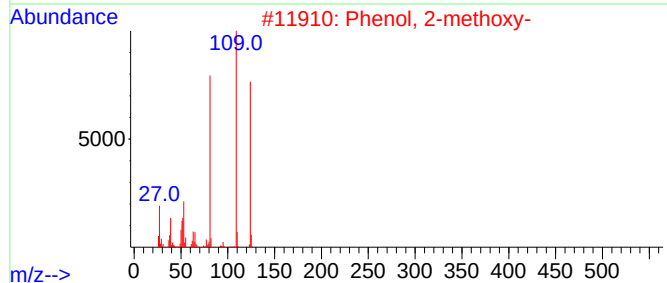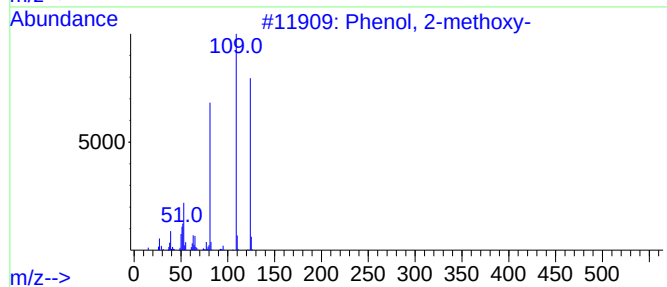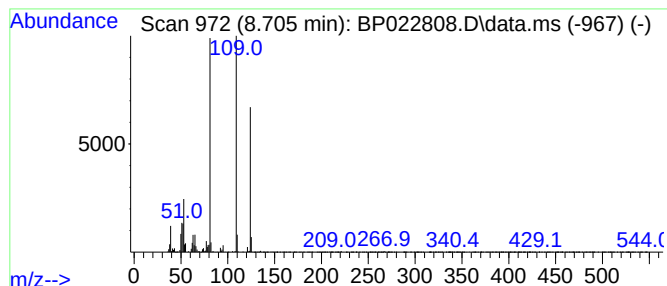

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022808.D
Acq On : 01 Nov 2024 17:28
Operator : RC/JU
Sample : P4583-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0P11










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.763	3.19 ng/ul	259867	Phenanthrene-d10	17.063

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	97		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	90		
3	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	83		
4	2-Hydroxy-4-methoxy-5-(2-methylb...	220	C13H16O3	2108511-28-8	46		
5	Ethanone, 1-(5,6,7,8-tetrahydro...	220	C14H20O2	071596-88-8	46		

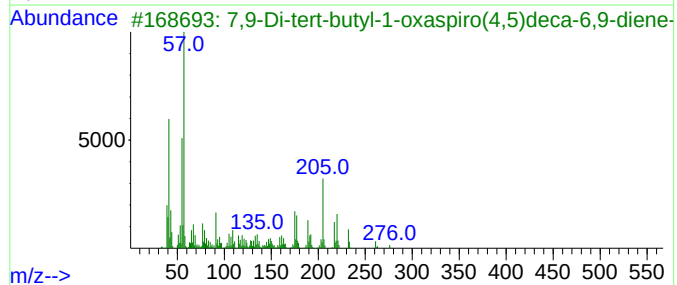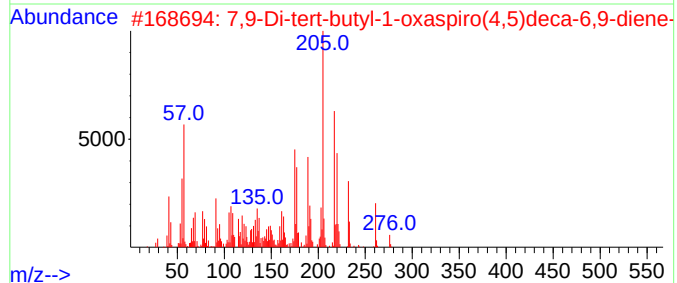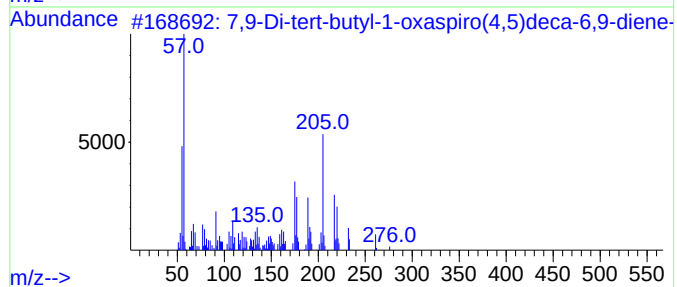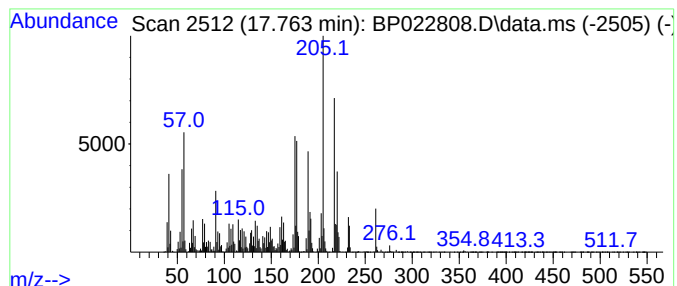

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022808.D
Acq On : 01 Nov 2024 17:28
Operator : RC/JU
Sample : P4583-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0P11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 2-methoxy-	8.705	3.0	ng/u1	88984	1	7.628	585566	20.0
7,9-Di-tert-but...	17.763	3.2	ng/u1	259867	4	17.063	1631120	20.0