

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022811.D
 Acq On : 01 Nov 2024 19:31
 Operator : RC/JU
 Sample : P4627-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COCP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rVB	13231	18773	0.71%	0.093%
2	3.599	100	104	116	rBV	41985	76298	2.89%	0.379%
3	3.899	151	155	160	rVB2	4922	7499	0.28%	0.037%
4	4.393	232	239	245	rBV	111278	152348	5.77%	0.756%
5	5.193	369	375	379	rBV3	2367	3084	0.12%	0.015%
6	5.322	391	397	405	rBV3	7396	17022	0.64%	0.084%
7	5.681	455	458	462	rBV4	3219	4592	0.17%	0.023%
8	6.305	558	564	573	rVB4	7789	15428	0.58%	0.077%
9	6.634	615	620	630	rBV	21125	45962	1.74%	0.228%
10	6.828	647	653	665	rVB2	67446	127562	4.83%	0.633%
11	6.969	671	677	692	rVB	174654	299513	11.34%	1.486%
12	7.175	705	712	722	rBV	251098	404960	15.34%	2.009%
13	7.281	728	730	734	rVB4	3350	3615	0.14%	0.018%
14	7.628	782	789	798	rBV	216339	365641	13.85%	1.814%
15	7.710	800	803	812	rVB8	3259	7575	0.29%	0.038%
16	8.334	901	909	925	rBV	210293	388748	14.72%	1.929%
17	8.451	925	929	936	rVB5	3985	7318	0.28%	0.036%
18	8.769	976	983	995	rBV	274941	460367	17.44%	2.284%
19	9.169	1045	1051	1056	rBV7	3415	6506	0.25%	0.032%
20	9.481	1096	1104	1121	rBV	238585	419167	15.88%	2.079%
21	10.028	1190	1197	1223	rBV	353794	659060	24.96%	3.269%
22	10.387	1250	1258	1269	rVB	304565	503143	19.06%	2.496%
23	10.534	1275	1283	1300	rBV	240180	487426	18.46%	2.418%
24	10.940	1345	1352	1356	rBV7	3030	6169	0.23%	0.031%
25	10.998	1356	1362	1365	rVV4	3082	5916	0.22%	0.029%
26	11.051	1365	1371	1379	rVB3	16180	33599	1.27%	0.167%
27	11.451	1434	1439	1445	rBV9	4474	9923	0.38%	0.049%
28	11.604	1458	1465	1469	rBV2	6665	11871	0.45%	0.059%
29	11.651	1469	1473	1479	rVB3	3635	5778	0.22%	0.029%
30	11.904	1508	1516	1525	rBV2	10272	22348	0.85%	0.111%
31	11.992	1525	1531	1537	rVB3	3937	7796	0.30%	0.039%
32	13.669	1808	1816	1827	rBV	632110	1019240	38.61%	5.056%
33	13.798	1834	1838	1845	rBV10	2717	4511	0.17%	0.022%
34	13.945	1856	1863	1871	rBV	708052	1055740	39.99%	5.237%
35	14.251	1908	1915	1929	rBV	561415	753786	28.55%	3.739%
36	14.475	1948	1953	1956	rVB6	2224	2667	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022811.D
 Acq On : 01 Nov 2024 19:31
 Operator : RC/JU
 Sample : P4627-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	14.528	1956	1962	1975	rBV2	32935	100326	3.80%	0.498%
38	15.104	2051	2060	2063	rBV8	2921	5468	0.21%	0.027%
39	15.263	2080	2087	2096	rBV	1067261	1525654	57.79%	7.569%
40	15.422	2106	2114	2126	rBV	288691	427778	16.20%	2.122%
41	15.516	2128	2130	2136	rVB3	6928	9761	0.37%	0.048%
42	15.851	2181	2187	2189	rBV6	1877	3540	0.13%	0.018%
43	16.033	2211	2218	2223	rBV8	8233	18287	0.69%	0.091%
44	16.133	2231	2235	2240	rBV	7113	10937	0.41%	0.054%
45	16.192	2240	2245	2250	rVV2	12625	20346	0.77%	0.101%
46	16.245	2250	2254	2258	rVV2	9567	13669	0.52%	0.068%
47	16.286	2258	2261	2265	rVB5	3884	5401	0.20%	0.027%
48	16.357	2267	2273	2276	rBV7	2408	5032	0.19%	0.025%
49	16.463	2285	2291	2298	rVB6	4885	10314	0.39%	0.051%
50	16.527	2298	2302	2307	rBV3	8136	16292	0.62%	0.081%
51	16.598	2311	2314	2320	rVB6	4558	7855	0.30%	0.039%
52	16.727	2333	2336	2342	rVB8	1973	3103	0.12%	0.015%
53	17.057	2385	2392	2401	rBV	692076	1001258	37.92%	4.967%
54	17.157	2402	2409	2423	rBV2	1060202	1823690	69.07%	9.047%
55	17.757	2506	2511	2513	rBV5	2172	3553	0.13%	0.018%
56	17.886	2529	2533	2537	rVB5	4605	5716	0.22%	0.028%
57	17.998	2546	2552	2558	rBV4	20309	34175	1.29%	0.170%
58	18.063	2560	2563	2566	rVB5	2868	3433	0.13%	0.017%
59	18.333	2605	2609	2611	rBV5	1863	3037	0.12%	0.015%
60	18.369	2611	2615	2617	rBV5	2160	3231	0.12%	0.016%
61	19.098	2735	2739	2744	rBV	19106	25705	0.97%	0.128%
62	19.169	2747	2751	2755	rBV3	15974	24382	0.92%	0.121%
63	19.333	2775	2779	2785	rBV7	20355	27178	1.03%	0.135%
64	19.545	2809	2815	2824	rBV	1929822	2382180	90.23%	11.818%
65	21.510	3142	3149	3159	rVB2	721702	1244843	47.15%	6.175%
66	24.539	3655	3664	3679	rVB	984114	2640173	100.00%	13.097%
67	24.774	3694	3704	3719	rVB	435879	1330654	50.40%	6.601%


Sum of corrected areas: 20157922

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022811.D
Acq On : 01 Nov 2024 19:31
Operator : RC/JU
Sample : P4627-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

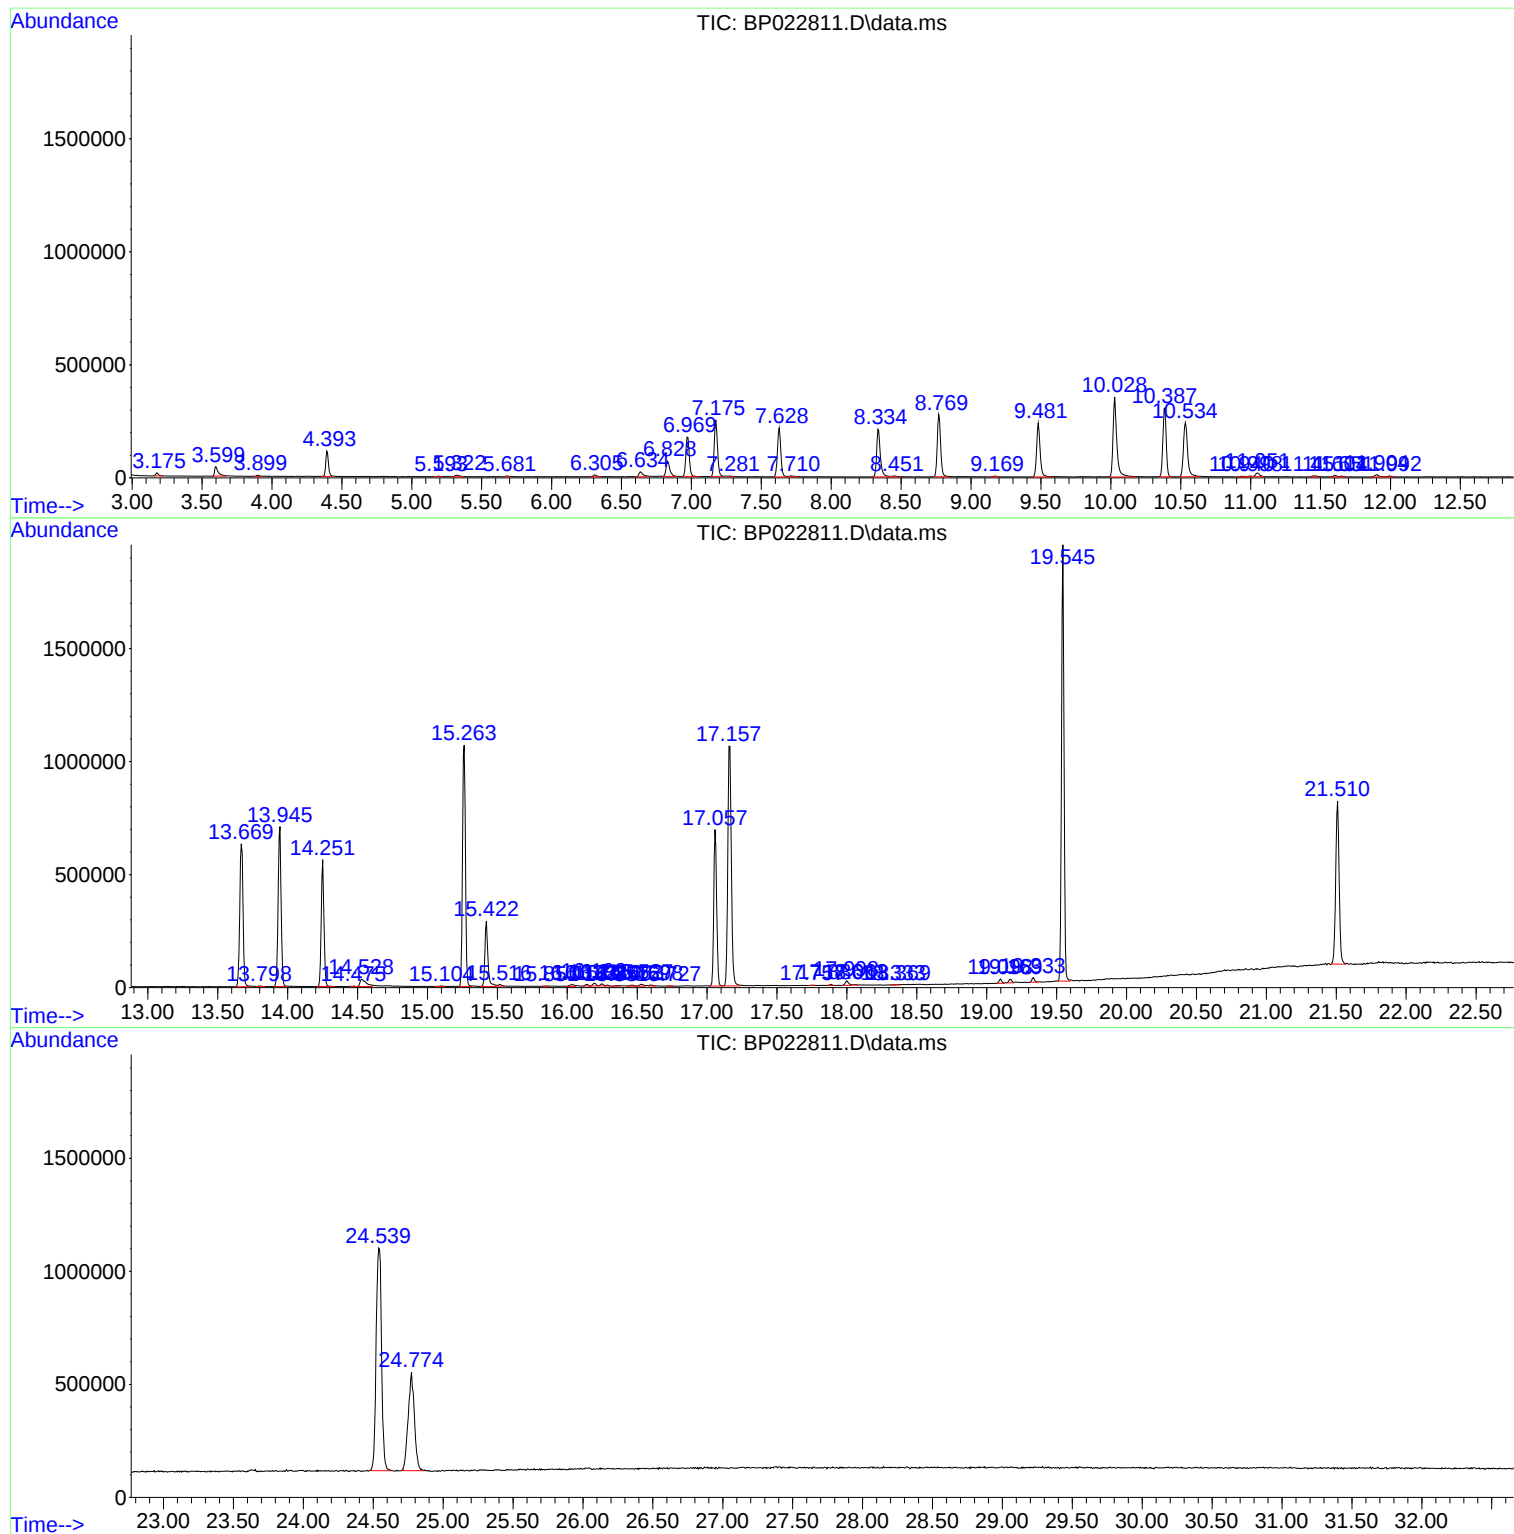

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022811.D
Acq On : 01 Nov 2024 19:31
Operator : RC/JU
Sample : P4627-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022811.D
Acq On : 01 Nov 2024 19:31
Operator : RC/JU
Sample : P4627-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc