

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022812.D
 Acq On : 01 Nov 2024 20:12
 Operator : RC/JU
 Sample : P4627-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	39	rBV2	13217	18633	0.71%	0.094%
2	3.593	100	103	119	rBV	73273	131309	5.01%	0.661%
3	3.899	152	155	163	rVB2	3683	5517	0.21%	0.028%
4	4.393	234	239	249	rBV	94698	131783	5.03%	0.664%
5	5.193	371	375	382	rVB6	2338	4104	0.16%	0.021%
6	5.322	390	397	407	rBV2	7022	14872	0.57%	0.075%
7	5.675	454	457	463	rVB6	2430	4413	0.17%	0.022%
8	6.311	559	565	574	rBV3	6408	12488	0.48%	0.063%
9	6.775	640	644	647	rVV3	2301	3687	0.14%	0.019%
10	6.828	647	653	669	rVV	72943	141059	5.38%	0.710%
11	6.969	669	677	692	rVV	182720	307399	11.73%	1.548%
12	7.175	704	712	723	rBV	260238	413305	15.76%	2.081%
13	7.628	782	789	797	rBV	227502	386118	14.73%	1.944%
14	8.340	903	910	925	rBV	227288	396245	15.11%	1.995%
15	8.769	976	983	997	rBV	290081	464160	17.70%	2.337%
16	8.910	1002	1007	1019	rVV	1427	4156	0.16%	0.021%
17	9.163	1046	1050	1058	rVB5	4314	8451	0.32%	0.043%
18	9.481	1097	1104	1116	rBV	244766	411860	15.71%	2.074%
19	10.028	1190	1197	1224	rBV	301875	638714	24.36%	3.216%
20	10.387	1248	1258	1270	rBV	329478	527786	20.13%	2.658%
21	10.534	1274	1283	1297	rBV	234690	479845	18.30%	2.416%
22	11.640	1467	1471	1480	rBV8	2693	6098	0.23%	0.031%
23	12.004	1524	1533	1539	rBV4	3641	6919	0.26%	0.035%
24	13.651	1807	1813	1826	rBV	741657	1012652	38.63%	5.100%
25	13.945	1856	1863	1874	rBV	744922	1047260	39.95%	5.274%
26	14.257	1910	1916	1924	rBV	590622	773737	29.51%	3.896%
27	14.534	1957	1963	1964	rBV	29923	40763	1.55%	0.205%
28	15.069	2051	2054	2057	rBV5	2004	2857	0.11%	0.014%
29	15.092	2057	2058	2065	rVB6	2175	3206	0.12%	0.016%
30	15.269	2081	2088	2096	rBV	941870	1434088	54.70%	7.222%
31	15.328	2096	2098	2104	rVB5	6525	9368	0.36%	0.047%
32	15.404	2104	2111	2124	rBV	246092	456397	17.41%	2.298%
33	15.639	2146	2151	2161	rVB	45360	60947	2.32%	0.307%
34	16.022	2207	2216	2221	rBV3	4974	11219	0.43%	0.056%
35	17.063	2386	2393	2401	rBV	728804	1042566	39.77%	5.250%
36	17.163	2403	2410	2421	rBV	1312627	1754515	66.92%	8.835%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022812.D
Acq On : 01 Nov 2024 20:12
Operator : RC/JU
Sample : P4627-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.363	2440	2444	2449	rBV7	3090	4912	0.19%	0.025%
38	17.757	2506	2511	2515	rVB8	4963	7777	0.30%	0.039%
39	17.998	2548	2552	2561	rBV2	43096	57732	2.20%	0.291%
40	18.075	2562	2565	2569	rVB3	2898	4552	0.17%	0.023%
41	19.098	2735	2739	2744	rVB2	14865	20368	0.78%	0.103%
42	19.175	2748	2752	2757	rBV	16730	21797	0.83%	0.110%
43	19.275	2767	2769	2771	rVB2	4740	3642	0.14%	0.018%
44	19.333	2775	2779	2787	rVB4	28451	40083	1.53%	0.202%
45	19.545	2809	2815	2825	rBV	1578954	2214615	84.47%	11.152%
46	21.498	3141	3147	3159	rBV2	710349	1305590	49.80%	6.575%
47	24.533	3654	3663	3681	rVB	1152607	2621678	100.00%	13.202%
48	24.763	3693	3702	3715	rVB	465326	1386571	52.89%	6.982%




Sum of corrected areas: 19857813

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022812.D
Acq On : 01 Nov 2024 20:12
Operator : RC/JU
Sample : P4627-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

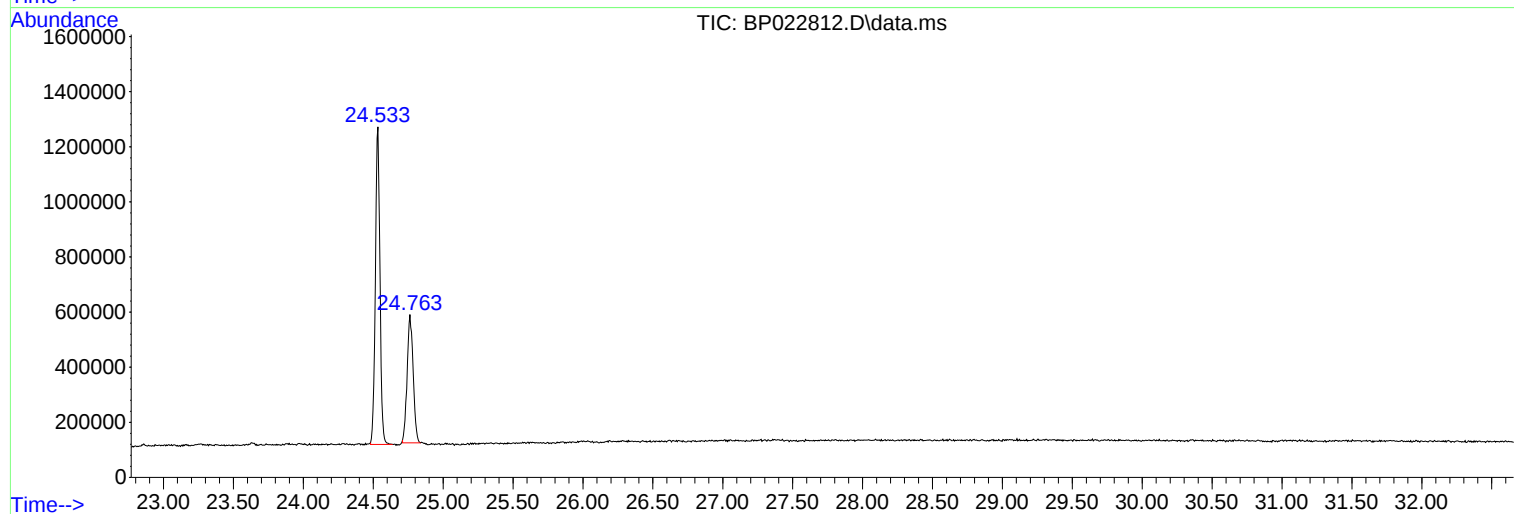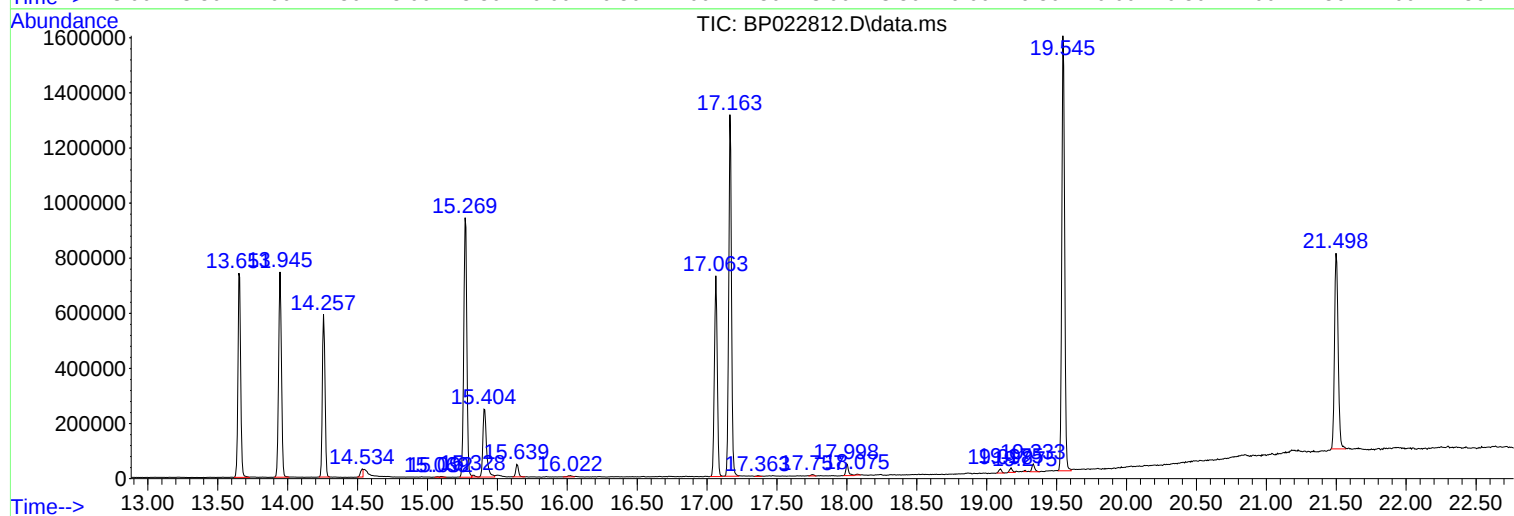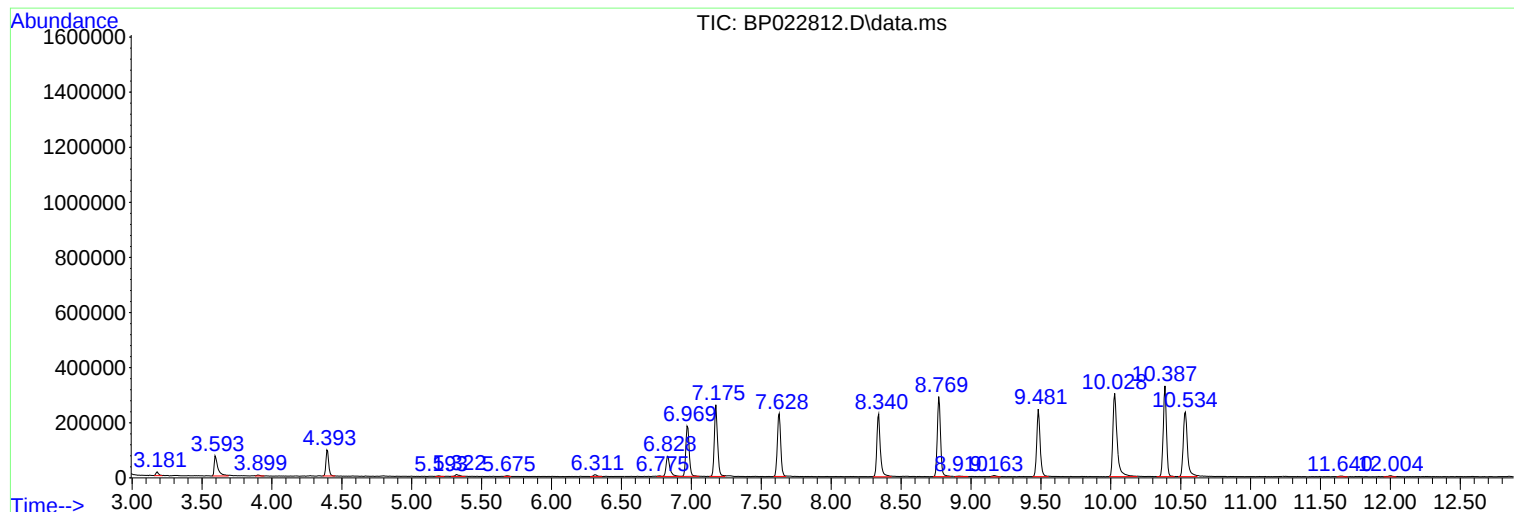

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022812.D
Acq On : 01 Nov 2024 20:12
Operator : RC/JU
Sample : P4627-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022812.D
Acq On : 01 Nov 2024 20:12
Operator : RC/JU
Sample : P4627-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc