

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022816.D
 Acq On : 01 Nov 2024 23:36
 Operator : RC/JU
 Sample : PB164567BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK567

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	40	rBV	19030	24447	1.03%	0.113%
2	3.587	98	102	125	rBV	223120	364571	15.38%	1.680%
3	3.899	150	155	162	rVB2	5917	9169	0.39%	0.042%
4	6.769	639	643	645	rBV4	2935	3686	0.16%	0.017%
5	6.816	645	651	669	rVV	266842	472846	19.95%	2.180%
6	6.969	671	677	689	rVB	198249	321184	13.55%	1.480%
7	7.169	704	711	723	rBV	287552	472228	19.92%	2.177%
8	7.622	781	788	800	rBV	258912	442137	18.65%	2.038%
9	8.334	901	909	932	rBV2	315692	601320	25.37%	2.772%
10	8.763	975	982	996	rBV	267317	474850	20.03%	2.189%
11	9.169	1045	1051	1055	rVB4	5237	8990	0.38%	0.041%
12	9.475	1096	1103	1120	rBV	221664	418676	17.66%	1.930%
13	10.022	1189	1196	1214	rBV	328026	660699	27.87%	3.045%
14	10.381	1249	1257	1266	rBV	365104	601539	25.38%	2.773%
15	10.522	1272	1281	1303	rBV	291876	598006	25.23%	2.756%
16	11.640	1467	1471	1477	rVB6	3974	6632	0.28%	0.031%
17	11.993	1525	1531	1533	rBV4	4191	6938	0.29%	0.032%
18	13.657	1806	1814	1829	rBV	798268	1027014	43.33%	4.734%
19	13.946	1856	1863	1874	rBV	863630	1140737	48.12%	5.258%
20	14.257	1909	1916	1929	rBV	611996	905212	38.19%	4.172%
21	14.510	1950	1959	1976	rBV	148500	451958	19.07%	2.083%
22	14.693	1988	1990	1996	rVB7	2382	3829	0.16%	0.018%
23	15.263	2078	2087	2101	rBV	895590	1507746	63.61%	6.950%
24	15.410	2104	2112	2125	rBV	174102	371292	15.66%	1.711%
25	16.051	2218	2221	2226	rBV7	1405	2397	0.10%	0.011%
26	16.545	2300	2305	2307	rBV6	2250	3665	0.15%	0.017%
27	16.845	2352	2356	2360	rBV7	2098	3640	0.15%	0.017%
28	17.045	2384	2390	2400	rBV	865755	1223628	51.62%	5.640%
29	17.157	2400	2409	2425	rBV2	976192	1787113	75.39%	8.237%
30	17.475	2457	2463	2466	rBV7	1316	3100	0.13%	0.014%
31	17.998	2550	2552	2555	rVB4	3094	2604	0.11%	0.012%
32	19.086	2733	2737	2741	rBV	21531	24936	1.05%	0.115%
33	19.157	2745	2749	2757	rBV3	17863	28058	1.18%	0.129%
34	19.528	2807	2812	2823	rBV	1517071	2250193	94.93%	10.372%
35	21.492	3140	3146	3157	rVB2	890110	1503009	63.41%	6.928%
36	24.510	3651	3659	3675	rVB	1015600	2370469	100.00%	10.926%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022816.D
Acq On : 01 Nov 2024 23:36
Operator : RC/JU
Sample : PB164567BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.745	3691	3699	3720	rVB	502144	1596349	67.34%	7.358%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 21694867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022816.D
Acq On : 01 Nov 2024 23:36
Operator : RC/JU
Sample : PB164567BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

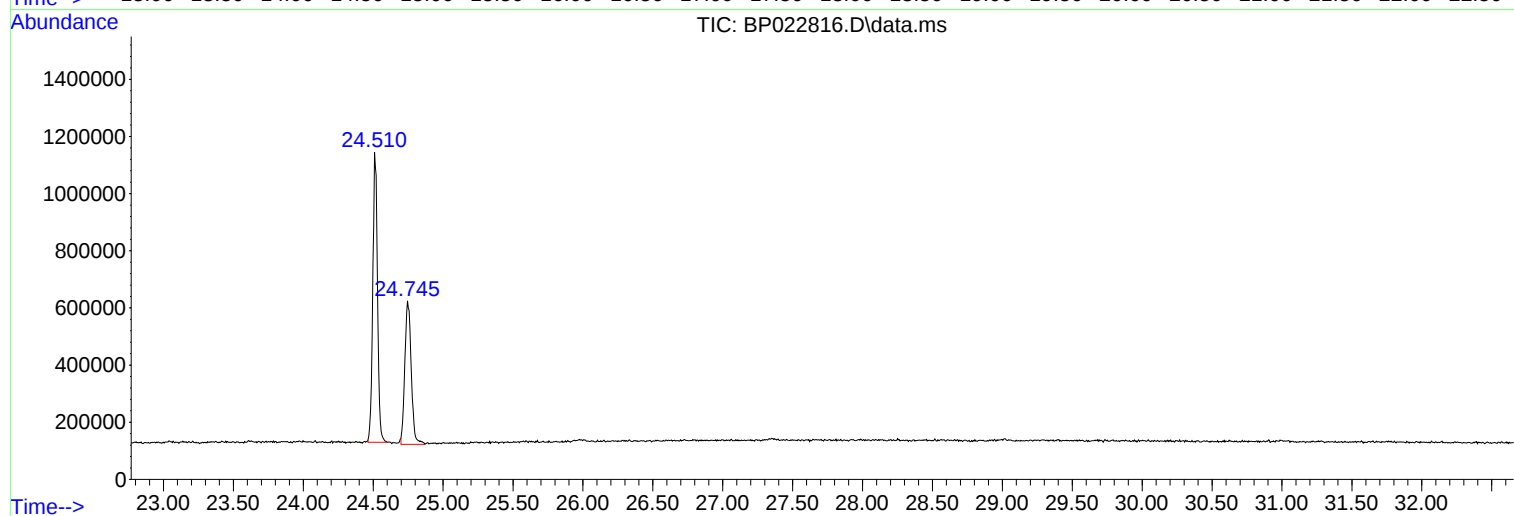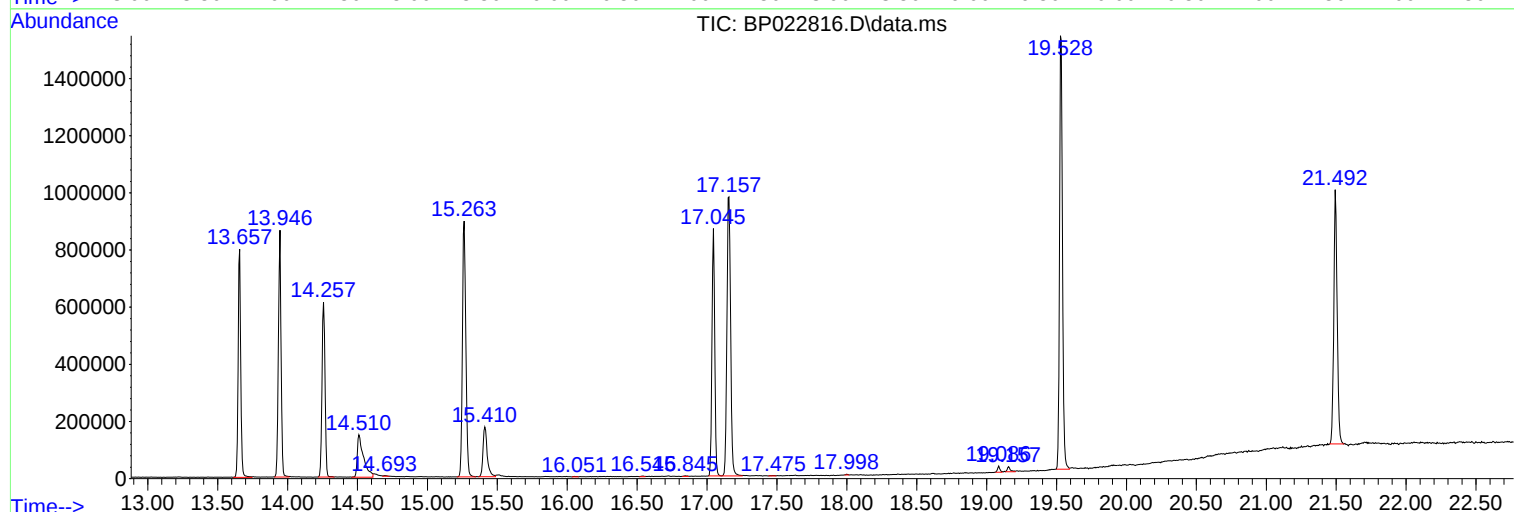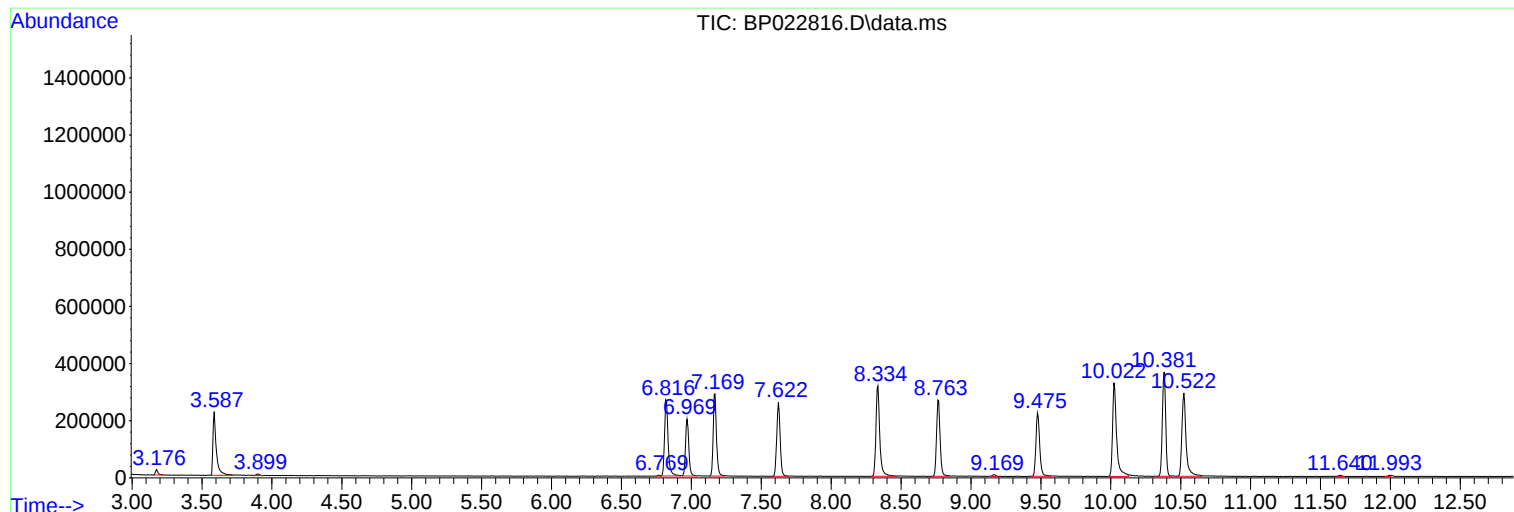

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022816.D
Acq On : 01 Nov 2024 23:36
Operator : RC/JU
Sample : PB164567BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022816.D
Acq On : 01 Nov 2024 23:36
Operator : RC/JU
Sample : PB164567BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc