

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022817.D
 Acq On : 02 Nov 2024 00:17
 Operator : RC/JU
 Sample : P4630-19
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	35	rBV	10957	14354	0.64%	0.074%
2	3.216	35	39	48	rVV	36183	51698	2.32%	0.265%
3	3.304	51	54	59	rVV7	3350	4057	0.18%	0.021%
4	3.893	152	154	163	rVB3	3774	5996	0.27%	0.031%
5	4.022	169	176	177	rBV8	2213	3578	0.16%	0.018%
6	4.081	177	186	190	rVB	37689	72856	3.26%	0.374%
7	4.328	225	228	232	rBV5	2447	3963	0.18%	0.020%
8	5.234	375	382	392	rBV2	11370	23221	1.04%	0.119%
9	5.498	421	427	433	rBV3	3656	7126	0.32%	0.037%
10	6.775	638	644	647	rBV	5338	8547	0.38%	0.044%
11	6.828	647	653	666	rVV2	92310	176060	7.89%	0.903%
12	6.975	670	678	692	rBV	188559	316129	14.16%	1.621%
13	7.169	704	711	722	rBV	251833	450667	20.19%	2.311%
14	7.245	722	724	728	rVB4	2098	2655	0.12%	0.014%
15	7.363	741	744	749	rBV4	1781	2255	0.10%	0.012%
16	7.628	783	789	798	rBV	232146	383924	17.20%	1.969%
17	7.693	798	800	806	rVB7	2306	4240	0.19%	0.022%
18	8.340	903	910	924	rBV	262425	442959	19.85%	2.272%
19	8.463	927	931	934	rVV6	1988	3176	0.14%	0.016%
20	8.522	936	941	947	rVB8	2079	3907	0.18%	0.020%
21	8.775	977	984	996	rBV	263887	469457	21.03%	2.407%
22	8.863	996	999	1002	rVB4	2289	2704	0.12%	0.014%
23	9.175	1046	1052	1058	rBV	8655	13225	0.59%	0.068%
24	9.422	1089	1094	1097	rBV5	2151	3758	0.17%	0.019%
25	9.487	1097	1105	1121	rVV	223537	430741	19.30%	2.209%
26	9.681	1133	1138	1143	rBV8	1672	2940	0.13%	0.015%
27	9.910	1169	1177	1181	rBV6	3014	5663	0.25%	0.029%
28	9.986	1183	1190	1191	rBV5	2589	4565	0.20%	0.023%
29	10.028	1191	1197	1222	rVB	290763	650626	29.15%	3.336%
30	10.386	1251	1258	1269	rBV	294038	515913	23.12%	2.646%
31	10.939	1348	1352	1355	rBV5	1648	2688	0.12%	0.014%
32	11.657	1469	1474	1479	rVB8	4231	7768	0.35%	0.040%
33	11.704	1479	1482	1483	rVV3	2532	2453	0.11%	0.013%
34	11.722	1483	1485	1491	rVB6	2663	3427	0.15%	0.018%
35	11.839	1496	1505	1513	rVB2	47629	74815	3.35%	0.384%
36	11.986	1524	1530	1540	rVB3	5788	11027	0.49%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
 Data File : BP022817.D
 Acq On : 02 Nov 2024 00:17
 Operator : RC/JU
 Sample : P4630-19
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	12.186	1560	1564	1568	rBV7	1722	2793	0.13%	0.014%
38	12.610	1628	1636	1639	rVV10	1161	2533	0.11%	0.013%
39	12.739	1652	1658	1662	rBV2	2578	3984	0.18%	0.020%
40	13.151	1723	1728	1733	rBV7	1783	3702	0.17%	0.019%
41	13.439	1773	1777	1781	rVB6	2115	3070	0.14%	0.016%
42	13.669	1809	1816	1828	rBV	825150	1063012	47.63%	5.451%
43	13.798	1834	1838	1847	rVB8	5321	8732	0.39%	0.045%
44	13.939	1853	1862	1872	rBV2	435222	742029	33.25%	3.805%
45	14.251	1905	1915	1924	rBV	473779	804180	36.03%	4.124%
46	14.339	1924	1930	1936	rVB	22030	36619	1.64%	0.188%
47	14.516	1954	1960	1970	rBV	54825	152321	6.82%	0.781%
48	14.680	1986	1988	1994	rVB6	3274	4521	0.20%	0.023%
49	15.027	2043	2047	2052	rVV2	8217	11784	0.53%	0.060%
50	15.074	2052	2055	2057	rVV3	2648	3639	0.16%	0.019%
51	15.098	2057	2059	2064	rVB2	3986	4025	0.18%	0.021%
52	15.257	2077	2086	2096	rBV	1032400	1559811	69.89%	7.999%
53	15.410	2104	2112	2126	rBV	307561	460051	20.61%	2.359%
54	15.510	2126	2129	2143	rVB7	8380	15050	0.67%	0.077%
55	15.786	2174	2176	2181	rVV6	1749	2335	0.10%	0.012%
56	15.845	2184	2186	2190	rVV4	1908	2238	0.10%	0.011%
57	16.639	2316	2321	2328	rBV2	21897	34091	1.53%	0.175%
58	16.721	2331	2335	2339	rVV6	1623	2355	0.11%	0.012%
59	16.845	2353	2356	2361	rBV7	1699	2409	0.11%	0.012%
60	17.051	2384	2391	2402	rVB	752253	1073149	48.08%	5.503%
61	17.163	2402	2410	2427	rBV	936152	1714799	76.83%	8.794%
62	17.563	2473	2478	2481	rBV4	3027	5338	0.24%	0.027%
63	17.639	2487	2491	2494	rBV6	2270	3595	0.16%	0.018%
64	17.763	2505	2512	2520	rBV6	16899	32837	1.47%	0.168%
65	17.945	2536	2543	2547	rBV4	28857	42361	1.90%	0.217%
66	17.992	2547	2551	2557	rVV3	50220	76335	3.42%	0.391%
67	18.057	2559	2562	2568	rVB3	5172	8668	0.39%	0.044%
68	18.298	2600	2603	2606	rVV4	3244	3656	0.16%	0.019%
69	18.515	2637	2640	2648	rVB8	13967	20119	0.90%	0.103%
70	18.980	2716	2719	2722	rBV4	14426	17299	0.78%	0.089%
71	19.086	2733	2737	2741	rBV5	18473	25122	1.13%	0.129%
72	19.127	2741	2744	2746	rVV2	19722	24078	1.08%	0.123%
73	19.157	2746	2749	2752	rVV	16732	21725	0.97%	0.111%
74	19.204	2752	2757	2767	rVB2	58414	94939	4.25%	0.487%
75	19.327	2773	2778	2783	rBV2	55763	80661	3.61%	0.414%
76	19.533	2807	2813	2822	rBV	1522444	2062354	92.41%	10.576%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022817.D
Acq On : 02 Nov 2024 00:17
Operator : RC/JU
Sample : P4630-19
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP13

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

77	21.498	3141	3147	3156	rBV2	863375	1355805	60.75%	6.953%
78	24.527	3653	3662	3675	rVB2	904788	2231861	100.00%	11.445%
79	24.762	3692	3702	3717	rVB2	496959	1497400	67.09%	7.679%




Sum of corrected areas: 19500523

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022817.D
Acq On : 02 Nov 2024 00:17
Operator : RC/JU
Sample : P4630-19
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

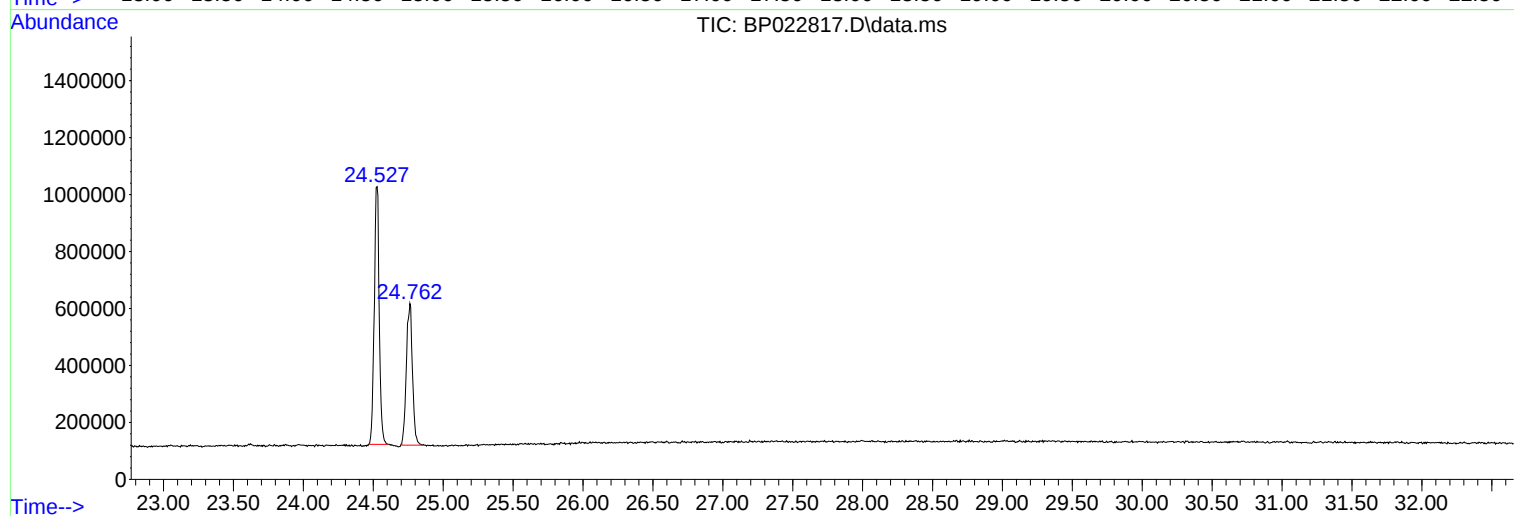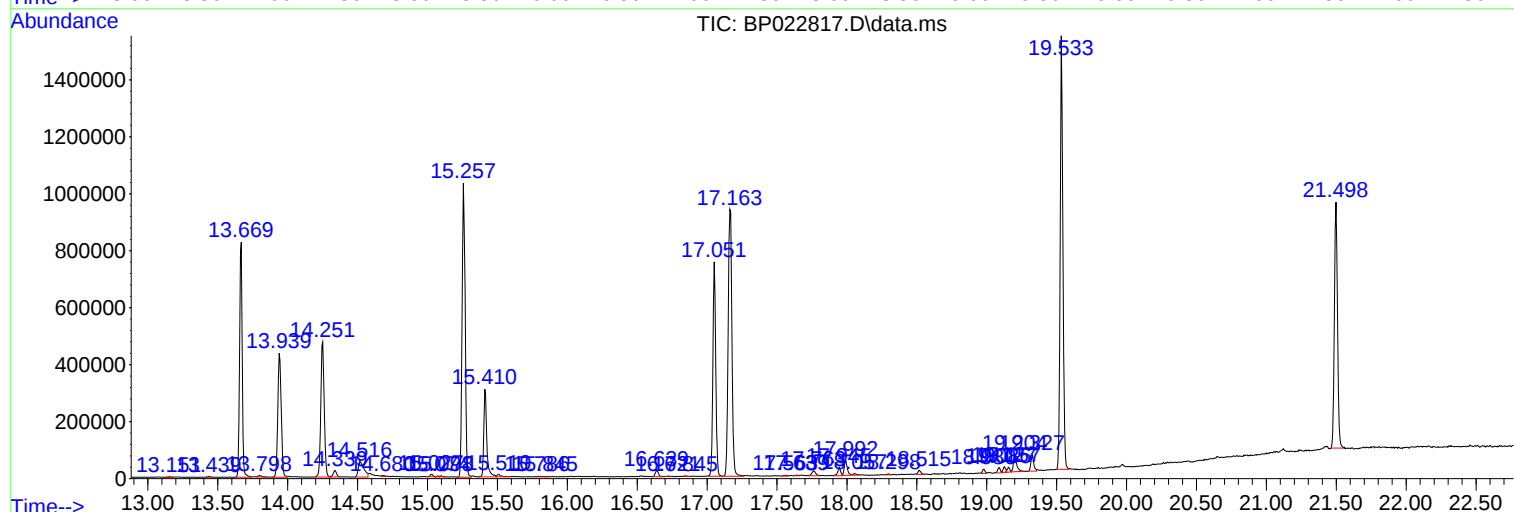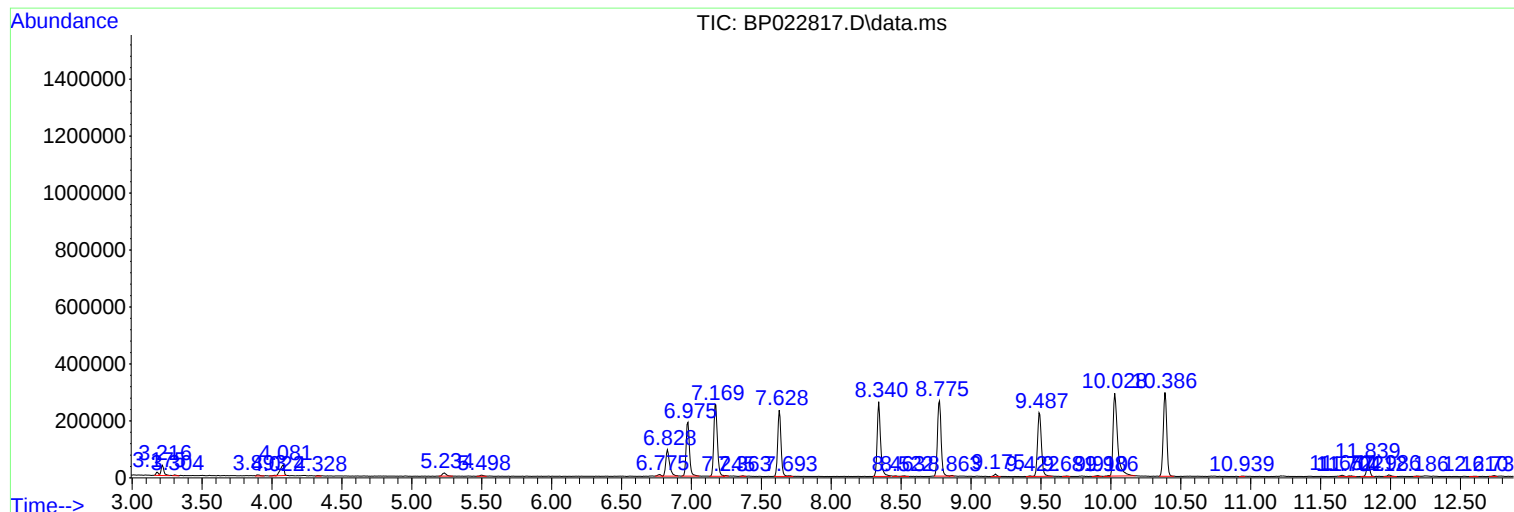

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022817.D
Acq On : 02 Nov 2024 00:17
Operator : RC/JU
Sample : P4630-19
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103024\
Data File : BP022817.D
Acq On : 02 Nov 2024 00:17
Operator : RC/JU
Sample : P4630-19
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc