

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012404.D
 Acq On : 01 Nov 2022 01:16
 Operator : CG/JU
 Sample : N5216-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA59

Quant Time: Nov 01 01:52:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 01 01:03:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	256901	20.000	ng/u1	0.00
20) Naphthalene-d8	10.593	136	1136152	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	749303	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	1677682	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1955092	20.000	ng/u1	0.00
88) Perylene-d12	23.686	264	2063884	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	24256	3.802	ng/uL	0.00
4) Pyridine-d5	3.675	84	67041	3.658	ng/u1	0.02
7) Phenol-d5	6.969	99	151446	6.573	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	440555	32.028	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	442276	26.284	ng/u1	0.00
15) 4-Methylphenol-d8	8.510	113	302292	16.587	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	306232	41.564	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	323709	42.330	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	545937	32.942	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	635345	25.747	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	2047210	39.911	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	2305831	39.337	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	65560	6.753	ng/u1	0.00
60) Fluorene-d10	15.440	176	1790869	40.779	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	318791	36.497	ng/u1	0.00
73) Anthracene-d10	17.304	188	2996384	41.451	ng/u1	0.00
81) Pyrene-d10	19.545	212	3728064	37.980	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.533	264	4223225	41.879	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.204	149	71977	1.006	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012404.D
Acq On : 01 Nov 2022 01:16
Operator : CG/JU
Sample : N5216-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA59

Quant Time: Nov 01 01:52:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 01 01:03:58 2022
Response via : Initial Calibration

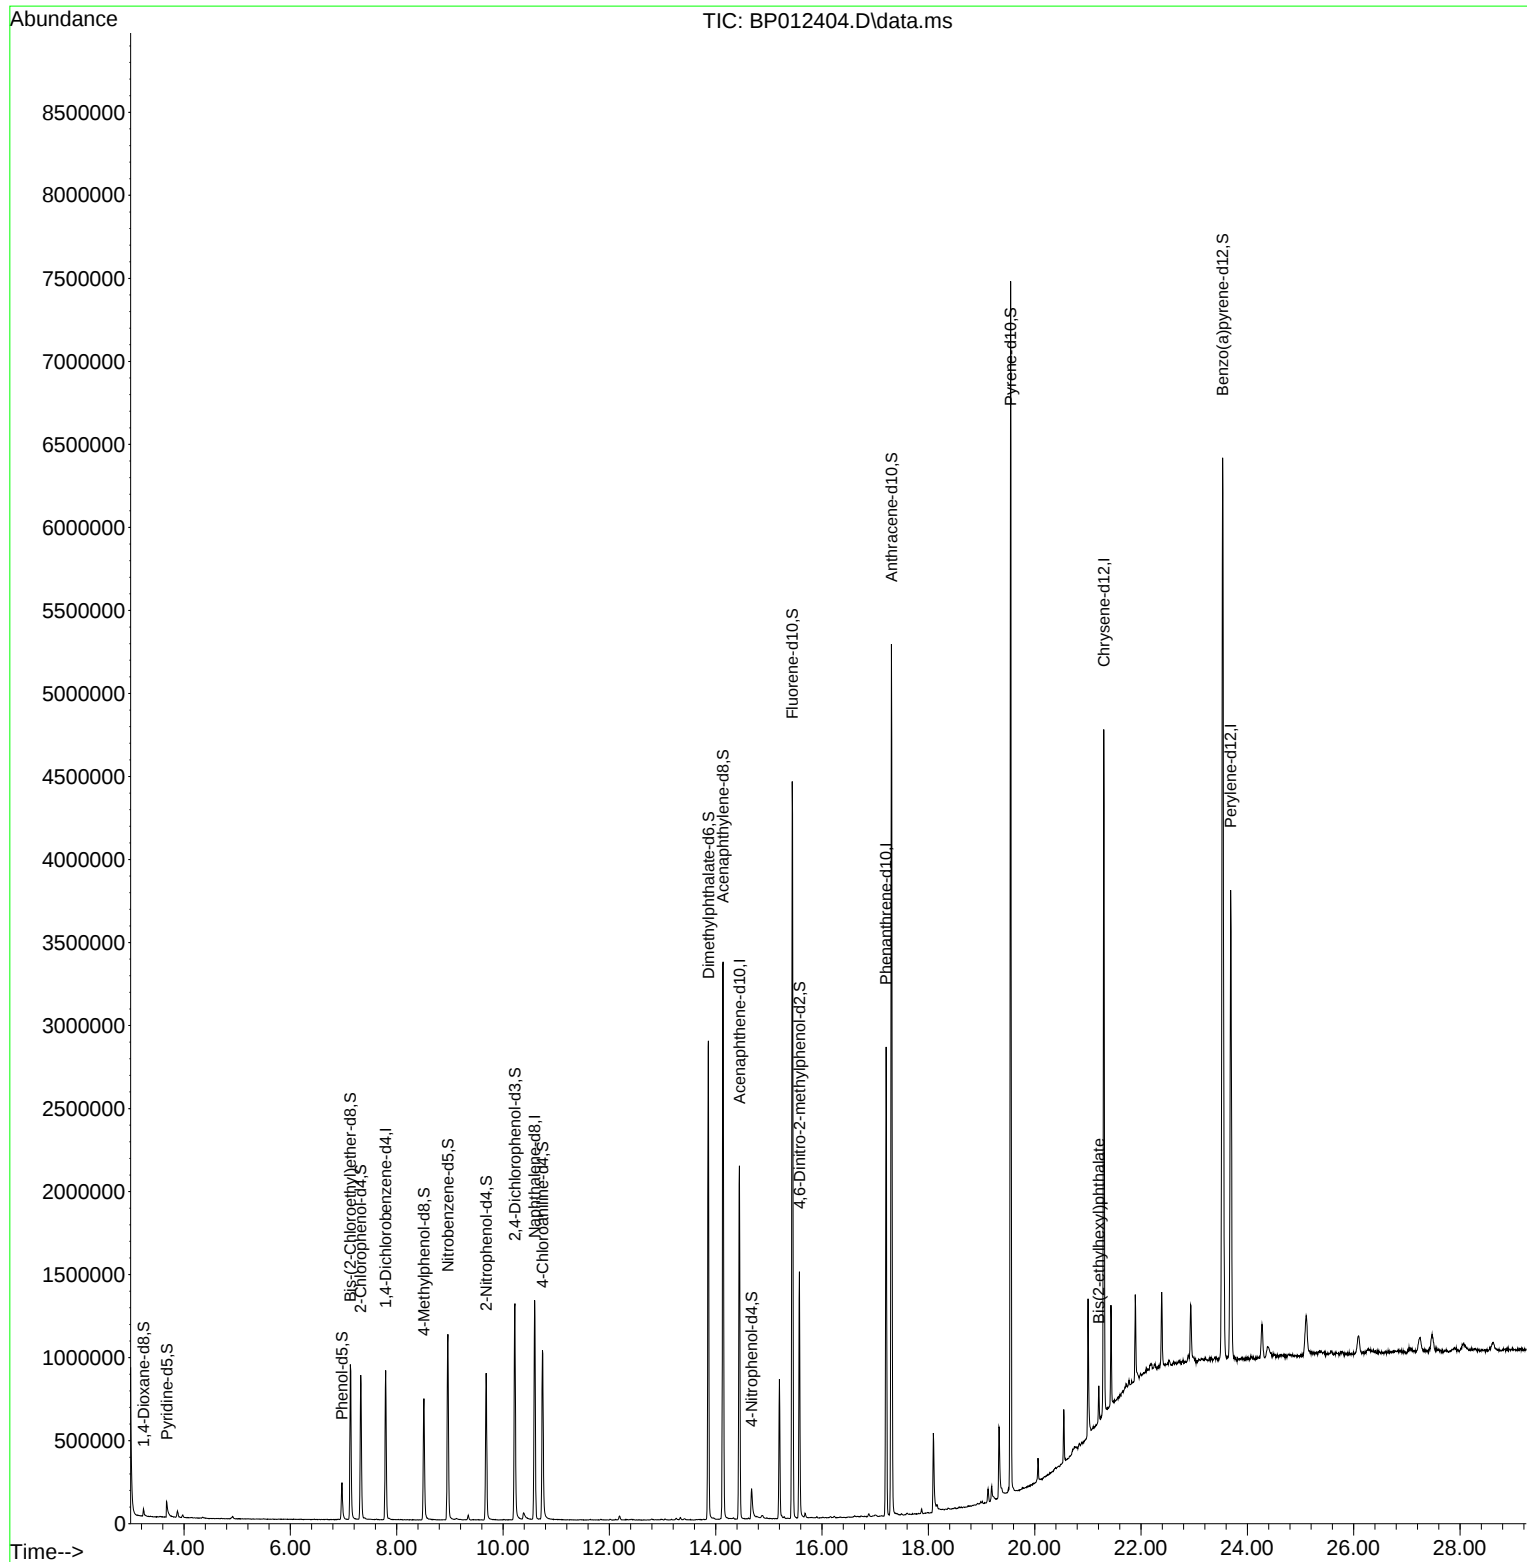

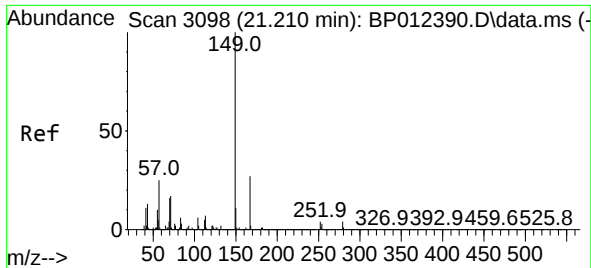

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.006 ng/ul
 RT: 21.204 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP012404.D
 Acq: 01 Nov 2022 01:16

Instrument :
 BNA_P
 ClientSampleId :
 BHA59

Tgt Ion:149 Resp: 71977
 Ion Ratio Lower Upper
 149 100
 167 26.3 22.1 33.1
 279 4.1 3.7 5.5

