

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012441.D
 Acq On : 01 Nov 2022 23:02
 Operator : CG/JU
 Sample : N5300-07
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHAC1

Quant Time: Nov 02 00:54:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 01 01:03:58 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	247153	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	1138370	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.440	164	767574	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1706932	20.000	ng/u1	-0.01
79) Chrysene-d12	21.298	240	1717143	20.000	ng/u1	0.00
88) Perylene-d12	23.680	264	1464119	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	28098	4.578	ng/uL	0.00
4) Pyridine-d5	3.664	84	147503	8.365	ng/u1	0.00
7) Phenol-d5	6.963	99	190162	8.578	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	497559	37.599	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	515304	31.832	ng/u1	0.00
15) 4-Methylphenol-d8	8.505	113	379174	21.627	ng/u1	0.00
21) Nitrobenzene-d5	8.957	128	355898	48.211	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	384146	50.136	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	667837	40.219	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	688019	27.828	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	2325441	44.257	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	2588265	43.104	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	67802	6.818	ng/u1	0.00
60) Fluorene-d10	15.440	176	1991284	44.263	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	237166	26.687	ng/u1	-0.01
73) Anthracene-d10	17.298	188	3246418	44.140	ng/u1	-0.01
81) Pyrene-d10	19.545	212	3838735	44.527	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.527	264	3264250	45.629	ng/u1	-0.02
Target Compounds						
52) Acenaphthene	14.504	153	76422	1.615	ng/u1	98
61) Fluorene	15.492	166	75756	1.476	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012441.D
Acq On : 01 Nov 2022 23:02
Operator : CG/JU
Sample : N5300-07
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHAC1

Quant Time: Nov 02 00:54:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 01 01:03:58 2022
Response via : Initial Calibration




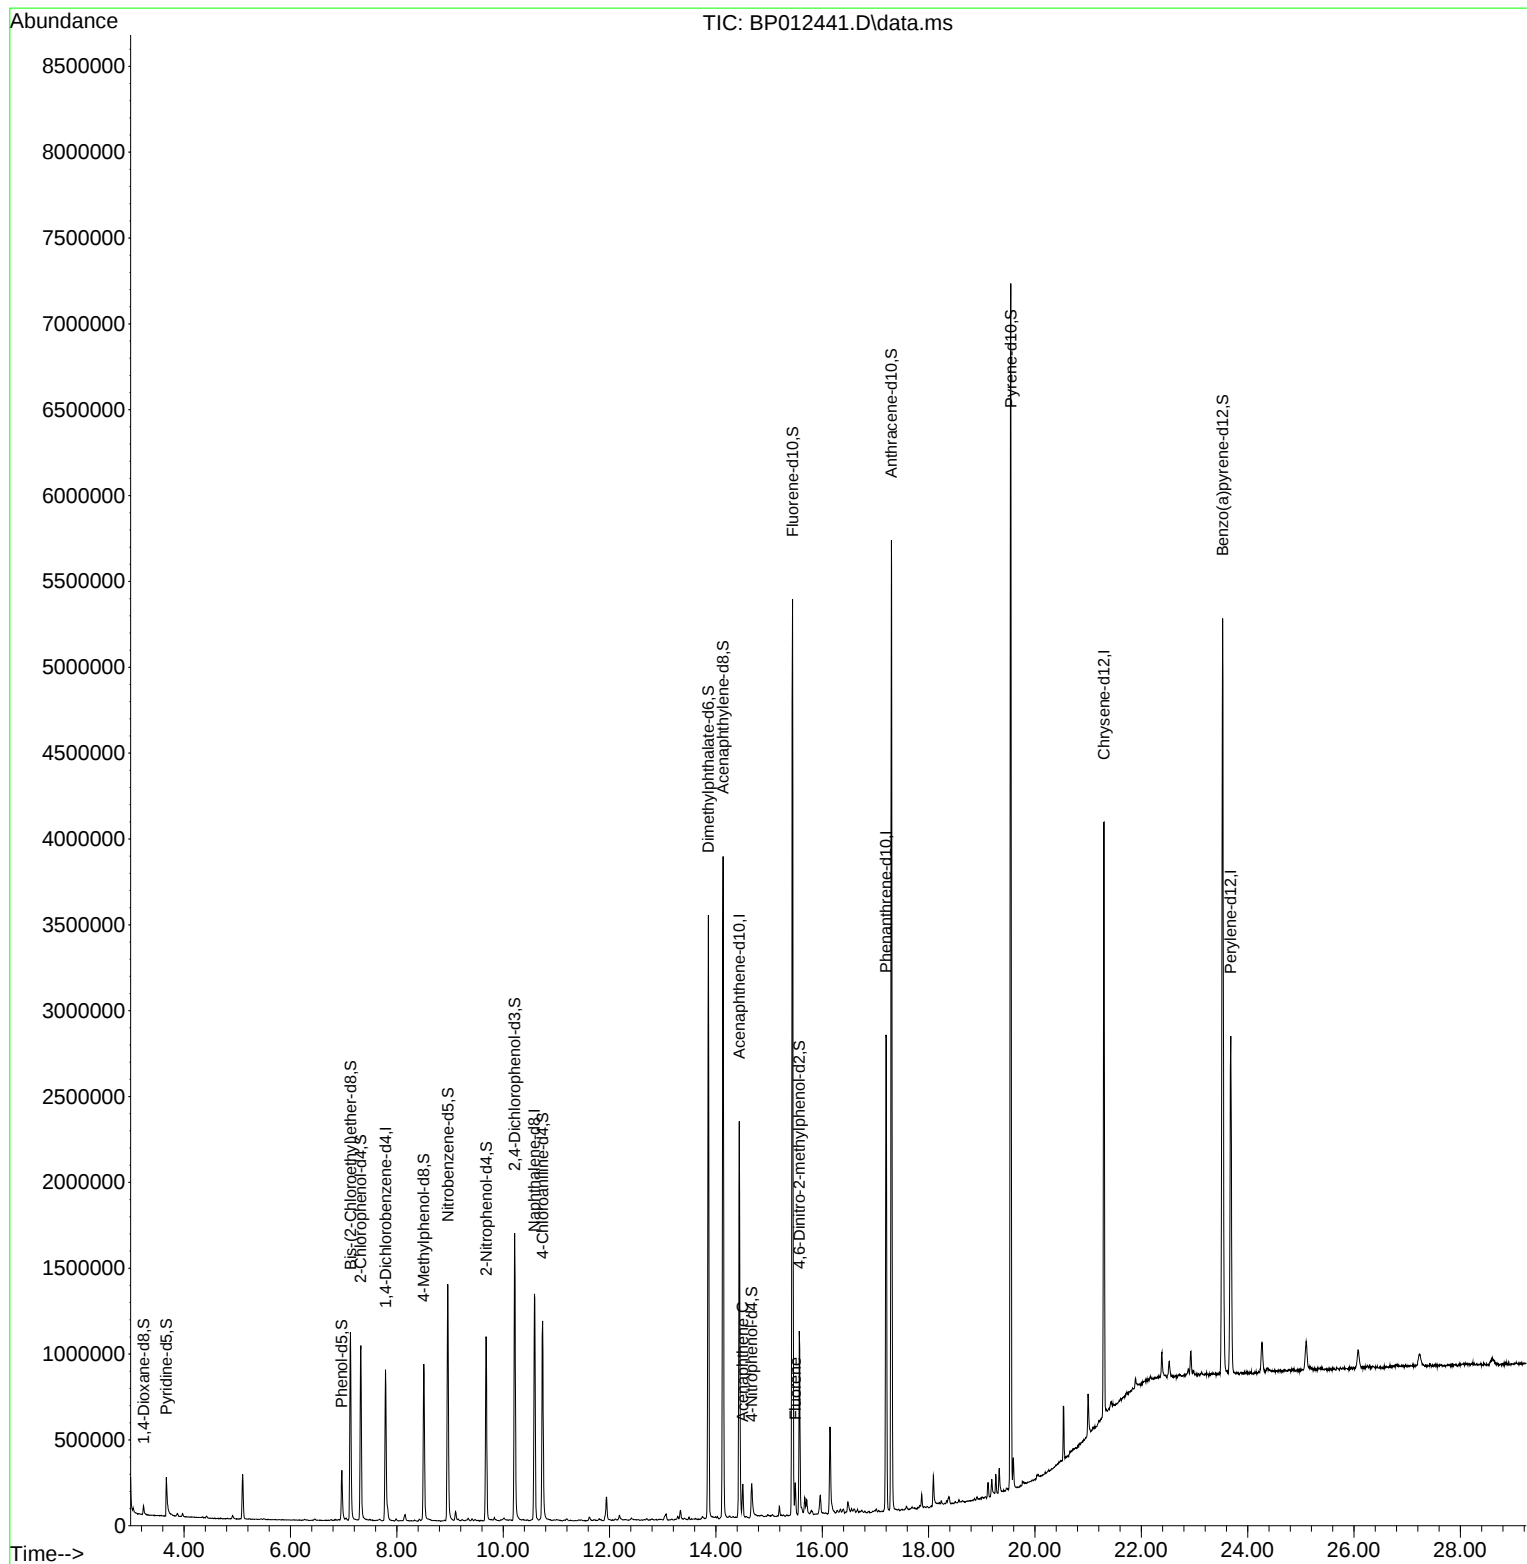


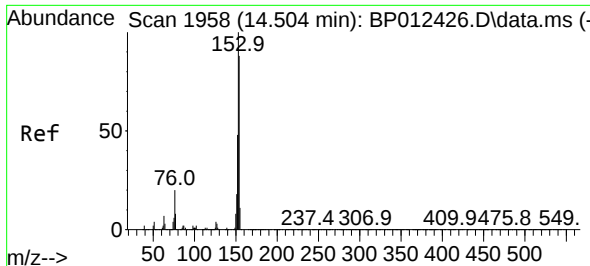

#52
Acenaphthene
Concen: 1.615 ng/ul
RT: 14.504 min Scan# 1958
Delta R.T. -0.006 min
Lab File: BP012441.D
Acq: 01 Nov 2022 23:02

Instrument :
BNA_P
ClientSampleId :
BHAC1

Tgt Ion:153 Resp: 76422
Ion Ratio Lower Upper
153 100
152 47.4 38.6 58.0
154 88.0 71.6 107.4

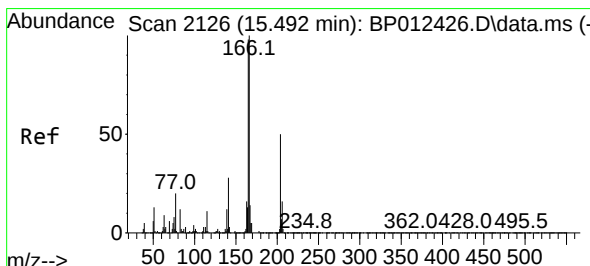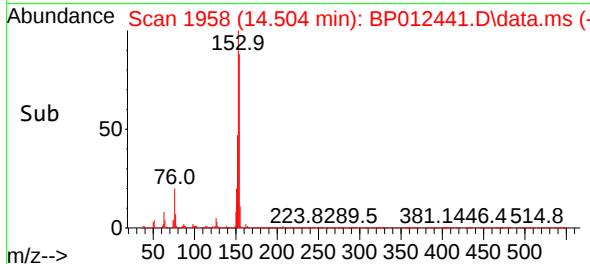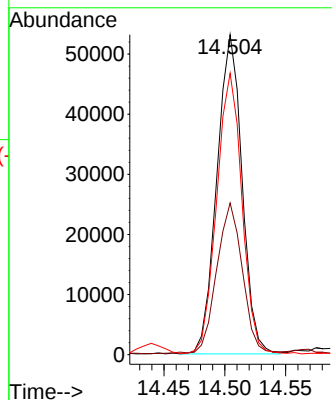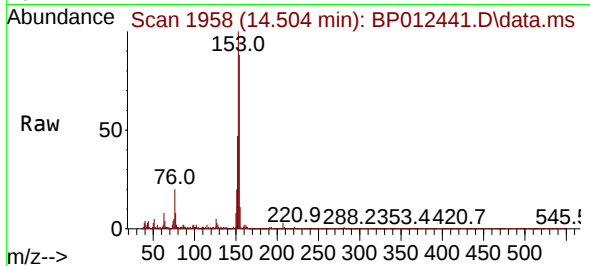

#61
Fluorene
Concen: 1.476 ng/ul
RT: 15.492 min Scan# 2126
Delta R.T. -0.012 min
Lab File: BP012441.D
Acq: 01 Nov 2022 23:02

Tgt Ion:166 Resp: 75756
Ion Ratio Lower Upper
166 100
165 99.1 77.8 116.8
167 14.4 10.6 15.8

