

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012382.D
 Acq On : 31 Oct 2022 12:04
 Operator : CG/JU
 Sample : PB148438BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK438

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	51	rVB	75092	104078	1.20%	0.129%
2	3.658	111	114	134	rBV	821565	1444681	16.69%	1.789%
3	3.975	164	168	174	rVB	21846	31385	0.36%	0.039%
4	6.969	670	677	693	rBV	1122175	1862656	21.52%	2.307%
5	7.134	698	705	718	rBV	956331	1554041	17.95%	1.925%
6	7.328	731	738	753	rBV	1143572	1843346	21.29%	2.283%
7	7.799	810	818	833	rBV	977585	1667294	19.26%	2.065%
8	8.510	931	939	955	rBV	1366658	2346652	27.11%	2.906%
9	8.963	1007	1016	1031	rBV	1069634	1815669	20.97%	2.249%
10	9.687	1130	1139	1153	rBV	872218	1485301	17.16%	1.839%
11	10.222	1222	1230	1250	rBV	1246108	2305004	26.63%	2.855%
12	10.599	1285	1294	1305	rBV	1478744	2504908	28.94%	3.102%
13	10.746	1312	1319	1341	rBV	1335004	2489309	28.75%	3.083%
14	12.198	1560	1566	1576	rBV2	18618	40891	0.47%	0.051%
15	13.428	1769	1775	1779	rBV6	5201	9461	0.11%	0.012%
16	13.863	1842	1849	1863	rBV	2533096	3651255	42.18%	4.522%
17	14.140	1889	1896	1917	rBV	2938690	4396547	50.79%	5.445%
18	14.451	1942	1949	1966	rBV	2331840	3479341	40.19%	4.309%
19	14.669	1980	1986	2008	rBV	1012537	1805288	20.85%	2.236%
20	15.445	2111	2118	2134	rBV	4005424	5675647	65.56%	7.029%
21	15.581	2135	2141	2155	rVV	1074189	1692215	19.55%	2.096%
22	15.687	2156	2159	2168	rVB3	23772	43997	0.51%	0.054%
23	17.210	2411	2418	2428	rBV	3108334	4346953	50.21%	5.383%
24	17.310	2428	2435	2453	rVV2	4505321	6510187	75.20%	8.062%
25	17.833	2521	2524	2530	rBV4	9426	14914	0.17%	0.018%
26	18.133	2571	2575	2578	rBV6	29014	50312	0.58%	0.062%
27	19.128	2741	2744	2749	rBV3	54415	67377	0.78%	0.083%
28	19.198	2752	2756	2761	rBV	56070	86119	0.99%	0.107%
29	19.551	2810	2816	2827	rBV	6181617	8234521	95.12%	10.198%
30	21.304	3109	3114	3121	rBV	4139085	5413481	62.53%	6.704%
31	23.545	3489	3495	3510	rVB2	4276820	8656998	100.00%	10.721%
32	23.698	3515	3521	3531	rVB2	2596768	5119002	59.13%	6.339%




Sum of corrected areas: 80748830

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012382.D
Acq On : 31 Oct 2022 12:04
Operator : CG/JU
Sample : PB148438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

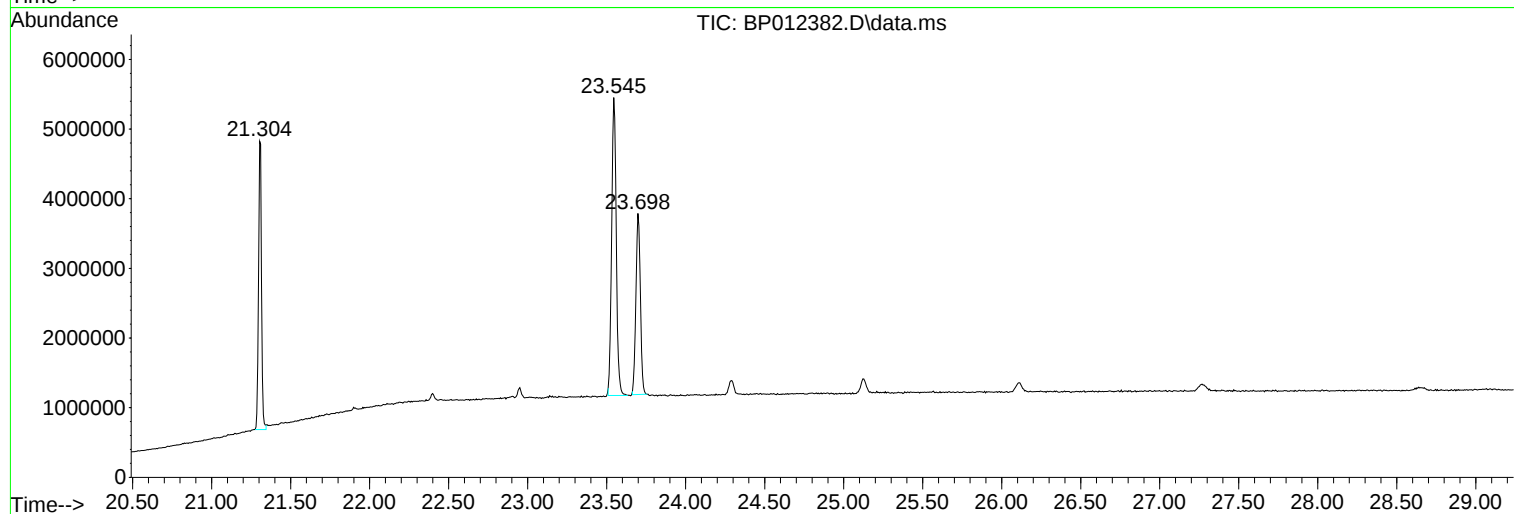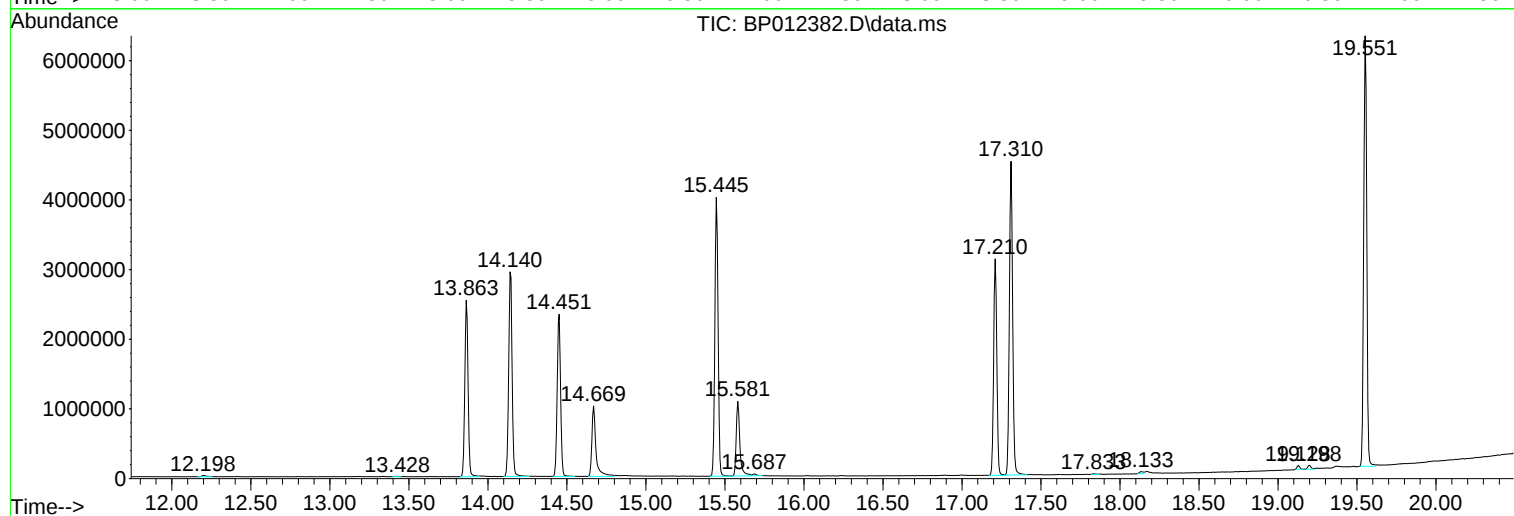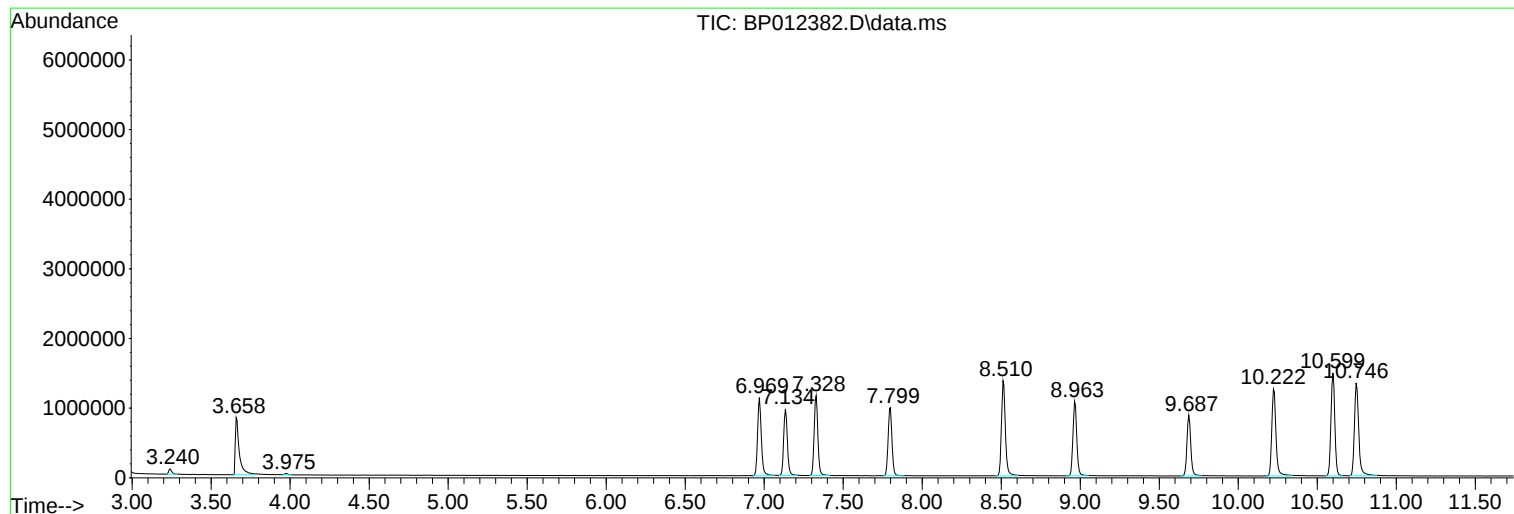

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012382.D
Acq On : 31 Oct 2022 12:04
Operator : CG/JU
Sample : PB148438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012382.D
Acq On : 31 Oct 2022 12:04
Operator : CG/JU
Sample : PB148438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc