

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012385.D
 Acq On : 31 Oct 2022 13:47
 Operator : CG/JU
 Sample : N5180-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	57	rVB	59619	96748	0.94%	0.122%
2	3.669	114	116	142	rBV	242114	473698	4.58%	0.596%
3	3.881	147	152	161	rVV	41178	74480	0.72%	0.094%
4	3.975	164	168	174	rVB2	23207	36923	0.36%	0.046%
5	4.357	230	233	240	rVB6	7259	11707	0.11%	0.015%
6	5.104	356	360	368	rVB	23265	35416	0.34%	0.045%
7	6.975	674	678	692	rVB	31368	71268	0.69%	0.090%
8	7.134	697	705	719	rBV	1048821	1727036	16.71%	2.172%
9	7.328	733	738	747	rBV	127929	229170	2.22%	0.288%
10	7.798	808	818	828	rBV	1199666	2045765	19.80%	2.573%
11	8.145	870	877	884	rBV4	13584	26665	0.26%	0.034%
12	8.516	932	940	954	rBV2	170311	348207	3.37%	0.438%
13	8.963	1007	1016	1036	rBV	1149467	2034636	19.69%	2.559%
14	9.351	1076	1082	1087	rVB	31796	51949	0.50%	0.065%
15	9.692	1133	1140	1151	rBV	77944	158424	1.53%	0.199%
16	10.228	1224	1231	1249	rBV	171090	362845	3.51%	0.456%
17	10.457	1262	1270	1279	rBV	8393	22972	0.22%	0.029%
18	10.598	1285	1294	1309	rBV	1746219	3045207	29.47%	3.829%
19	10.745	1311	1319	1342	rBV	806820	1602030	15.50%	2.015%
20	11.428	1427	1435	1444	rBV	7149	21105	0.20%	0.027%
21	11.845	1499	1506	1511	rVB2	22889	38927	0.38%	0.049%
22	12.022	1528	1536	1546	rBV4	19594	42318	0.41%	0.053%
23	12.198	1560	1566	1575	rVB2	22719	47665	0.46%	0.060%
24	12.798	1661	1668	1672	rBV9	7470	13230	0.13%	0.017%
25	13.263	1737	1747	1750	rBV6	12105	23285	0.23%	0.029%
26	13.345	1756	1761	1765	rVB5	7599	13607	0.13%	0.017%
27	13.416	1769	1773	1777	rVB6	7186	11226	0.11%	0.014%
28	13.775	1829	1834	1841	rBV	54591	92043	0.89%	0.116%
29	13.863	1842	1849	1862	rBV	3163719	4345080	42.05%	5.464%
30	14.139	1889	1896	1908	rBV	3345654	4989364	48.29%	6.274%
31	14.339	1927	1930	1935	rVB3	9220	13033	0.13%	0.016%
32	14.445	1940	1948	1963	rBV	2783959	4221608	40.86%	5.309%
33	15.204	2072	2077	2080	rBV	24137	35277	0.34%	0.044%
34	15.245	2080	2084	2088	rVV	40951	56058	0.54%	0.070%
35	15.292	2088	2092	2098	rVB4	12020	19533	0.19%	0.025%
36	15.445	2111	2118	2125	rBV	4581173	6726928	65.10%	8.459%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012385.D
 Acq On : 31 Oct 2022 13:47
 Operator : CG/JU
 Sample : N5180-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.504	2125	2128	2139	rVB	82592	155310	1.50%	0.195%
38	15.686	2155	2159	2165	rBV3	20503	33307	0.32%	0.042%
39	16.163	2235	2240	2248	rBV	15276	24767	0.24%	0.031%
40	16.233	2248	2252	2257	rVB7	7254	11021	0.11%	0.014%
41	16.957	2372	2375	2378	rBV5	12061	15681	0.15%	0.020%
42	17.210	2411	2418	2428	rBV	3589534	5136947	49.71%	6.460%
43	17.310	2428	2435	2448	rBV	5708465	8133115	78.71%	10.227%
44	17.704	2499	2502	2507	rBV7	11146	13178	0.13%	0.017%
45	18.145	2572	2577	2578	rBV4	22199	37690	0.36%	0.047%
46	19.127	2740	2744	2750	rBV3	71141	108470	1.05%	0.136%
47	19.198	2752	2756	2761	rVV	66837	96807	0.94%	0.122%
48	19.551	2810	2816	2830	rBV	7191065	9854447	95.37%	12.392%
49	19.810	2856	2860	2866	rBV	65255	121119	1.17%	0.152%
50	21.304	3109	3114	3121	rBV	4938667	6219918	60.19%	7.822%
51	23.545	3488	3495	3509	rVB2	5130243	10332993	100.00%	12.994%
52	23.698	3514	3521	3530	rVB2	3013720	6062980	58.68%	7.624%




Sum of corrected areas: 79523183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012385.D
Acq On : 31 Oct 2022 13:47
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

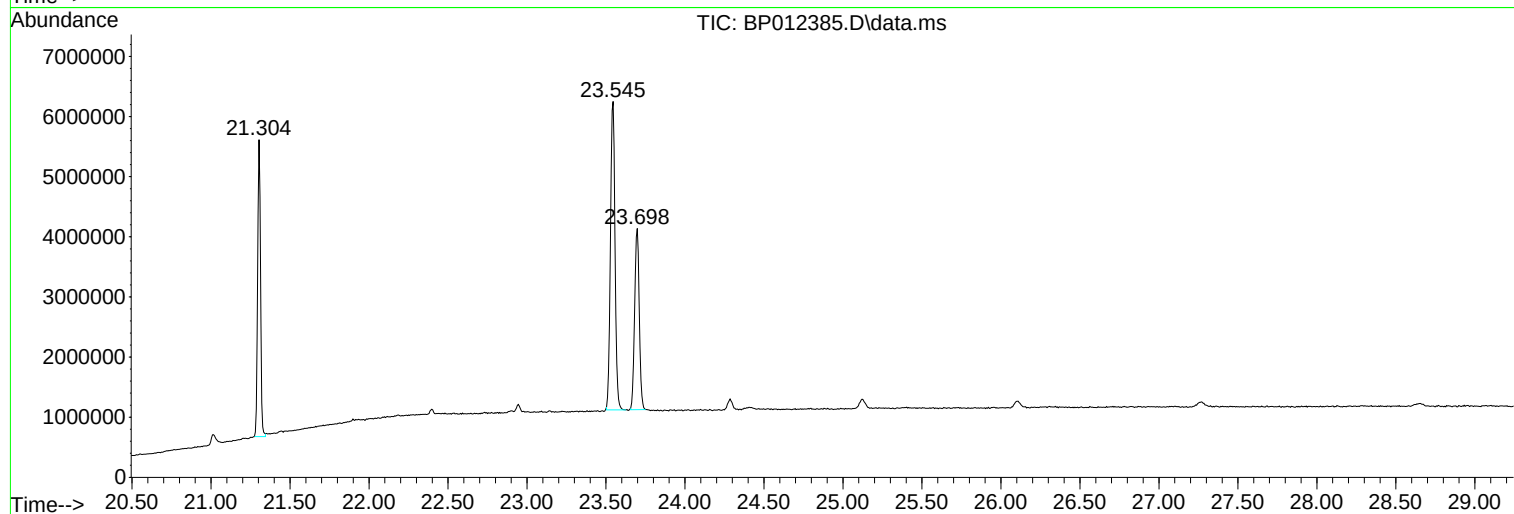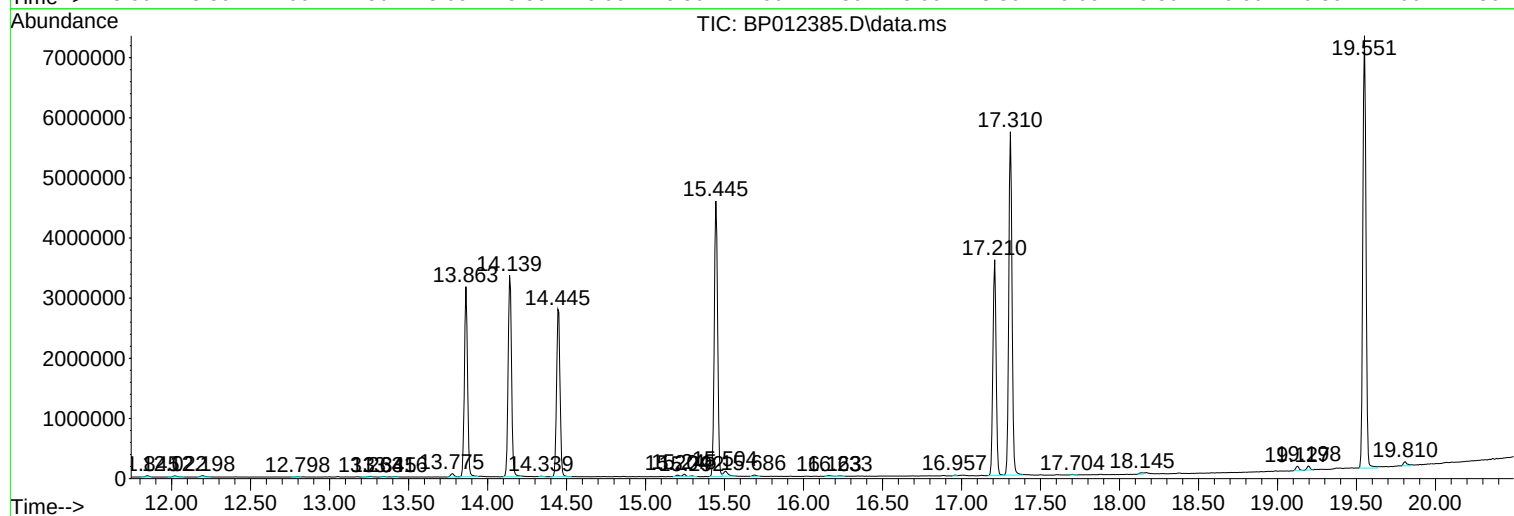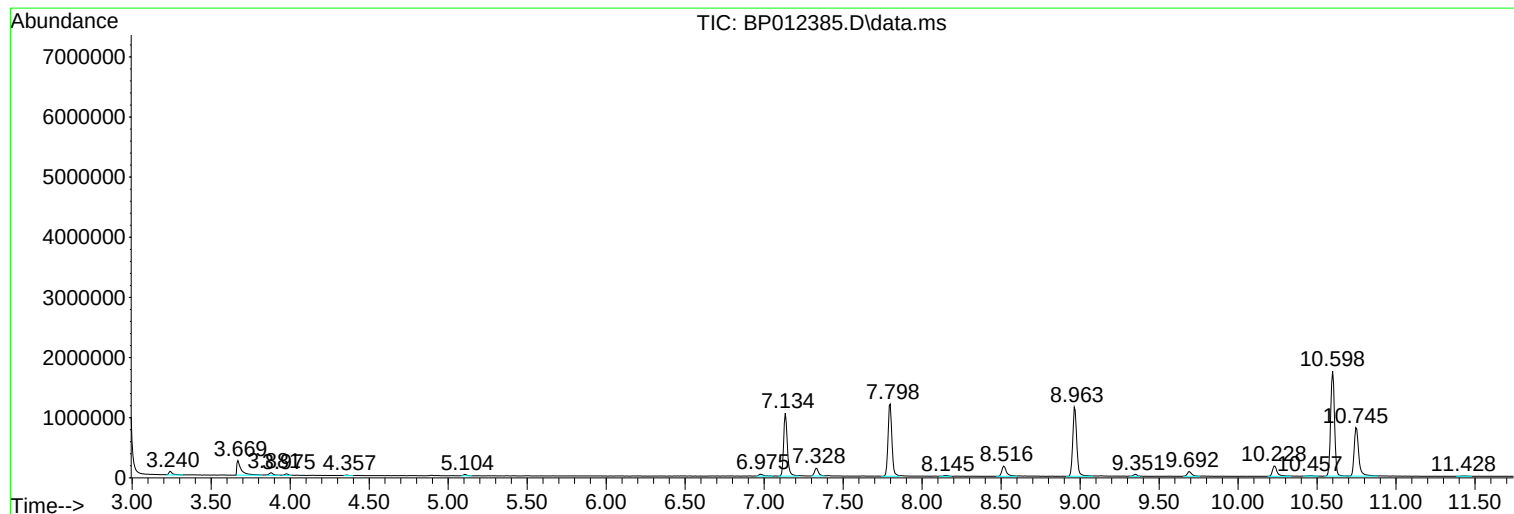

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012385.D
Acq On : 31 Oct 2022 13:47
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012385.D
Acq On : 31 Oct 2022 13:47
Operator : CG/JU
Sample : N5180-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc