

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012387.D
 Acq On : 31 Oct 2022 15:31
 Operator : CG/JU
 Sample : N5180-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	56	rVB	47409	82351	0.75%	0.097%
2	3.670	114	116	139	rBV	174599	357431	3.26%	0.419%
3	3.881	146	152	164	rVB	32427	56641	0.52%	0.066%
4	3.975	164	168	174	rVB	16064	21461	0.20%	0.025%
5	4.917	320	328	335	rBV2	24023	47348	0.43%	0.056%
6	6.969	671	677	691	rVV	176004	331287	3.02%	0.389%
7	7.134	697	705	720	rBV	932270	1519091	13.84%	1.782%
8	7.328	731	738	749	rBV	776592	1270157	11.57%	1.490%
9	7.799	811	818	829	rBV	833401	1397227	12.73%	1.639%
10	8.516	933	940	955	rBV	606349	1069425	9.74%	1.255%
11	8.963	1007	1016	1032	rBV	1057170	1830296	16.68%	2.147%
12	9.222	1035	1060	1077	rBV	2220493	9844768	89.70%	11.551%
13	9.352	1079	1082	1092	rVB	42804	90778	0.83%	0.107%
14	9.687	1132	1139	1152	rBV	770801	1291591	11.77%	1.515%
15	10.046	1193	1200	1203	rBV7	10692	25517	0.23%	0.030%
16	10.222	1223	1230	1247	rBV	1091715	1991533	18.15%	2.337%
17	10.599	1286	1294	1307	rVB	1284733	2156380	19.65%	2.530%
18	10.746	1312	1319	1335	rBV	738514	1387348	12.64%	1.628%
19	10.910	1343	1347	1361	rVB	11534	38143	0.35%	0.045%
20	11.057	1364	1372	1383	rVB10	17657	53931	0.49%	0.063%
21	11.475	1432	1443	1454	rVV6	21137	90117	0.82%	0.106%
22	11.610	1464	1466	1473	rVB7	8583	15162	0.14%	0.018%
23	11.710	1479	1483	1487	rBV6	7311	12341	0.11%	0.014%
24	11.846	1502	1506	1514	rVB2	18525	35232	0.32%	0.041%
25	12.193	1560	1565	1570	rVB	23412	38818	0.35%	0.046%
26	12.352	1586	1592	1598	rBV5	15297	33874	0.31%	0.040%
27	13.057	1706	1712	1718	rBV9	9232	16306	0.15%	0.019%
28	13.340	1754	1760	1769	rBV	127417	210754	1.92%	0.247%
29	13.863	1841	1849	1855	rBV	2640409	3685878	33.58%	4.325%
30	13.910	1855	1857	1864	rVB	39629	52800	0.48%	0.062%
31	14.140	1888	1896	1907	rBV	3012685	4542474	41.39%	5.330%
32	14.293	1917	1922	1923	rBV	36804	45064	0.41%	0.053%
33	14.451	1942	1949	1960	rVB	2015427	3014749	27.47%	3.537%
34	14.687	1983	1989	2005	rBV2	72744	200770	1.83%	0.236%
35	14.810	2005	2010	2014	rBV6	12193	24850	0.23%	0.029%
36	15.204	2073	2077	2080	rBV2	9691	12550	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012387.D
 Acq On : 31 Oct 2022 15:31
 Operator : CG/JU
 Sample : N5180-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.245	2080	2084	2088	rBV	25630	31220	0.28%	0.037%
38	15.445	2111	2118	2124	rBV	4158614	6087364	55.46%	7.142%
39	15.498	2124	2127	2135	rVV	86121	141333	1.29%	0.166%
40	15.575	2135	2140	2154	rVV3	83761	199517	1.82%	0.234%
41	15.687	2155	2159	2166	rVB2	21354	35416	0.32%	0.042%
42	16.028	2213	2217	2223	rVB8	18163	25970	0.24%	0.030%
43	16.234	2247	2252	2257	rVB7	8895	16468	0.15%	0.019%
44	17.210	2411	2418	2428	rBV	2737487	3780468	34.45%	4.436%
45	17.310	2429	2435	2450	rVV2	5139738	7306731	66.57%	8.573%
46	17.516	2466	2470	2477	rVB5	18307	36765	0.33%	0.043%
47	17.875	2528	2531	2538	rBV6	16291	21943	0.20%	0.026%
48	18.139	2572	2576	2577	rBV3	26862	35181	0.32%	0.041%
49	19.128	2740	2744	2750	rBV2	68302	101733	0.93%	0.119%
50	19.198	2752	2756	2759	rBV	66713	98981	0.90%	0.116%
51	19.551	2810	2816	2829	rBV	6926097	9353694	85.23%	10.975%
52	21.304	3110	3114	3122	rVB	3925878	4855421	44.24%	5.697%
53	23.545	3488	3495	3510	rVB2	5121800	10975267	100.00%	12.877%
54	23.698	3515	3521	3538	rVB2	2665097	5232631	47.68%	6.139%




Sum of corrected areas: 85230546

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012387\
Data File : BP012387.D
Acq On : 31 Oct 2022 15:31
Operator : CG/JU
Sample : N5180-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

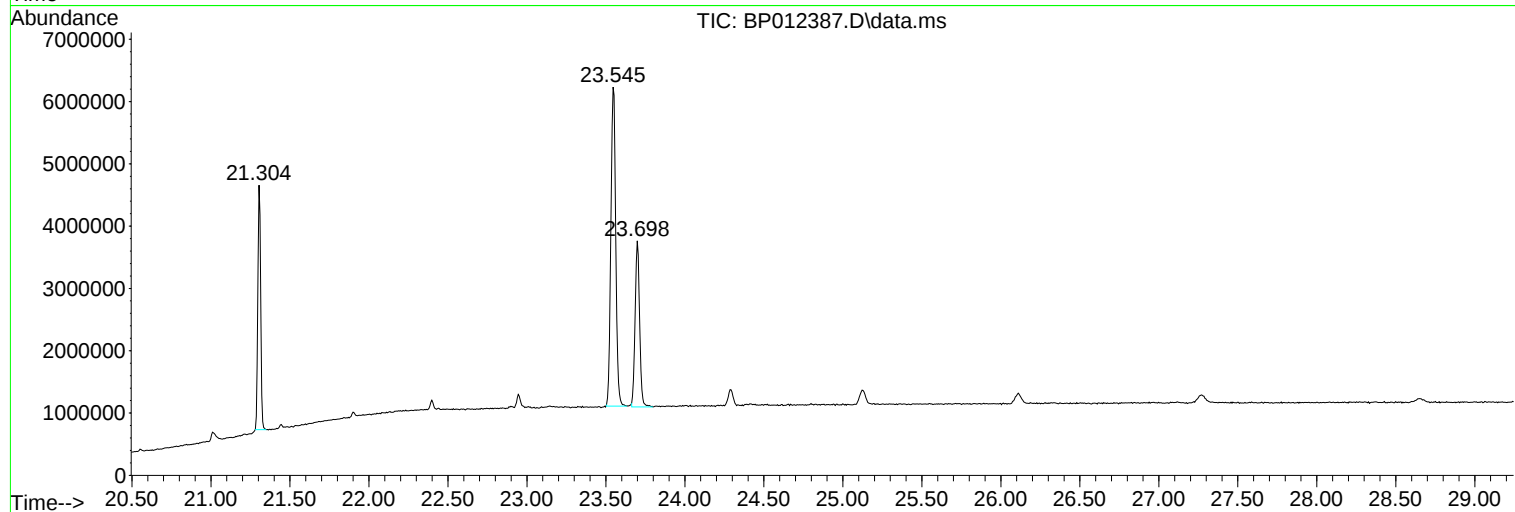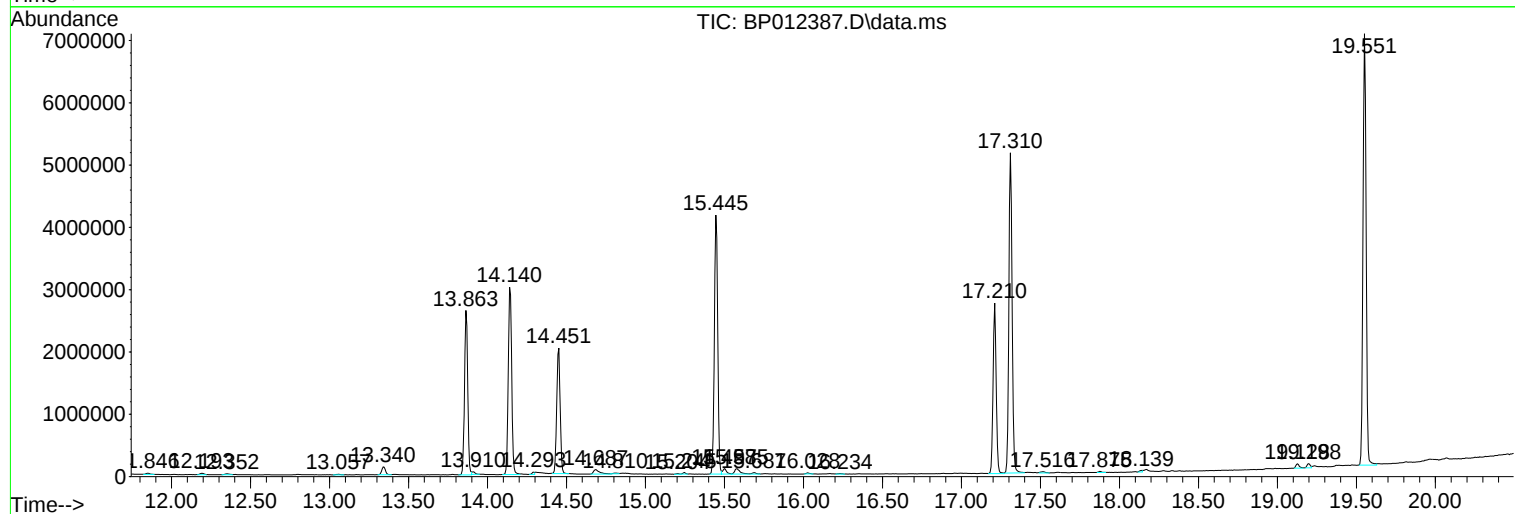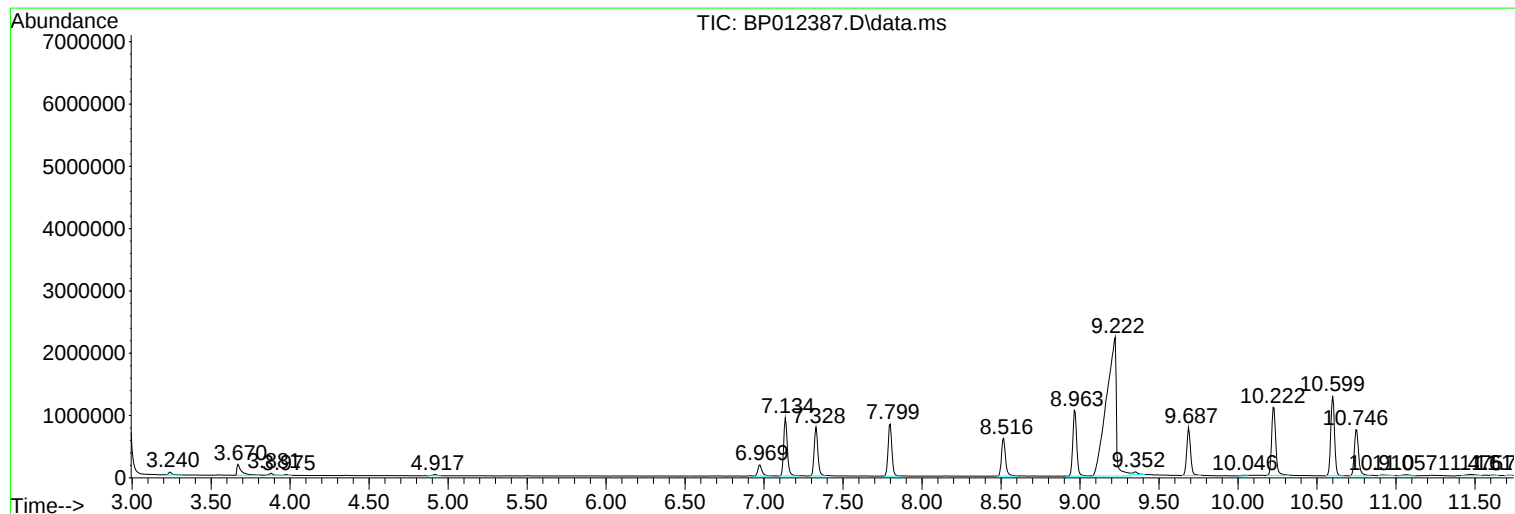

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012387.D
Acq On : 31 Oct 2022 15:31
Operator : CG/JU
Sample : N5180-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.222	91.31 ng/ul	9844770	Naphthalene-d8	10.599

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	90
2			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	90
3			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
4			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	86
5			Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	83

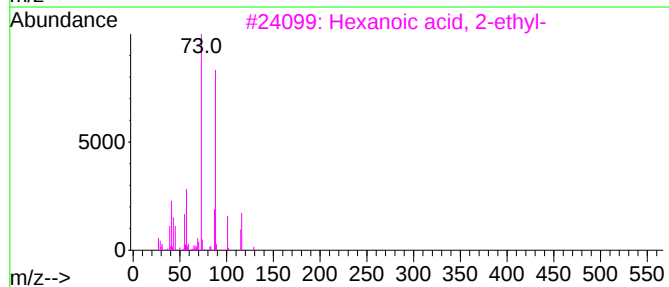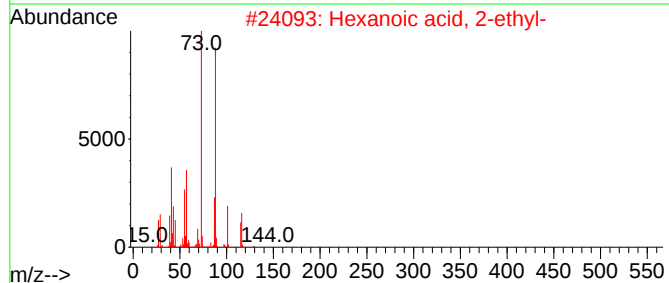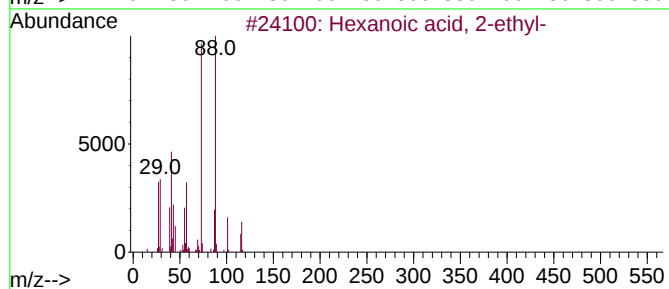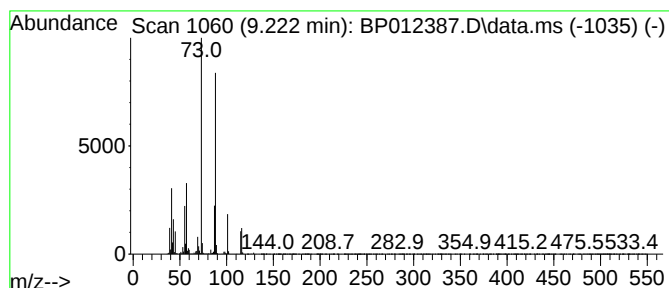

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012387.D
Acq On : 31 Oct 2022 15:31
Operator : CG/JU
Sample : N5180-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanoic acid, ...	9.222	91.3	ng/ul	9844770	2	10.599	2156380	20.0