

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012391.D
 Acq On : 31 Oct 2022 17:49
 Operator : CG/JU
 Sample : PB148509BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK509

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	38	43	50	rBV	66697	94646	0.94%	0.111%
2	3.658	112	114	135	rBV	699408	1278108	12.65%	1.502%
3	3.975	164	168	178	rVB2	20225	37527	0.37%	0.044%
4	6.969	670	677	697	rBV	1014318	1712888	16.95%	2.013%
5	7.134	697	705	719	rBV	891339	1435601	14.21%	1.687%
6	7.328	731	738	753	rBV	1009721	1690485	16.73%	1.987%
7	7.793	810	817	833	rBV	905152	1506096	14.91%	1.770%
8	8.510	931	939	960	rBV	1272661	2201644	21.79%	2.587%
9	8.963	1008	1016	1030	rBV	1017263	1702810	16.85%	2.001%
10	9.687	1132	1139	1155	rBV	804435	1371873	13.58%	1.612%
11	10.222	1223	1230	1261	rBV	1182354	2172246	21.50%	2.553%
12	10.599	1286	1294	1307	rBV	1362458	2309392	22.86%	2.714%
13	10.746	1312	1319	1340	rBV	1252302	2377010	23.53%	2.793%
14	12.204	1561	1567	1578	rBV2	17329	41162	0.41%	0.048%
15	13.340	1756	1760	1765	rBV7	6940	15549	0.15%	0.018%
16	13.863	1842	1849	1862	rBV	2720422	3905518	38.66%	4.590%
17	14.140	1889	1896	1915	rBV	3177513	4755991	47.07%	5.589%
18	14.445	1941	1948	1960	rBV	2370853	3624764	35.88%	4.260%
19	14.669	1979	1986	2011	rBV	961878	1838370	18.20%	2.160%
20	15.445	2111	2118	2131	rBV	4462777	6202717	61.39%	7.289%
21	15.581	2135	2141	2155	rBV	1006034	1583612	15.67%	1.861%
22	15.687	2156	2159	2166	rVB2	25951	44909	0.44%	0.053%
23	16.239	2246	2253	2256	rBV8	7765	14349	0.14%	0.017%
24	16.886	2359	2363	2367	rBV6	6147	11090	0.11%	0.013%
25	17.210	2411	2418	2428	rBV	3269139	4593195	45.46%	5.398%
26	17.310	2428	2435	2449	rVV	4967753	7055767	69.84%	8.292%
27	19.128	2740	2744	2749	rBV2	64583	90207	0.89%	0.106%
28	19.198	2752	2756	2761	rVV	62032	91330	0.90%	0.107%
29	19.551	2810	2816	2825	rBV	6734763	8979494	88.88%	10.553%
30	21.304	3109	3114	3122	rBV	4881721	6057557	59.96%	7.119%
31	23.539	3488	3494	3505	rVB2	5141653	10103182	100.00%	11.873%
32	23.698	3514	3521	3532	rVB2	3045014	6192576	61.29%	7.278%




Sum of corrected areas: 85091665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012391.D
Acq On : 31 Oct 2022 17:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

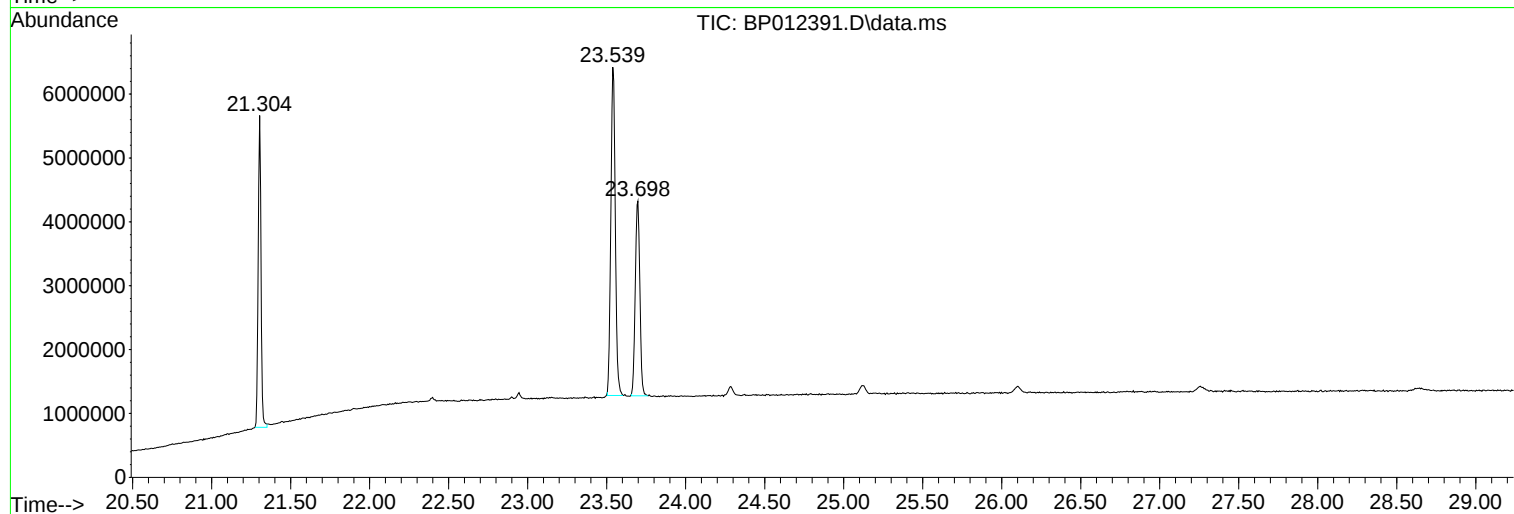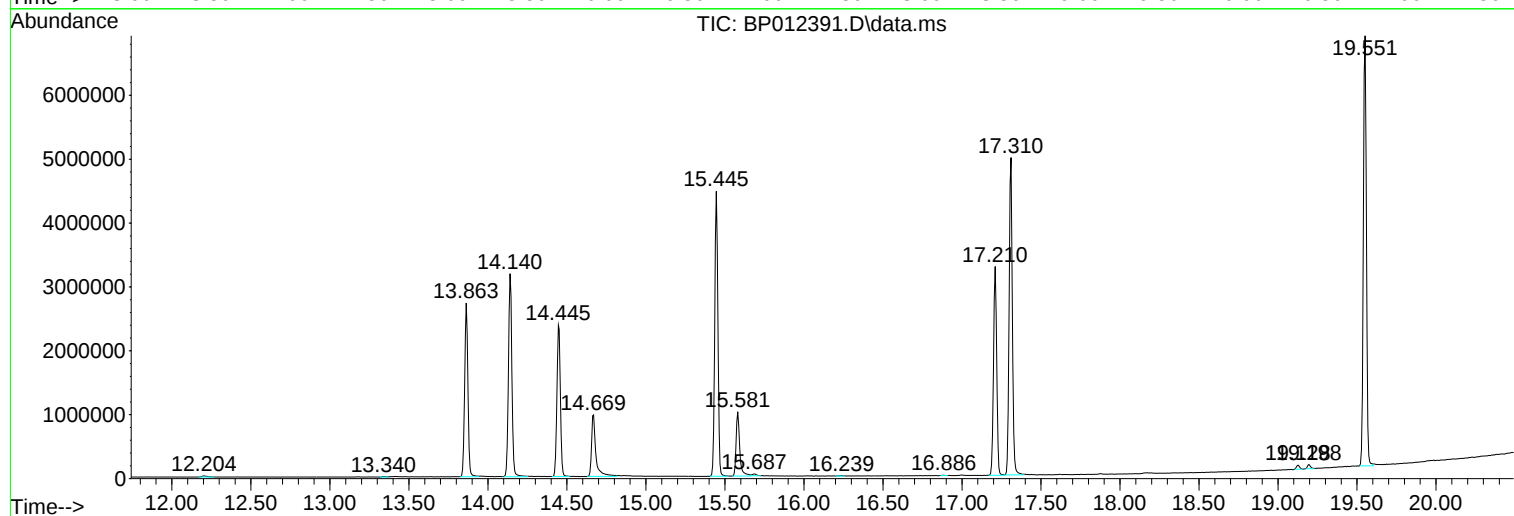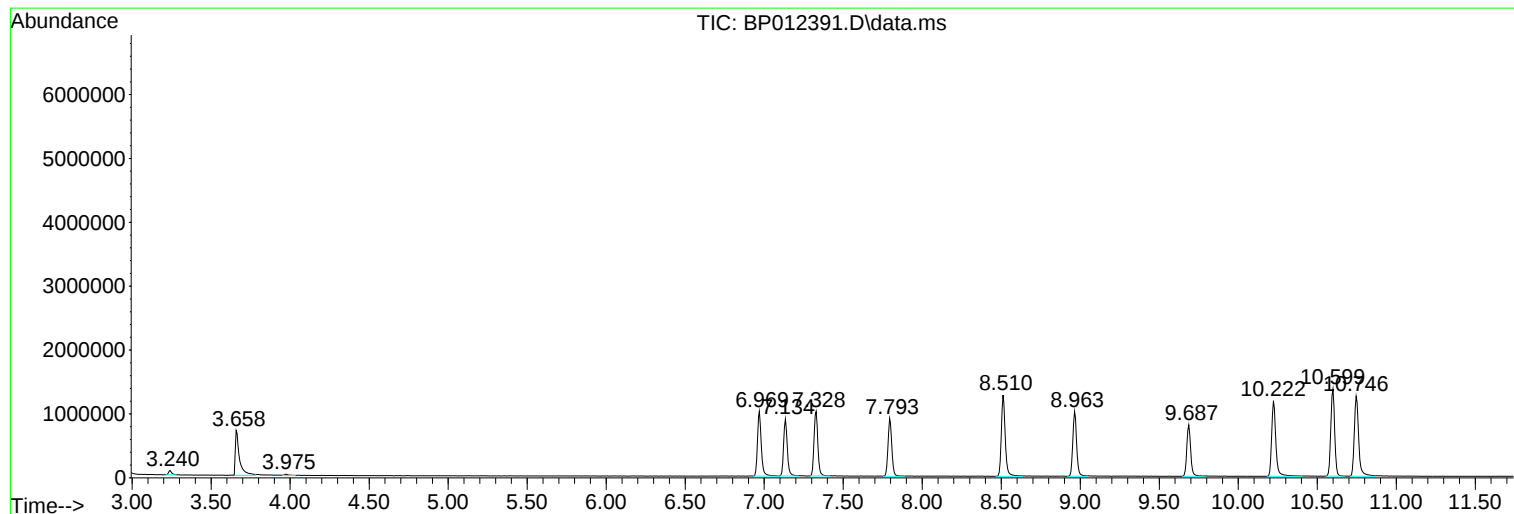

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012391.D
Acq On : 31 Oct 2022 17:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012391.D
Acq On : 31 Oct 2022 17:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc