

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012392.D
 Acq On : 31 Oct 2022 18:24
 Operator : CG/JU
 Sample : PB148473BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK473

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	53	rVB	93630	130140	1.30%	0.140%
2	3.663	113	115	134	rBV	457571	819395	8.22%	0.883%
3	3.975	164	168	176	rVB	25599	38668	0.39%	0.042%
4	5.105	357	360	366	rVB2	13670	21416	0.21%	0.023%
5	6.969	670	677	692	rBV	1321804	2185344	21.91%	2.354%
6	7.134	698	705	721	rBV	1156983	1850125	18.55%	1.993%
7	7.328	731	738	752	rBV	1322251	2175585	21.82%	2.343%
8	7.793	810	817	834	rBV	1249073	2031481	20.37%	2.188%
9	8.151	873	878	884	rVB5	9352	17749	0.18%	0.019%
10	8.510	932	939	963	rBV	1654485	2777739	27.85%	2.992%
11	8.963	1008	1016	1032	rBV	1279969	2153199	21.59%	2.319%
12	9.687	1131	1139	1154	rBV	1013469	1745519	17.50%	1.880%
13	10.222	1222	1230	1249	rBV	1536488	2736860	27.44%	2.948%
14	10.598	1286	1294	1306	rBV	1801381	3055242	30.64%	3.291%
15	10.745	1312	1319	1343	rBV	781715	1538437	15.43%	1.657%
16	12.198	1560	1566	1578	rBV2	17943	46899	0.47%	0.051%
17	13.339	1755	1760	1765	rBV6	8182	12456	0.12%	0.013%
18	13.422	1769	1774	1782	rVB5	6342	10302	0.10%	0.011%
19	13.863	1840	1849	1872	rBV	2965929	4265127	42.77%	4.594%
20	14.139	1888	1896	1916	rBV	3471457	5156979	51.71%	5.554%
21	14.445	1941	1948	1959	rBV	2862080	4188898	42.00%	4.512%
22	14.663	1979	1985	2009	rBV	1237374	2205383	22.11%	2.375%
23	14.857	2016	2018	2026	rVB9	6363	11140	0.11%	0.012%
24	15.445	2110	2118	2128	rBV	4504312	6604879	66.23%	7.114%
25	15.581	2135	2141	2155	rBV	1292141	2012250	20.18%	2.167%
26	15.686	2155	2159	2170	rVB2	29858	59229	0.59%	0.064%
27	16.998	2378	2382	2389	rVB4	6793	11606	0.12%	0.012%
28	17.210	2411	2418	2428	rBV	3658811	5193425	52.08%	5.593%
29	17.310	2428	2435	2453	rVV2	5185022	7542258	75.63%	8.123%
30	18.145	2572	2577	2579	rBV6	15143	27979	0.28%	0.030%
31	19.127	2740	2744	2749	rBV2	63768	86487	0.87%	0.093%
32	19.198	2752	2756	2761	rBV	60404	89862	0.90%	0.097%
33	19.551	2810	2816	2831	rBV	6980667	9363836	93.90%	10.085%
34	21.304	3109	3114	3121	rBV	5307338	6439874	64.58%	6.936%
35	23.539	3488	3494	3507	rVB2	4890187	9972660	100.00%	10.741%
36	23.698	3514	3521	3533	rVB2	3063922	6270669	62.88%	6.754%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012392.D
Acq On : 31 Oct 2022 18:24
Operator : CG/JU
Sample : PB148473BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK473

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 92849097

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012392.D
Acq On : 31 Oct 2022 18:24
Operator : CG/JU
Sample : PB148473BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK473

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

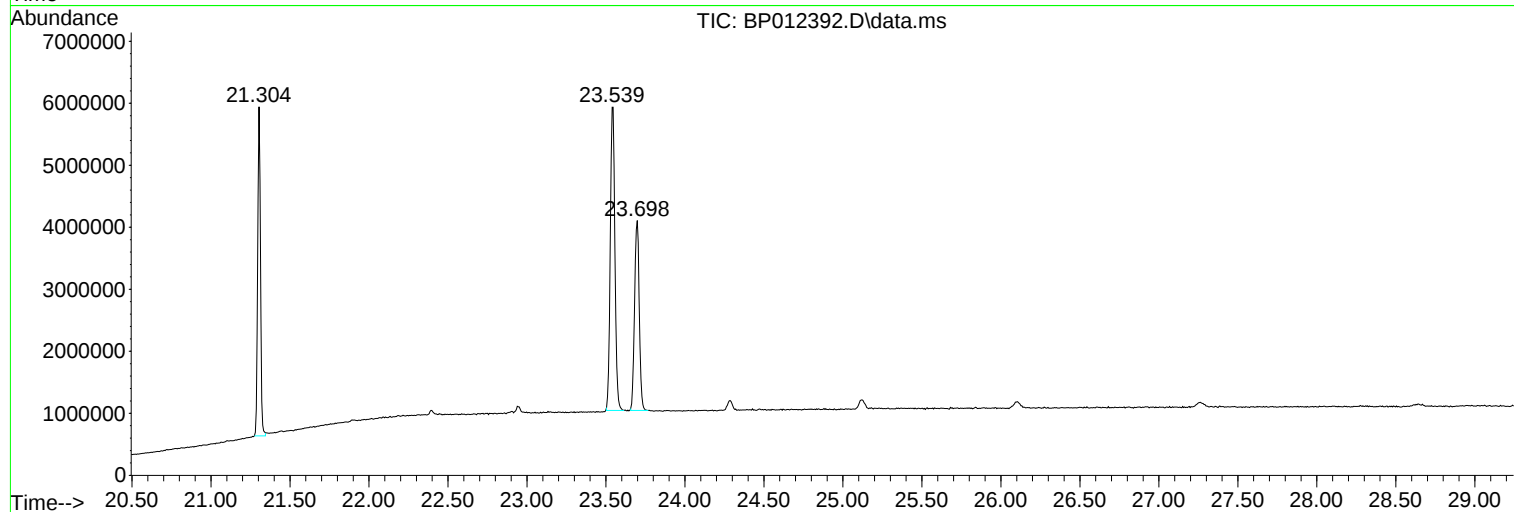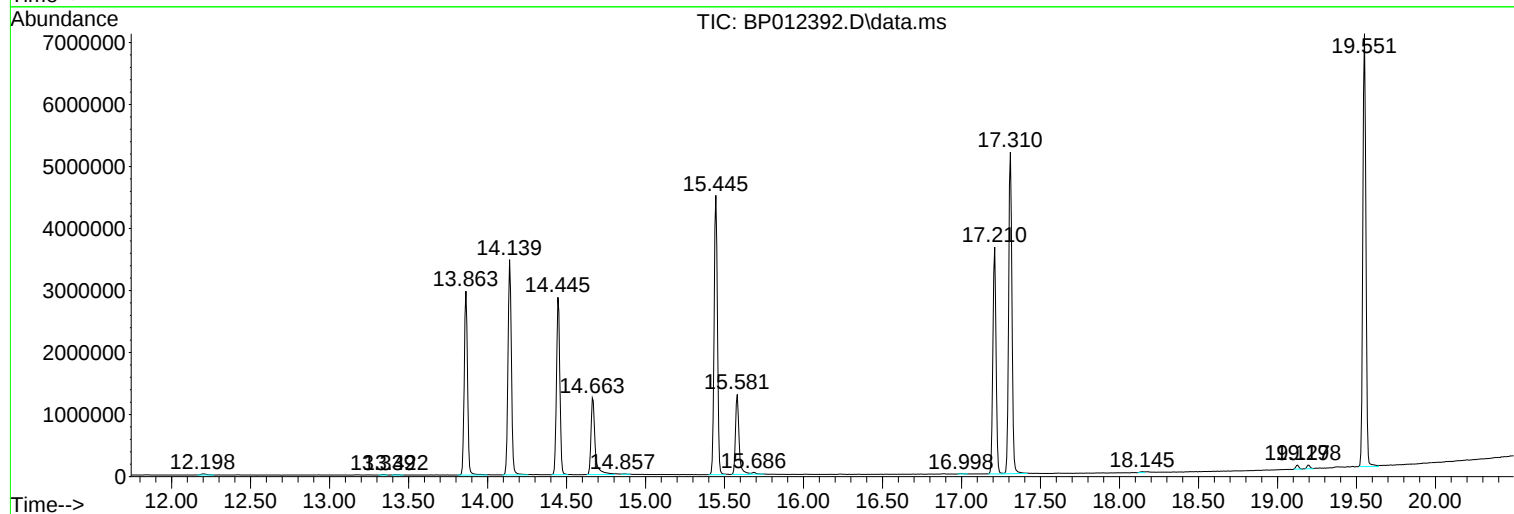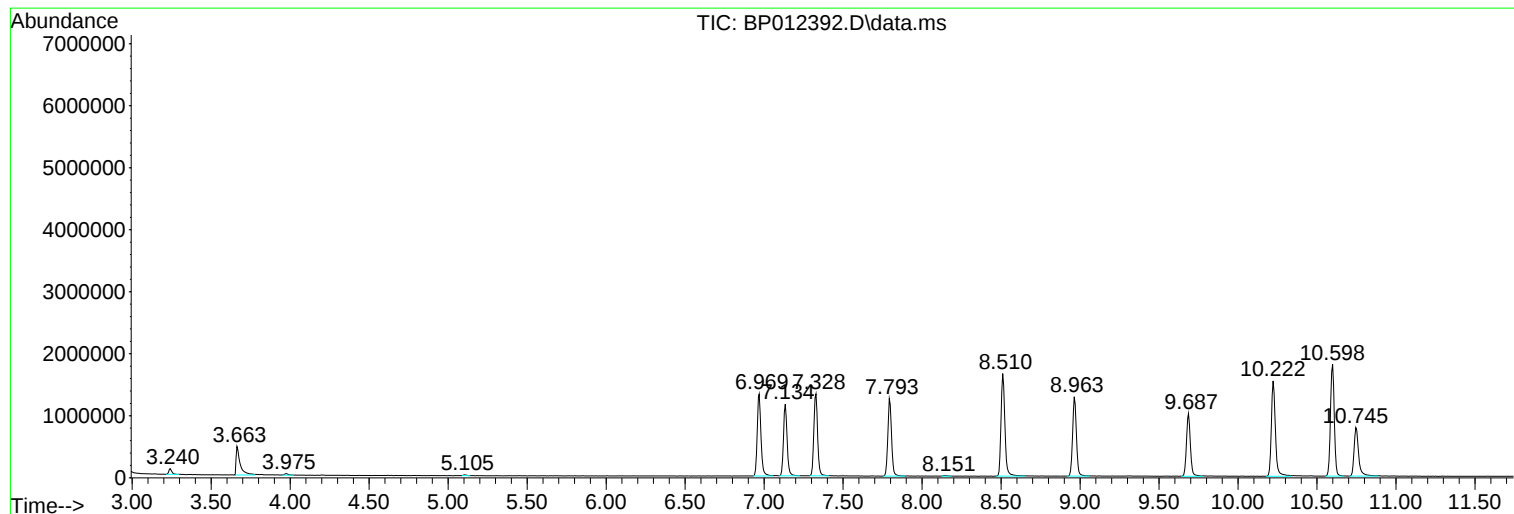

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012392.D
Acq On : 31 Oct 2022 18:24
Operator : CG/JU
Sample : PB148473BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK473

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012392.D
Acq On : 31 Oct 2022 18:24
Operator : CG/JU
Sample : PB148473BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK473

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc