

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012394.D
 Acq On : 31 Oct 2022 19:33
 Operator : CG/JU
 Sample : N5194-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	54	rVB	51037	78263	0.83%	0.096%
2	3.669	114	116	129	rBV	188523	353637	3.77%	0.432%
3	3.875	146	151	159	rVB	34791	59819	0.64%	0.073%
4	3.975	164	168	174	rBV	20679	30058	0.32%	0.037%
5	4.916	320	328	335	rBV2	35938	64522	0.69%	0.079%
6	6.969	670	677	691	rBV	191892	376184	4.01%	0.459%
7	7.134	698	705	721	rBV	994107	1656597	17.66%	2.022%
8	7.328	730	738	750	rBV	815231	1365552	14.55%	1.667%
9	7.793	808	817	827	rBV	1099840	1783581	19.01%	2.177%
10	8.510	932	939	954	rBV	609730	1087525	11.59%	1.327%
11	8.963	1008	1016	1037	rBV	1158544	1967640	20.97%	2.401%
12	9.128	1037	1044	1045	rBV7	6111	10355	0.11%	0.013%
13	9.346	1074	1081	1090	rVB	25838	48296	0.51%	0.059%
14	9.687	1131	1139	1149	rBV	804021	1411630	15.05%	1.723%
15	10.222	1222	1230	1248	rBV	1209229	2179043	23.23%	2.659%
16	10.410	1255	1262	1268	rBV7	9159	25297	0.27%	0.031%
17	10.598	1286	1294	1308	rBV	1568246	2749020	29.30%	3.355%
18	10.745	1312	1319	1339	rBV	1027002	1888102	20.12%	2.304%
19	12.192	1559	1565	1574	rVB	23170	42758	0.46%	0.052%
20	12.792	1664	1667	1675	rBV8	6956	15079	0.16%	0.018%
21	13.051	1705	1711	1713	rBV5	8822	11871	0.13%	0.014%
22	13.257	1740	1746	1750	rBV3	13616	18555	0.20%	0.023%
23	13.339	1755	1760	1767	rBV5	13486	22416	0.24%	0.027%
24	13.410	1767	1772	1780	rVB6	9549	15950	0.17%	0.019%
25	13.639	1805	1811	1816	rBV6	5178	10327	0.11%	0.013%
26	13.863	1842	1849	1861	rBV	2766727	3908162	41.66%	4.770%
27	14.139	1884	1896	1911	rBV2	3302290	4897258	52.20%	5.977%
28	14.334	1922	1929	1932	rBV4	13344	20570	0.22%	0.025%
29	14.445	1941	1948	1962	rBV	2579347	3828647	40.81%	4.673%
30	14.616	1971	1977	1979	rBV6	6372	9630	0.10%	0.012%
31	14.675	1982	1987	1999	rBV	98752	242972	2.59%	0.297%
32	15.245	2080	2084	2086	rBV	8060	9830	0.10%	0.012%
33	15.445	2111	2118	2125	rBV	4327376	6259749	66.72%	7.640%
34	15.498	2125	2127	2134	rVV6	27631	40075	0.43%	0.049%
35	15.575	2134	2140	2154	rVV	1105161	1640351	17.48%	2.002%
36	15.686	2154	2159	2166	rVB4	24817	49910	0.53%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012394.D
 Acq On : 31 Oct 2022 19:33
 Operator : CG/JU
 Sample : N5194-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB901

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.816	2179	2181	2185	rVB5	8566	9434	0.10%	0.012%
38	16.157	2236	2239	2247	rBV6	18479	35697	0.38%	0.044%
39	16.228	2249	2251	2256	rVB6	12516	14795	0.16%	0.018%
40	16.969	2373	2377	2380	rBV5	25155	36531	0.39%	0.045%
41	17.080	2393	2396	2400	rBV5	8821	11608	0.12%	0.014%
42	17.122	2400	2403	2407	rBV5	19392	24168	0.26%	0.029%
43	17.204	2411	2417	2428	rBV	3199575	4827782	51.46%	5.892%
44	17.304	2428	2434	2447	rBV2	4474025	6892812	73.47%	8.412%
45	17.569	2476	2479	2482	rBV5	10340	14996	0.16%	0.018%
46	17.875	2529	2531	2535	rVB4	15125	15058	0.16%	0.018%
47	18.098	2564	2569	2578	rBV	239430	424975	4.53%	0.519%
48	19.121	2740	2743	2748	rVB2	64546	82830	0.88%	0.101%
49	19.192	2751	2755	2758	rBV	77785	116061	1.24%	0.142%
50	19.333	2775	2779	2788	rBV	167993	292385	3.12%	0.357%
51	19.551	2810	2816	2830	rBV	6471641	8833508	94.15%	10.781%
52	21.010	3061	3064	3073	rBV2	273532	496365	5.29%	0.606%
53	21.304	3109	3114	3123	rBV	4837491	6176840	65.84%	7.539%
54	23.539	3487	3494	3507	rVB2	4691591	9382168	100.00%	11.451%
55	23.692	3514	3520	3530	rVB2	3005567	6068382	64.68%	7.406%




Sum of corrected areas: 81935626

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012394.D
Acq On : 31 Oct 2022 19:33
Operator : CG/JU
Sample : N5194-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

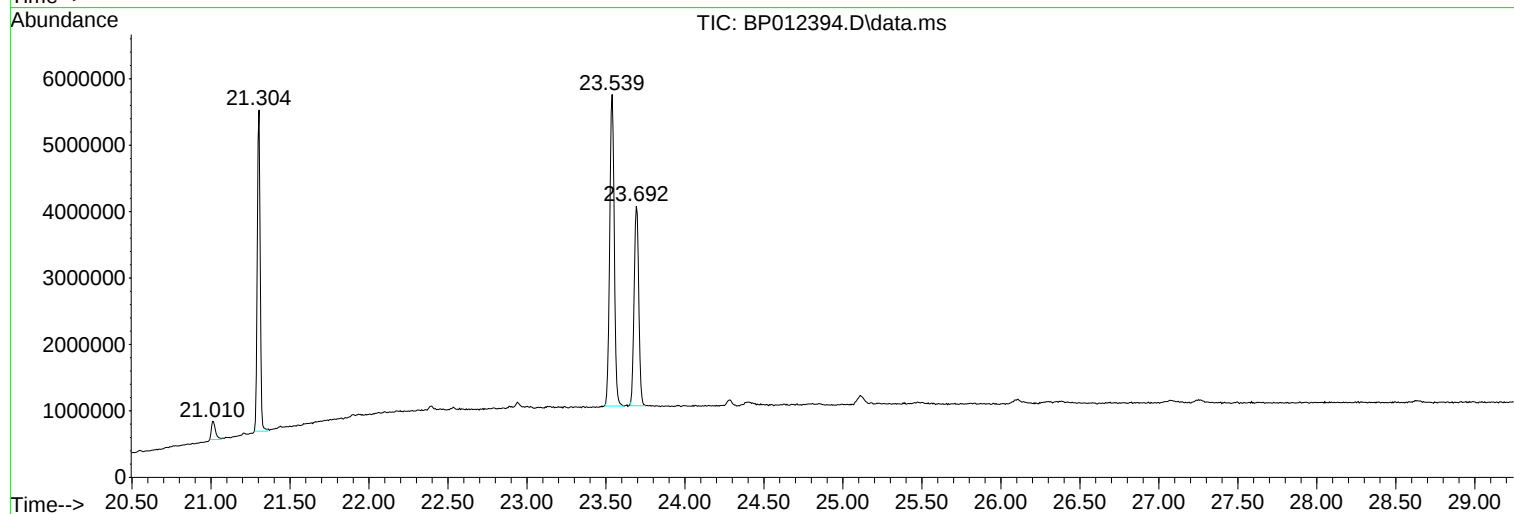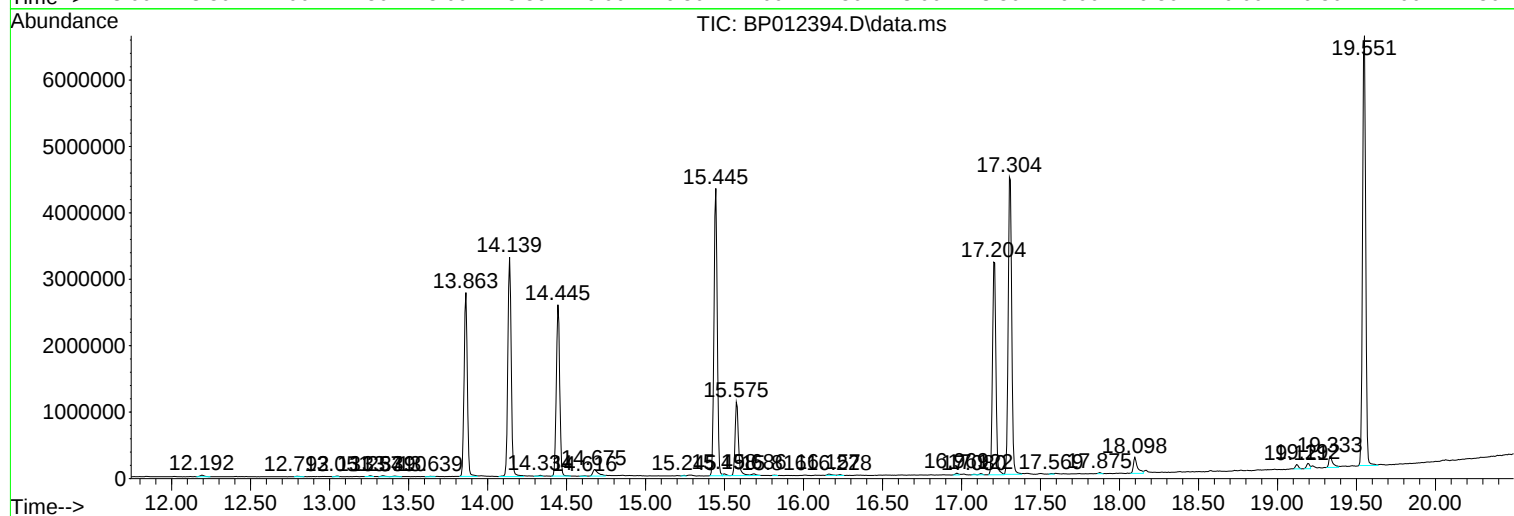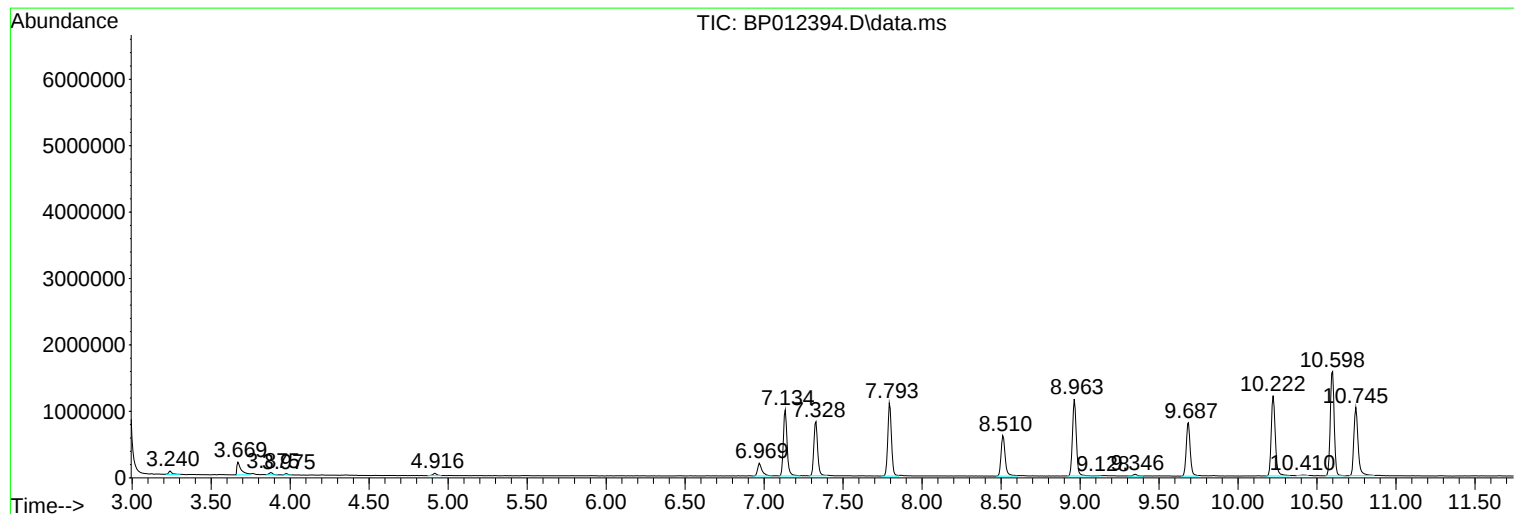

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012394.D
Acq On : 31 Oct 2022 19:33
Operator : CG/JU
Sample : N5194-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012394.D
Acq On : 31 Oct 2022 19:33
Operator : CG/JU
Sample : N5194-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB901

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc