

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012396.D
 Acq On : 31 Oct 2022 20:41
 Operator : CG/JU
 Sample : N5194-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	53	rVB	54206	84052	0.81%	0.095%
2	3.675	115	117	136	rBV	112534	248045	2.39%	0.279%
3	3.881	146	152	159	rVB	37160	64721	0.62%	0.073%
4	3.975	163	168	174	rBV	22366	36567	0.35%	0.041%
5	4.346	228	231	235	rBV5	8700	11390	0.11%	0.013%
6	4.916	321	328	337	rBV2	38991	68090	0.66%	0.077%
7	6.969	668	677	688	rBV	218104	407883	3.93%	0.459%
8	7.134	698	705	719	rBV	1022990	1735524	16.72%	1.955%
9	7.328	731	738	748	rBV	898332	1498270	14.43%	1.688%
10	7.793	807	817	832	rBV	1165886	1955591	18.84%	2.203%
11	8.057	855	862	873	rBV2	31490	68298	0.66%	0.077%
12	8.510	932	939	958	rBV	701105	1199235	11.55%	1.351%
13	8.963	1007	1016	1032	rBV	1238828	2066532	19.91%	2.328%
14	9.122	1037	1043	1049	rVB5	15863	26803	0.26%	0.030%
15	9.540	1108	1114	1129	rBV2	32562	66304	0.64%	0.075%
16	9.687	1131	1139	1156	rBV	870249	1553001	14.96%	1.749%
17	10.222	1221	1230	1250	rBV	1302564	2324476	22.39%	2.618%
18	10.593	1285	1293	1310	rBV	1751535	3013850	29.03%	3.395%
19	10.746	1310	1319	1338	rBV	1181658	2241959	21.60%	2.525%
20	12.198	1559	1566	1572	rBV	21929	44440	0.43%	0.050%
21	13.340	1755	1760	1766	rBV6	8540	13476	0.13%	0.015%
22	13.410	1769	1772	1777	rBV6	7194	11916	0.11%	0.013%
23	13.781	1828	1835	1841	rBV6	5489	13042	0.13%	0.015%
24	13.863	1841	1849	1862	rBV	2966075	4244764	40.89%	4.781%
25	14.139	1887	1896	1913	rBV	3414045	5172527	49.83%	5.826%
26	14.445	1940	1948	1960	rBV	2827489	4270684	41.14%	4.811%
27	14.675	1980	1987	2008	rBV	111746	317202	3.06%	0.357%
28	14.886	2015	2023	2026	rBV6	22166	39990	0.39%	0.045%
29	15.445	2111	2118	2129	rBV	4567794	6807364	65.58%	7.668%
30	15.575	2134	2140	2155	rVV	1236818	1915650	18.45%	2.158%
31	15.686	2155	2159	2168	rVB2	26347	47867	0.46%	0.054%
32	15.816	2178	2181	2185	rVB6	8308	10836	0.10%	0.012%
33	16.233	2246	2252	2258	rVB2	12008	22350	0.22%	0.025%
34	16.669	2320	2326	2328	rBV6	6402	13765	0.13%	0.016%
35	16.886	2359	2363	2370	rBV9	6168	10760	0.10%	0.012%
36	16.992	2378	2381	2387	rVB	7662	12508	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012396.D
 Acq On : 31 Oct 2022 20:41
 Operator : CG/JU
 Sample : N5194-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.204	2411	2417	2428	rBV	3559680	5189890	50.00%	5.846%
38	17.310	2428	2435	2450	rVV	5297366	7862455	75.74%	8.856%
39	17.875	2526	2531	2539	rVB4	45196	64694	0.62%	0.073%
40	17.992	2548	2551	2554	rBV5	8850	11212	0.11%	0.013%
41	18.098	2565	2569	2579	rBV	191461	365908	3.52%	0.412%
42	18.916	2705	2708	2712	rBV3	26521	38861	0.37%	0.044%
43	19.127	2740	2744	2749	rBV3	82131	115772	1.12%	0.130%
44	19.192	2751	2755	2759	rBV	71968	128396	1.24%	0.145%
45	19.333	2775	2779	2793	rBV2	167053	389460	3.75%	0.439%
46	19.551	2809	2816	2830	rBV	6981098	9803509	94.44%	11.043%
47	21.304	3109	3114	3120	rBV	4895826	6314286	60.83%	7.112%
48	23.539	3487	3494	3505	rVB	5321089	10380511	100.00%	11.693%
49	23.692	3513	3520	3532	rVB2	3189652	6473249	62.36%	7.292%




Sum of corrected areas: 88777935

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012396.D
Acq On : 31 Oct 2022 20:41
Operator : CG/JU
Sample : N5194-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

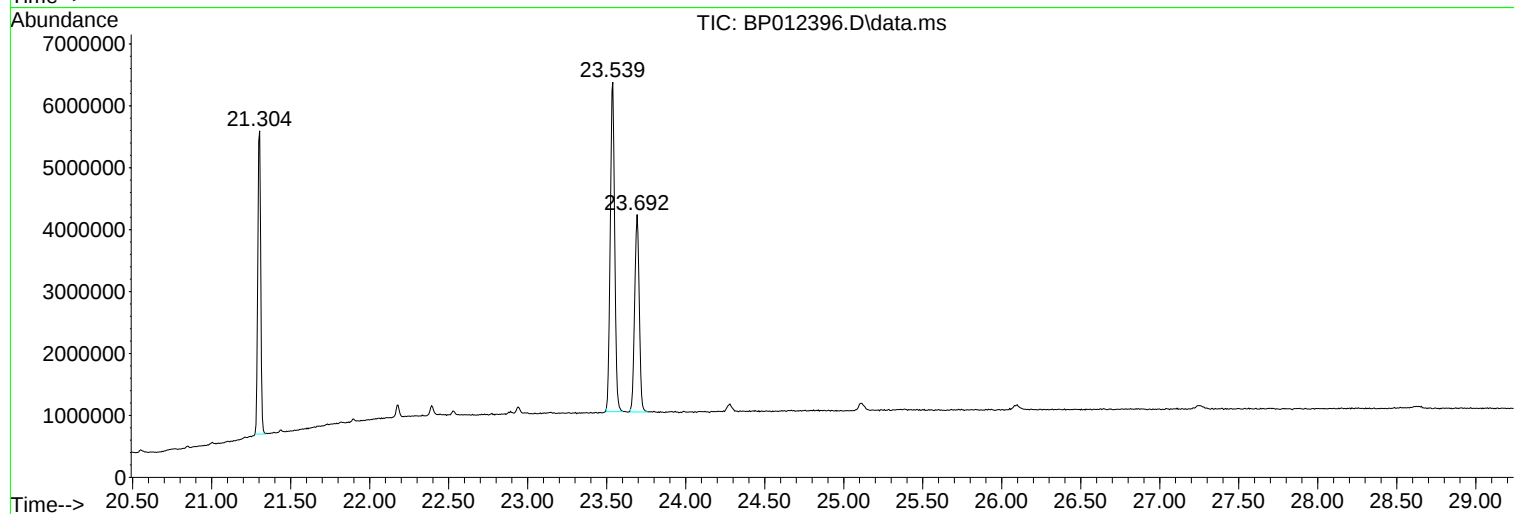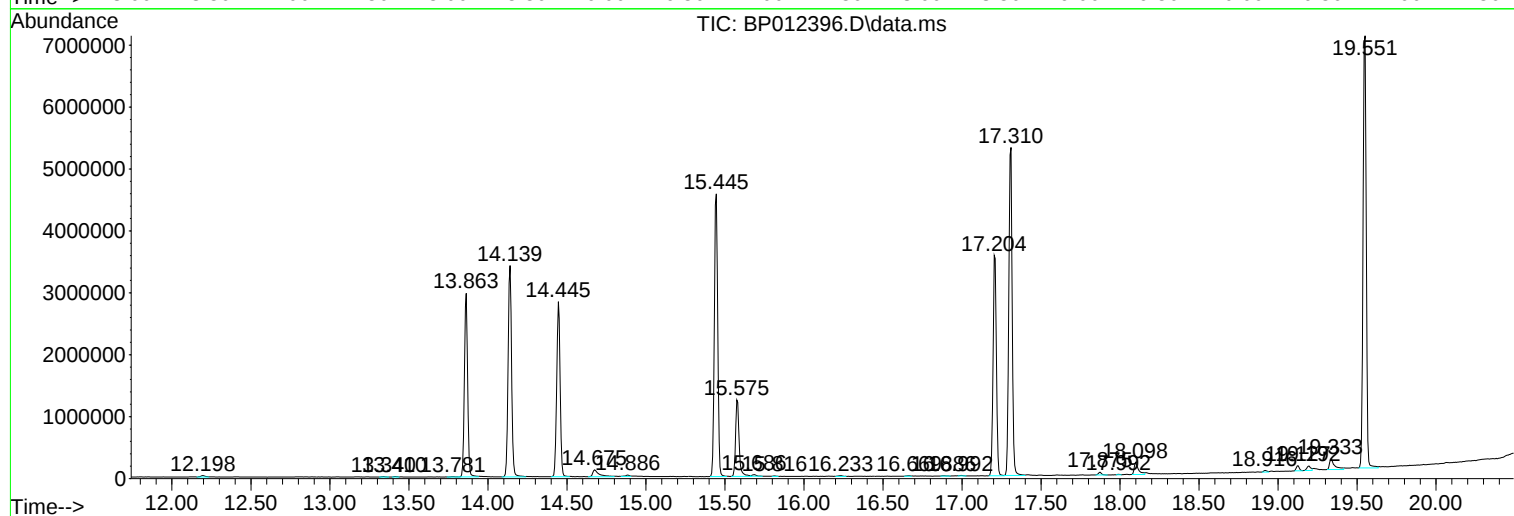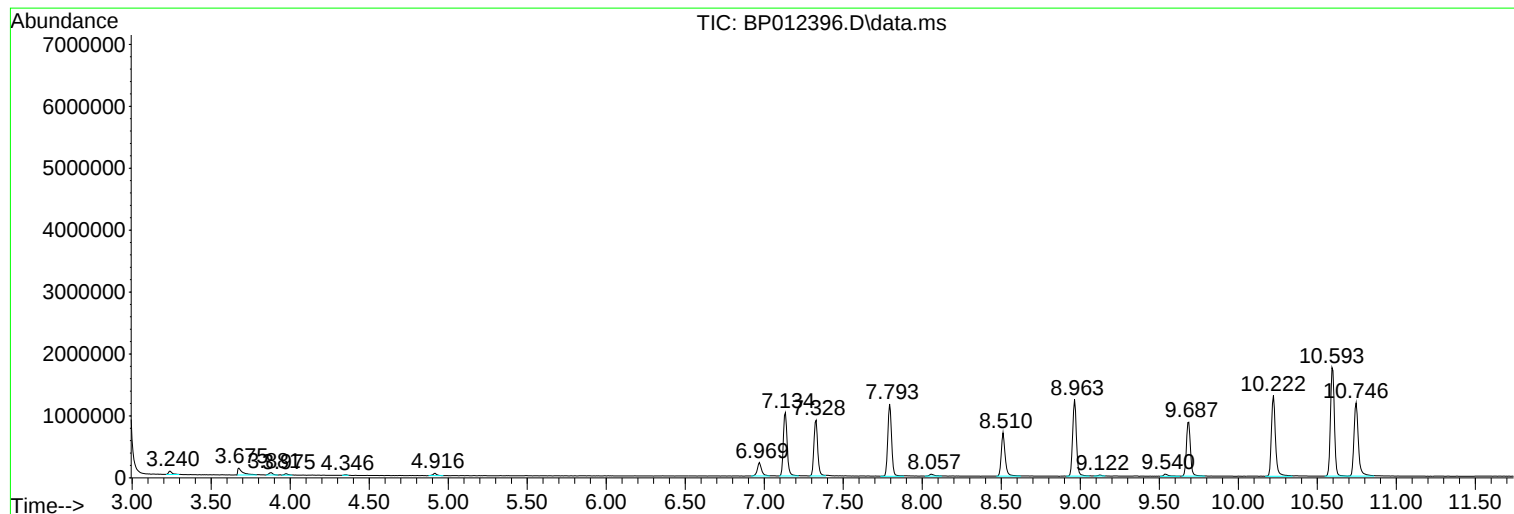

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012396.D
Acq On : 31 Oct 2022 20:41
Operator : CG/JU
Sample : N5194-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012396.D
Acq On : 31 Oct 2022 20:41
Operator : CG/JU
Sample : N5194-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
