

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012397.D
 Acq On : 31 Oct 2022 21:16
 Operator : CG/JU
 Sample : N5216-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	56	rVB	59008	98993	0.87%	0.107%
2	3.669	113	116	141	rBV	161881	356056	3.12%	0.384%
3	3.875	147	151	158	rVB	43628	63686	0.56%	0.069%
4	3.975	164	168	176	rVB	21978	35705	0.31%	0.039%
5	4.916	319	328	333	rBV2	17461	36766	0.32%	0.040%
6	5.105	353	360	366	rVB	30639	45781	0.40%	0.049%
7	5.505	424	428	435	rVB9	7570	13871	0.12%	0.015%
8	6.457	585	590	595	rBV6	8567	15158	0.13%	0.016%
9	6.969	671	677	691	rBV	238864	424067	3.71%	0.458%
10	7.134	698	705	719	rBV	1096791	1831143	16.04%	1.977%
11	7.328	730	738	748	rBV	941753	1620856	14.20%	1.750%
12	7.793	810	817	827	rBV	1165395	1853536	16.23%	2.001%
13	7.993	845	851	857	rBV8	12000	21058	0.18%	0.023%
14	8.163	872	880	887	rVB3	11985	22457	0.20%	0.024%
15	8.510	931	939	956	rBV	768756	1329246	11.64%	1.435%
16	8.963	1008	1016	1033	rBV	1284906	2204754	19.31%	2.380%
17	9.316	1070	1076	1078	rBV4	14896	21862	0.19%	0.024%
18	9.687	1132	1139	1155	rVV	943376	1639596	14.36%	1.770%
19	10.222	1220	1230	1242	rBV	1427141	2556165	22.39%	2.759%
20	10.593	1285	1293	1306	rBV	1655447	2908564	25.47%	3.140%
21	10.693	1306	1310	1312	rVV4	10684	15970	0.14%	0.017%
22	10.746	1312	1319	1340	rVB	1257330	2396813	20.99%	2.587%
23	11.951	1515	1524	1531	rBV2	14391	37140	0.33%	0.040%
24	12.145	1551	1557	1560	rBV6	6263	14098	0.12%	0.015%
25	12.192	1560	1565	1571	rVV3	23930	44288	0.39%	0.048%
26	12.434	1597	1606	1607	rBV9	6660	17380	0.15%	0.019%
27	12.487	1612	1615	1621	rVB4	9744	14450	0.13%	0.016%
28	13.081	1712	1716	1722	rVB2	18274	29998	0.26%	0.032%
29	13.339	1754	1760	1765	rVV3	22739	38340	0.34%	0.041%
30	13.416	1768	1773	1779	rVB5	7055	11652	0.10%	0.013%
31	13.863	1842	1849	1863	rBV	3253955	4639723	40.64%	5.008%
32	13.963	1863	1866	1871	rVB7	8434	15031	0.13%	0.016%
33	14.139	1889	1896	1910	rBV	3926751	5552472	48.63%	5.994%
34	14.398	1936	1940	1941	rBV4	10286	13126	0.11%	0.014%
35	14.445	1941	1948	1957	rVV	2820986	4103924	35.94%	4.430%
36	14.675	1981	1987	2002	rBV	165629	406373	3.56%	0.439%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012397.D
 Acq On : 31 Oct 2022 21:16
 Operator : CG/JU
 Sample : N5216-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	14.892	2020	2024	2029	rVB8	9051	16698	0.15%	0.018%
38	15.010	2039	2044	2054	rBV	18959	41050	0.36%	0.044%
39	15.281	2088	2090	2098	rVB8	7026	12104	0.11%	0.013%
40	15.445	2108	2118	2132	rBV	5111727	7379595	64.63%	7.966%
41	15.575	2134	2140	2152	rVV	1591827	2247743	19.69%	2.426%
42	15.681	2155	2158	2166	rVB3	26520	50835	0.45%	0.055%
43	15.822	2178	2182	2189	rVB3	13703	23134	0.20%	0.025%
44	15.975	2202	2208	2211	rBV	27214	49094	0.43%	0.053%
45	16.157	2236	2239	2242	rBV4	8572	12539	0.11%	0.014%
46	16.233	2247	2252	2263	rVB	21140	38161	0.33%	0.041%
47	16.716	2331	2334	2343	rVB8	15864	29240	0.26%	0.032%
48	17.210	2411	2418	2428	rBV	3419397	5083152	44.52%	5.487%
49	17.304	2428	2434	2450	rVV2	5740198	8551949	74.90%	9.232%
50	18.098	2565	2569	2577	rBV	82690	143114	1.25%	0.154%
51	19.122	2740	2743	2749	rVB2	82693	109318	0.96%	0.118%
52	19.192	2752	2755	2759	rVV	75081	95450	0.84%	0.103%
53	19.333	2776	2779	2788	rBV4	61681	106691	0.93%	0.115%
54	19.551	2810	2816	2822	rBV	7593543	10408404	91.16%	11.236%
55	21.298	3108	3113	3121	rBV	4723954	6267173	54.89%	6.765%
56	23.539	3487	3494	3507	rVB	5701131	11417985	100.00%	12.325%
57	23.692	3513	3520	3530	rVB2	3030209	6103870	53.46%	6.589%




Sum of corrected areas: 92637397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012397.D
Acq On : 31 Oct 2022 21:16
Operator : CG/JU
Sample : N5216-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

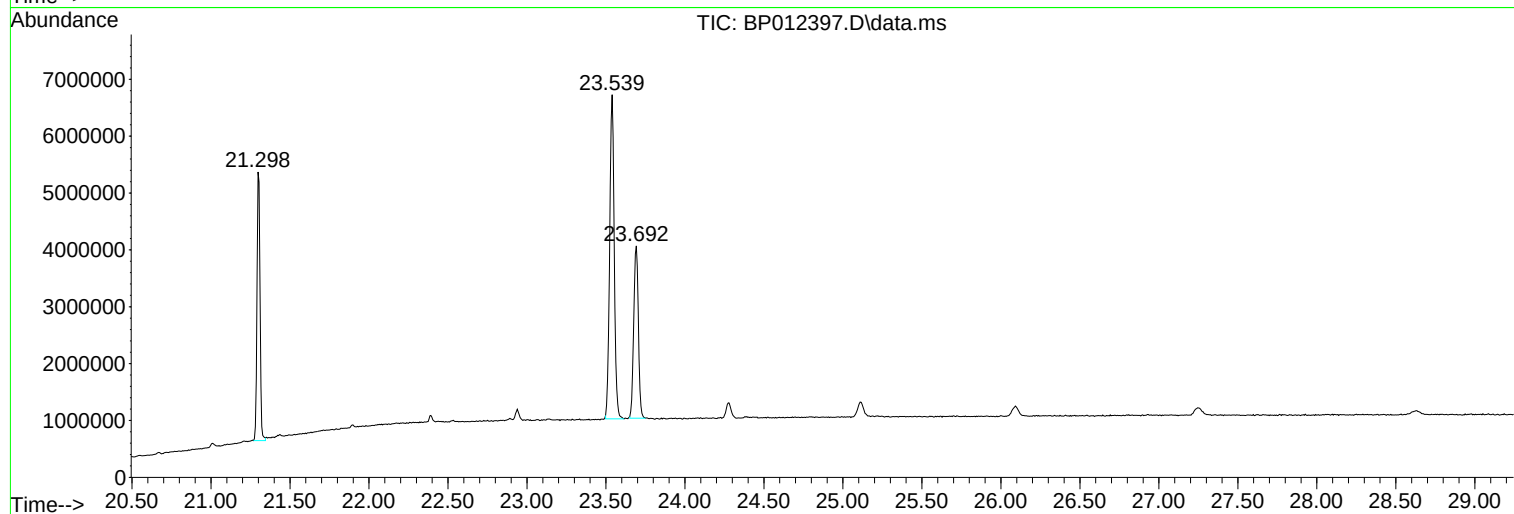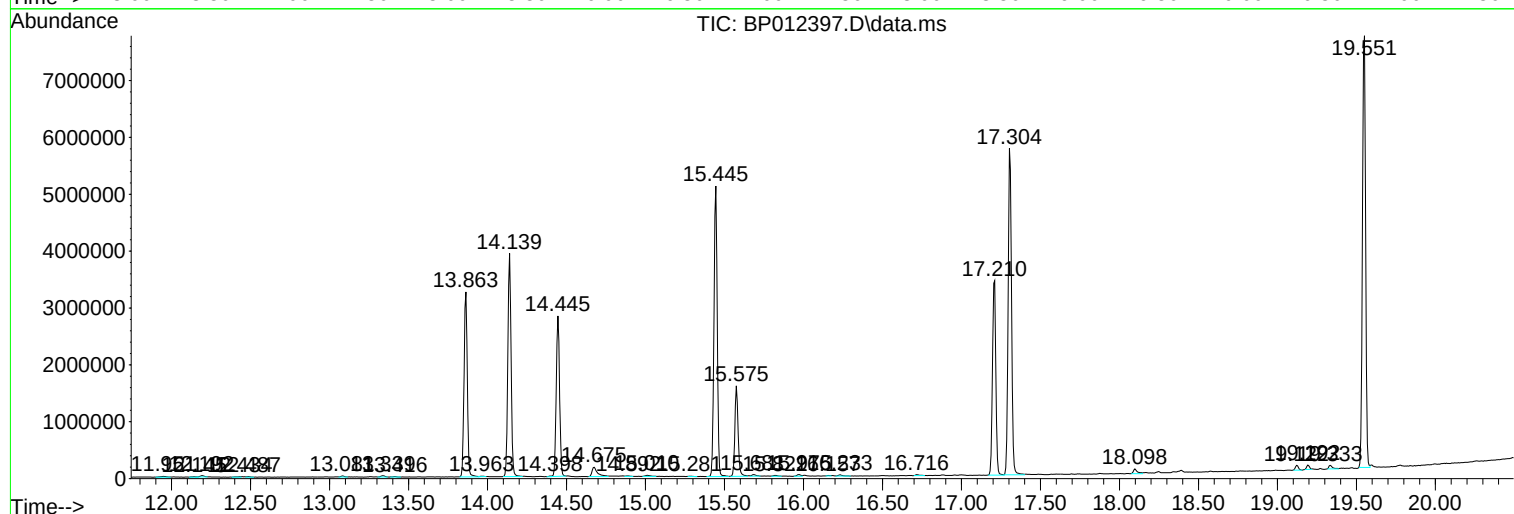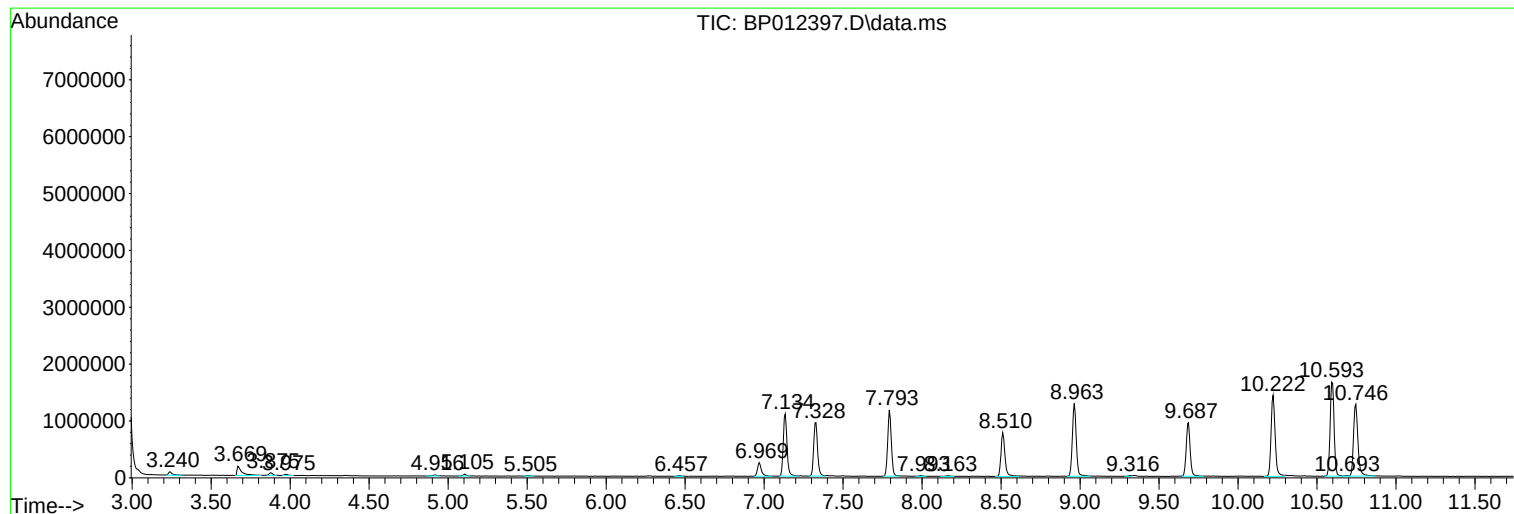

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012397.D
Acq On : 31 Oct 2022 21:16
Operator : CG/JU
Sample : N5216-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012397.D
Acq On : 31 Oct 2022 21:16
Operator : CG/JU
Sample : N5216-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc