

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012399.D
 Acq On : 31 Oct 2022 22:25
 Operator : CG/JU
 Sample : N5216-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	54	rVB	53317	88680	0.78%	0.101%
2	3.669	113	116	131	rBV	156660	308396	2.71%	0.350%
3	3.875	146	151	158	rVB	37744	61826	0.54%	0.070%
4	3.975	164	168	175	rVB	21803	32728	0.29%	0.037%
5	4.916	321	328	336	rBV2	19030	39032	0.34%	0.044%
6	6.969	669	677	696	rBV	194389	359841	3.16%	0.409%
7	7.134	698	705	722	rBV	993699	1653980	14.54%	1.878%
8	7.322	731	737	748	rBV	842509	1426580	12.54%	1.620%
9	7.793	810	817	827	rBV	1121566	1834593	16.12%	2.083%
10	8.510	932	939	957	rBV	632818	1125818	9.89%	1.278%
11	8.963	1008	1016	1035	rBV	1144418	1982489	17.42%	2.251%
12	9.345	1075	1081	1089	rBV2	17650	29185	0.26%	0.033%
13	9.681	1129	1138	1154	rBV	866785	1532192	13.47%	1.740%
14	10.222	1222	1230	1247	rBV	1259451	2274687	19.99%	2.583%
15	10.592	1285	1293	1306	rBV	1649499	2859816	25.13%	3.248%
16	10.745	1311	1319	1346	rVV	1172158	2184320	19.20%	2.480%
17	12.192	1559	1565	1575	rBV2	20418	41935	0.37%	0.048%
18	13.257	1741	1746	1750	rVB	15864	22282	0.20%	0.025%
19	13.339	1755	1760	1768	rVV5	9472	19028	0.17%	0.022%
20	13.863	1841	1849	1860	rBV	2876759	4082763	35.88%	4.636%
21	14.139	1889	1896	1914	rBV	3357564	4943733	43.45%	5.614%
22	14.445	1941	1948	1957	rBV	2720735	3956465	34.77%	4.493%
23	14.675	1981	1987	2004	rBV	125179	339420	2.98%	0.385%
24	14.880	2015	2022	2030	rVB	10485	24681	0.22%	0.028%
25	15.075	2050	2055	2063	rVB	8134	15914	0.14%	0.018%
26	15.198	2070	2076	2081	rBV	155580	218956	1.92%	0.249%
27	15.445	2111	2118	2133	rBV	4433108	6595884	57.97%	7.490%
28	15.575	2134	2140	2151	rBV	1542296	2148904	18.89%	2.440%
29	15.686	2155	2159	2164	rVB	24642	39322	0.35%	0.045%
30	15.963	2202	2206	2211	rBV7	16930	31006	0.27%	0.035%
31	17.204	2410	2417	2428	rBV	3419920	4933530	43.36%	5.602%
32	17.304	2428	2434	2448	rBV2	5479964	8060832	70.85%	9.154%
33	17.492	2464	2466	2472	rVB6	9171	14620	0.13%	0.017%
34	18.098	2564	2569	2578	rBV	123289	241354	2.12%	0.274%
35	19.121	2739	2743	2749	rBV2	80169	113400	1.00%	0.129%
36	19.192	2751	2755	2762	rBV	75503	121669	1.07%	0.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012399.D
Acq On : 31 Oct 2022 22:25
Operator : CG/JU
Sample : N5216-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA86

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	19.333	2775	2779	2790	rBV	101432	193053	1.70%	0.219%
38	19.545	2810	2815	2827	rBV	7300475	9953347	87.48%	11.303%
39	21.010	3060	3064	3072	rBV3	182061	385882	3.39%	0.438%
40	21.298	3108	3113	3121	rBV	4570830	6151042	54.06%	6.985%
41	23.539	3486	3494	3507	rVB2	5574699	11378073	100.00%	12.921%
42	23.686	3513	3519	3530	rVB2	3093649	6239113	54.83%	7.085%




Sum of corrected areas: 88060371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012399\
Data File : BP012399.D
Acq On : 31 Oct 2022 22:25
Operator : CG/JU
Sample : N5216-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

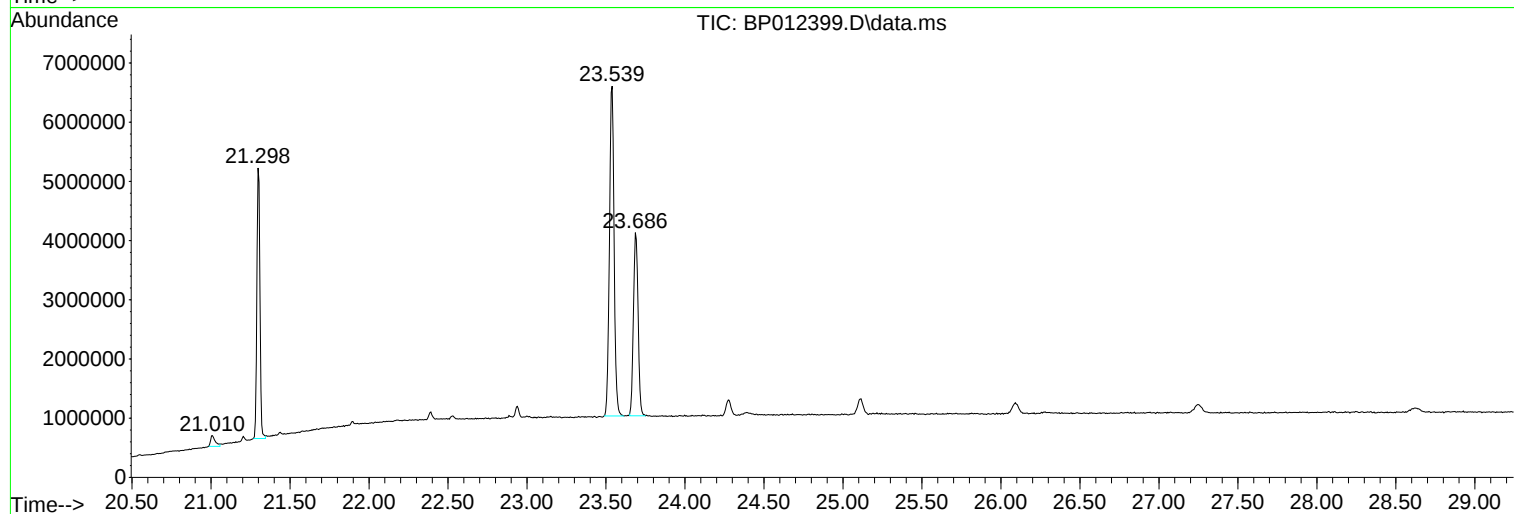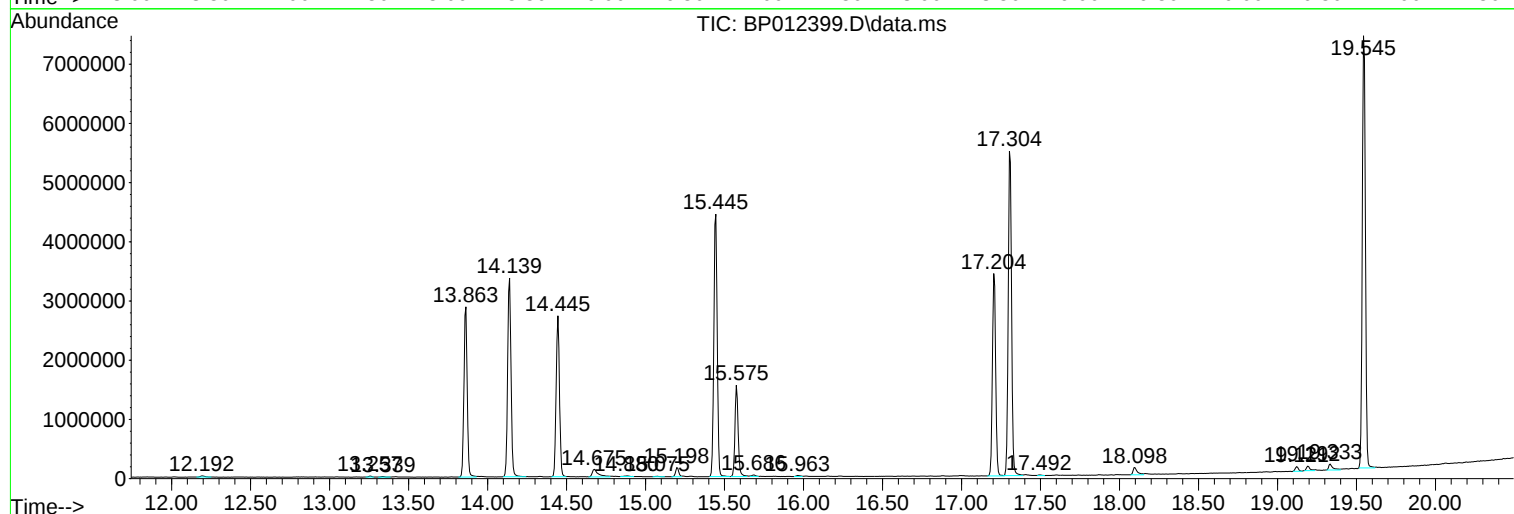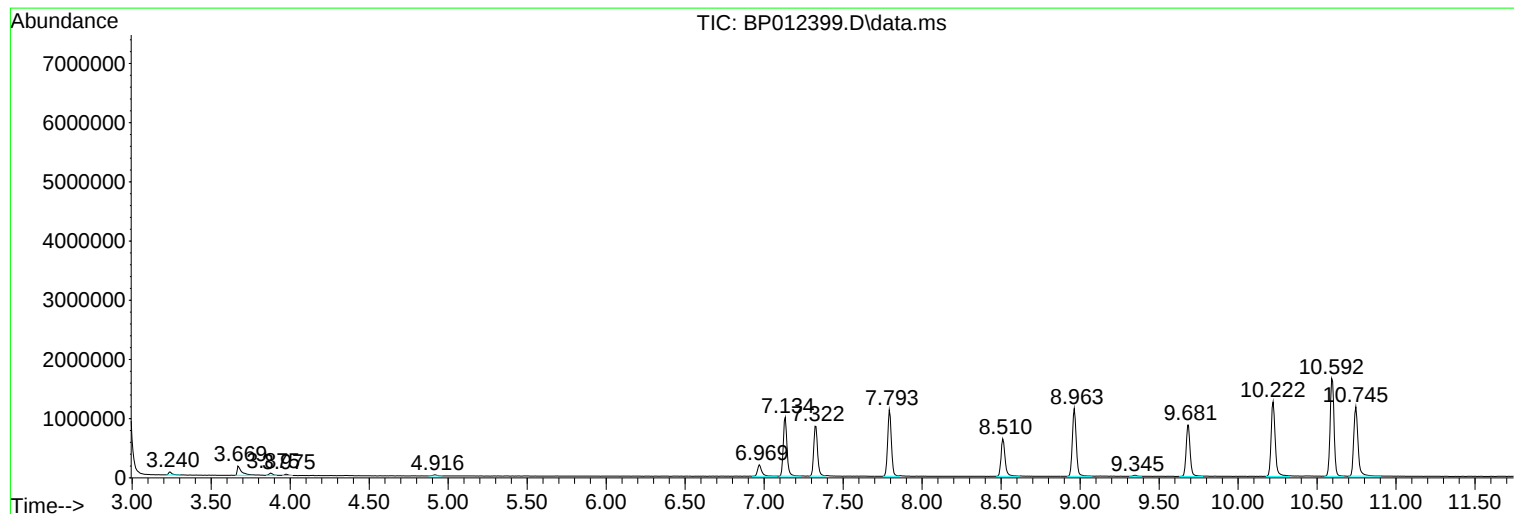

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012399.D
Acq On : 31 Oct 2022 22:25
Operator : CG/JU
Sample : N5216-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012399.D
Acq On : 31 Oct 2022 22:25
Operator : CG/JU
Sample : N5216-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc