

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012402.D
 Acq On : 01 Nov 2022 00:08
 Operator : CG/JU
 Sample : N5216-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	48	rBV	43233	59228	0.66%	0.071%
2	3.681	115	118	134	rBV	67999	155502	1.73%	0.187%
3	3.975	164	168	175	rVB	21053	32267	0.36%	0.039%
4	5.099	356	359	365	rVB4	8025	12627	0.14%	0.015%
5	6.964	669	676	693	rBV	936953	1598958	17.81%	1.922%
6	7.134	698	705	727	rVB	910103	1572236	17.51%	1.889%
7	7.322	730	737	752	rBV	1091933	1812751	20.19%	2.178%
8	7.793	809	817	828	rBV	1096538	1761724	19.62%	2.117%
9	8.510	931	939	956	rBV	1276542	2185001	24.33%	2.626%
10	8.963	1008	1016	1030	rBV	1097152	1864642	20.77%	2.241%
11	9.681	1131	1138	1153	rBV	898963	1523851	16.97%	1.831%
12	10.222	1222	1230	1252	rBV	1309531	2419034	26.94%	2.907%
13	10.428	1260	1265	1272	rBV9	9020	22391	0.25%	0.027%
14	10.593	1284	1293	1306	rBV	1608217	2727353	30.37%	3.278%
15	10.740	1311	1318	1335	rBV	1193487	2281244	25.41%	2.742%
16	12.193	1561	1565	1570	rBV5	5618	9192	0.10%	0.011%
17	13.340	1754	1760	1767	rBV2	33098	60355	0.67%	0.073%
18	13.857	1842	1848	1860	rBV	2700343	3893163	43.36%	4.679%
19	14.140	1887	1896	1912	rBV	3093425	4732414	52.70%	5.687%
20	14.445	1941	1948	1962	rBV	2523434	3864527	43.04%	4.644%
21	14.663	1979	1985	2007	rBV	859243	1592520	17.74%	1.914%
22	15.440	2110	2117	2130	rBV	4005741	6004896	66.87%	7.216%
23	15.575	2134	2140	2154	rVV	1244368	1837077	20.46%	2.208%
24	15.681	2154	2158	2160	rVV	44046	71892	0.80%	0.086%
25	15.710	2160	2163	2173	rVB	136475	192471	2.14%	0.231%
26	16.228	2247	2251	2258	rVB6	12221	18828	0.21%	0.023%
27	16.881	2357	2362	2367	rBV8	8719	14799	0.16%	0.018%
28	17.204	2410	2417	2427	rBV	3456483	4792768	53.38%	5.760%
29	17.304	2427	2434	2450	rVV2	4664157	6649109	74.05%	7.991%
30	17.875	2527	2531	2536	rBV2	37848	45991	0.51%	0.055%
31	18.098	2566	2569	2577	rBV4	35533	70102	0.78%	0.084%
32	19.010	2720	2724	2728	rBV3	72959	85219	0.95%	0.102%
33	19.133	2740	2745	2751	rBV4	47966	93945	1.05%	0.113%
34	19.545	2809	2815	2830	rBV	6257543	8440500	94.00%	10.143%
35	21.298	3108	3113	3124	rBV	4602969	5955172	66.32%	7.157%
36	23.533	3486	3493	3506	rVB	4300585	8979325	100.00%	10.791%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012402.D
Acq On : 01 Nov 2022 00:08
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA84

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	23.686	3513	3519	3536	rVB2	2873199	5777987	64.35%	6.944%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 83211061

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012402.D
Acq On : 01 Nov 2022 00:08
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

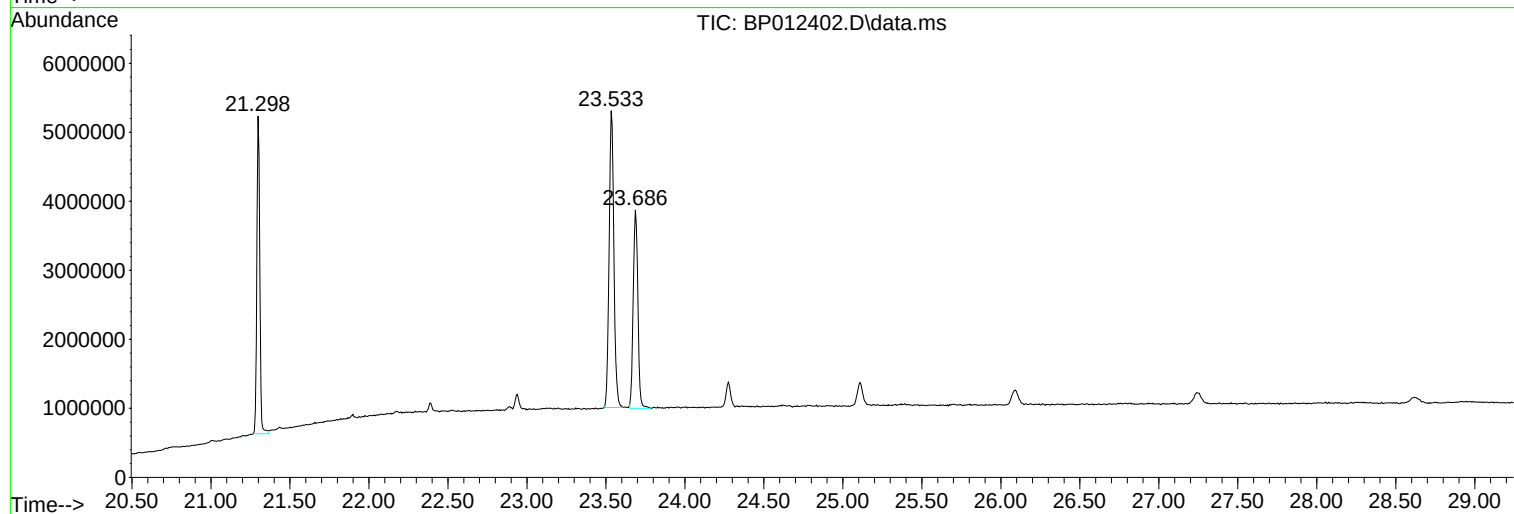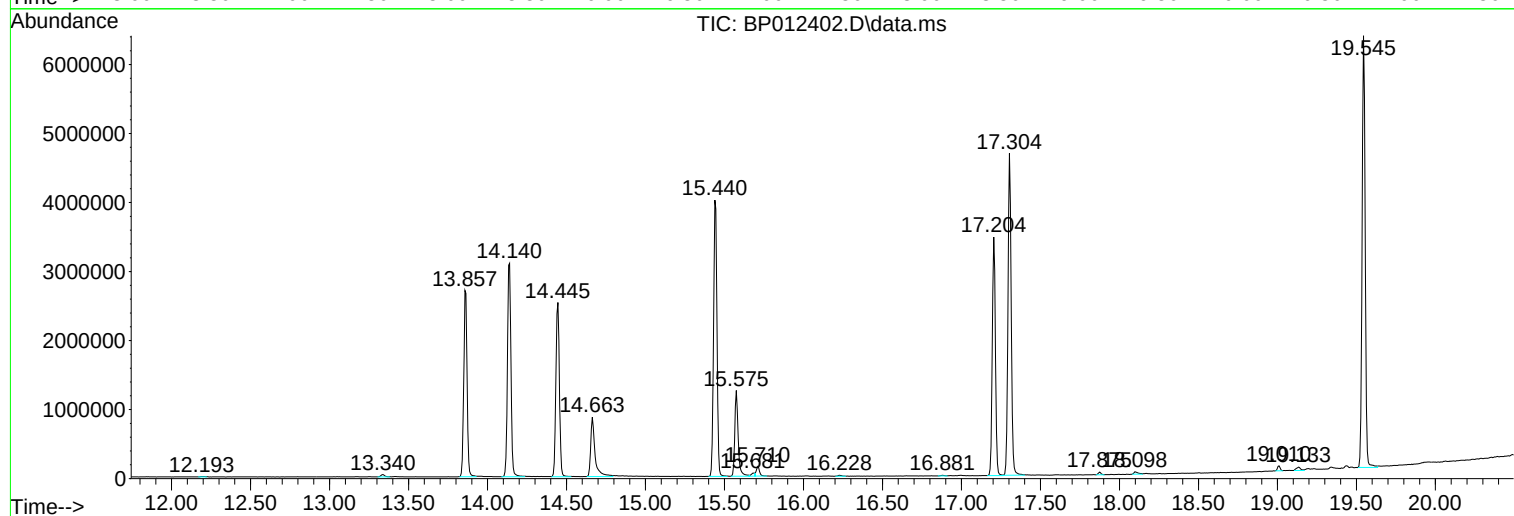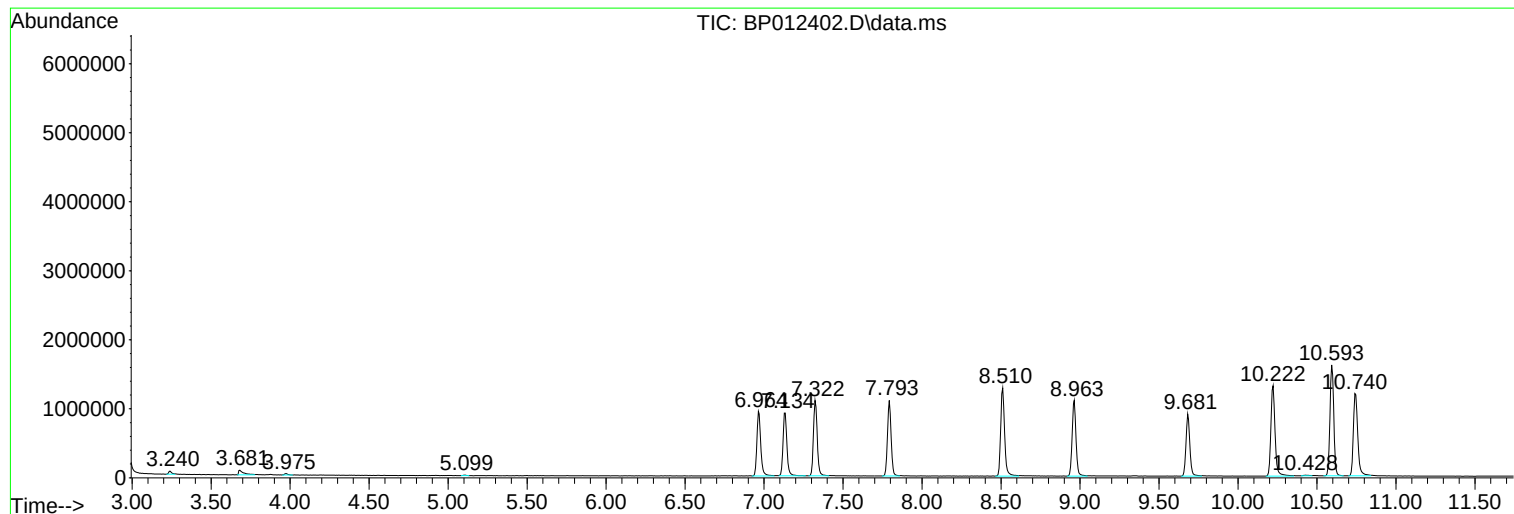

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012402.D
Acq On : 01 Nov 2022 00:08
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012402.D
Acq On : 01 Nov 2022 00:08
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc