

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012405.D
 Acq On : 01 Nov 2022 01:51
 Operator : CG/JU
 Sample : N5216-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	48	rBV	47506	66201	0.62%	0.081%
2	3.670	114	116	137	rBV	140998	292167	2.75%	0.358%
3	3.875	146	151	157	rVB	41442	65191	0.61%	0.080%
4	3.975	163	168	174	rBV	87117	127271	1.20%	0.156%
5	4.346	229	231	240	rVB8	6389	12071	0.11%	0.015%
6	4.911	319	327	335	rBV2	17865	36452	0.34%	0.045%
7	5.681	453	458	467	rVB	30243	49613	0.47%	0.061%
8	5.846	480	486	494	rVB	74019	117055	1.10%	0.144%
9	6.969	670	677	688	rBV	196845	359963	3.39%	0.442%
10	7.128	698	704	716	rBV	1026833	1698319	15.98%	2.084%
11	7.322	730	737	748	rBV	887264	1483720	13.96%	1.820%
12	7.793	808	817	829	rBV	875215	1420741	13.37%	1.743%
13	8.511	932	939	958	rBV	658884	1169322	11.00%	1.435%
14	8.905	1000	1006	1009	rBV2	8722	14142	0.13%	0.017%
15	8.963	1009	1016	1034	rVV	1181984	2057581	19.36%	2.524%
16	9.681	1128	1138	1153	rBV	929819	1601929	15.07%	1.965%
17	10.216	1220	1229	1246	rBV	1298709	2358407	22.19%	2.894%
18	10.593	1285	1293	1306	rBV	1311617	2219826	20.89%	2.723%
19	10.740	1311	1318	1343	rVB	1221327	2342669	22.05%	2.874%
20	12.193	1558	1565	1573	rBV	22894	45240	0.43%	0.056%
21	12.799	1661	1668	1671	rBV8	5680	12008	0.11%	0.015%
22	13.334	1755	1759	1765	rVB2	15347	25404	0.24%	0.031%
23	13.410	1768	1772	1780	rBV7	7229	13502	0.13%	0.017%
24	13.857	1842	1848	1861	rBV	2915208	4188363	39.41%	5.139%
25	13.969	1862	1867	1875	rVB2	61409	95691	0.90%	0.117%
26	14.140	1886	1896	1907	rBV	3445531	5165082	48.61%	6.337%
27	14.228	1909	1911	1915	rVB3	11603	13739	0.13%	0.017%
28	14.446	1941	1948	1957	rBV	2095740	3117249	29.33%	3.825%
29	14.675	1981	1987	2005	rBV	115050	320542	3.02%	0.393%
30	14.887	2020	2023	2027	rVB6	11016	15407	0.14%	0.019%
31	15.198	2070	2076	2081	rBV2	13493	19867	0.19%	0.024%
32	15.440	2110	2117	2133	rBV	4491097	6656137	62.64%	8.166%
33	15.575	2134	2140	2152	rVV	1427594	2022733	19.03%	2.482%
34	15.687	2152	2159	2170	rVB4	28071	71715	0.67%	0.088%
35	17.204	2411	2417	2428	rBV	2714303	3909419	36.79%	4.796%
36	17.304	2428	2434	2450	rVV2	5247365	7802616	73.43%	9.573%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012405.D
 Acq On : 01 Nov 2022 01:51
 Operator : CG/JU
 Sample : N5216-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA60

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	18.098	2565	2569	2575	rBV2	65975	110709	1.04%	0.136%
38	19.122	2739	2743	2750	rBV2	73560	102709	0.97%	0.126%
39	19.192	2751	2755	2760	rVV	74121	104040	0.98%	0.128%
40	19.269	2764	2768	2773	rBV	86840	101038	0.95%	0.124%
41	19.333	2775	2779	2785	rBV5	69582	115979	1.09%	0.142%
42	19.545	2809	2815	2822	rBV	7230107	9541815	89.79%	11.707%
43	21.298	3108	3113	3122	rBV	4081680	4918610	46.29%	6.035%
44	23.533	3486	3493	3504	rVB2	5206488	10626574	100.00%	13.038%
45	23.686	3513	3519	3532	rVB2	2418434	4898083	46.09%	6.009%




Sum of corrected areas: 81506911

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012405.D
Acq On : 01 Nov 2022 01:51
Operator : CG/JU
Sample : N5216-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

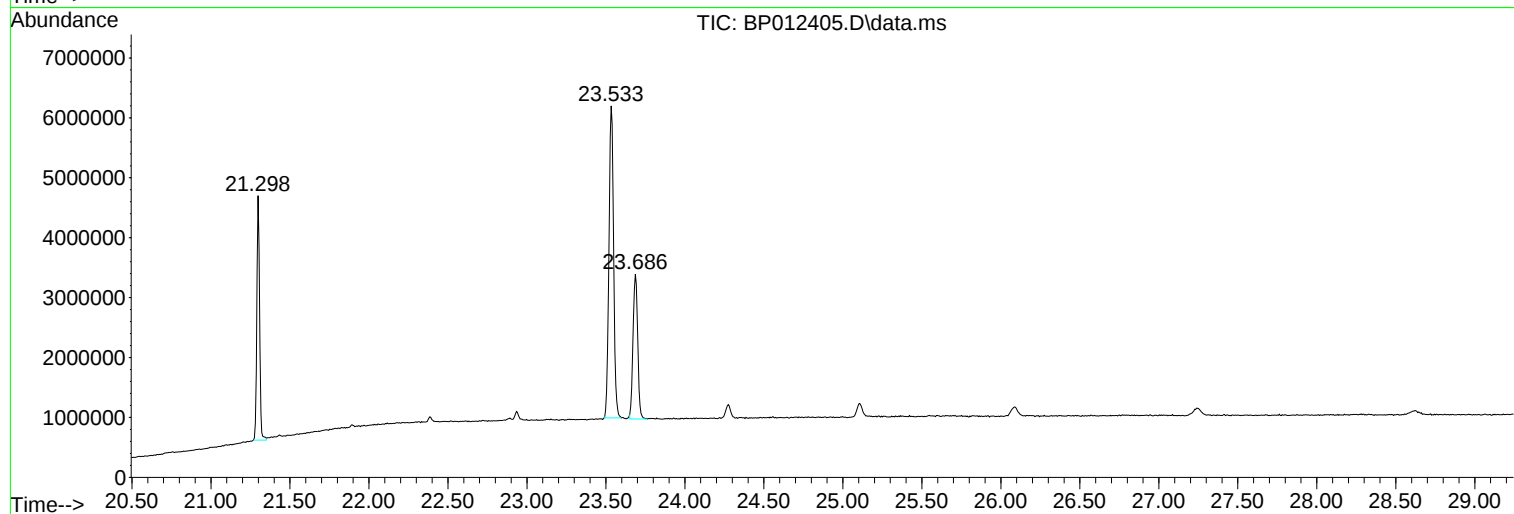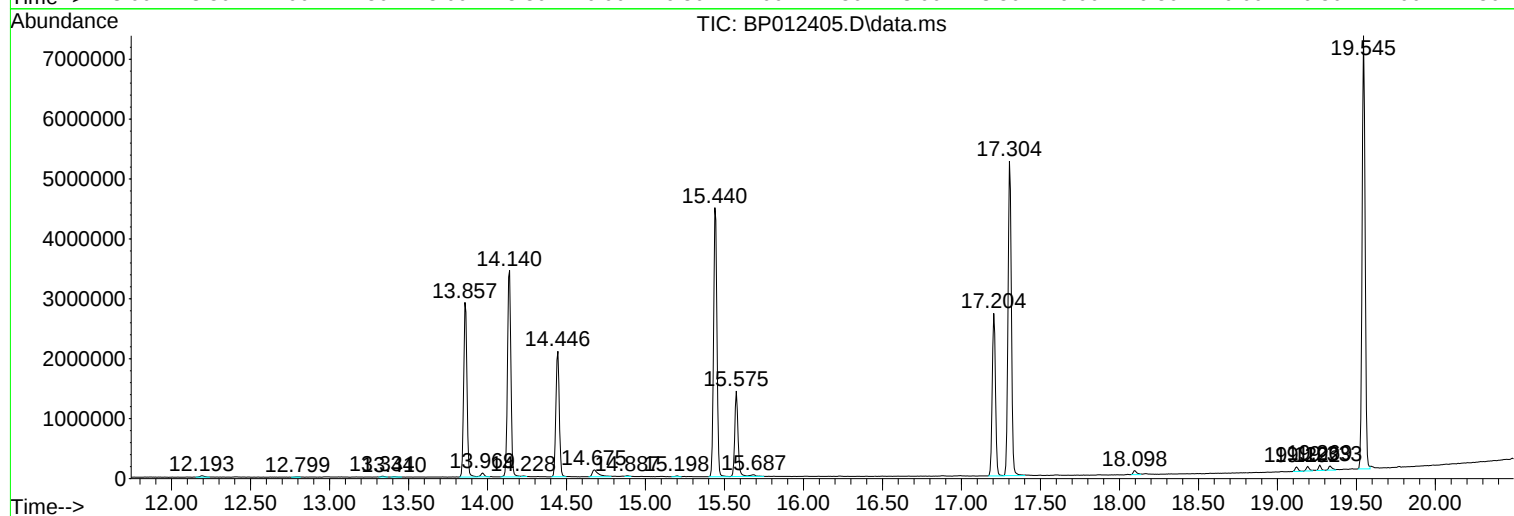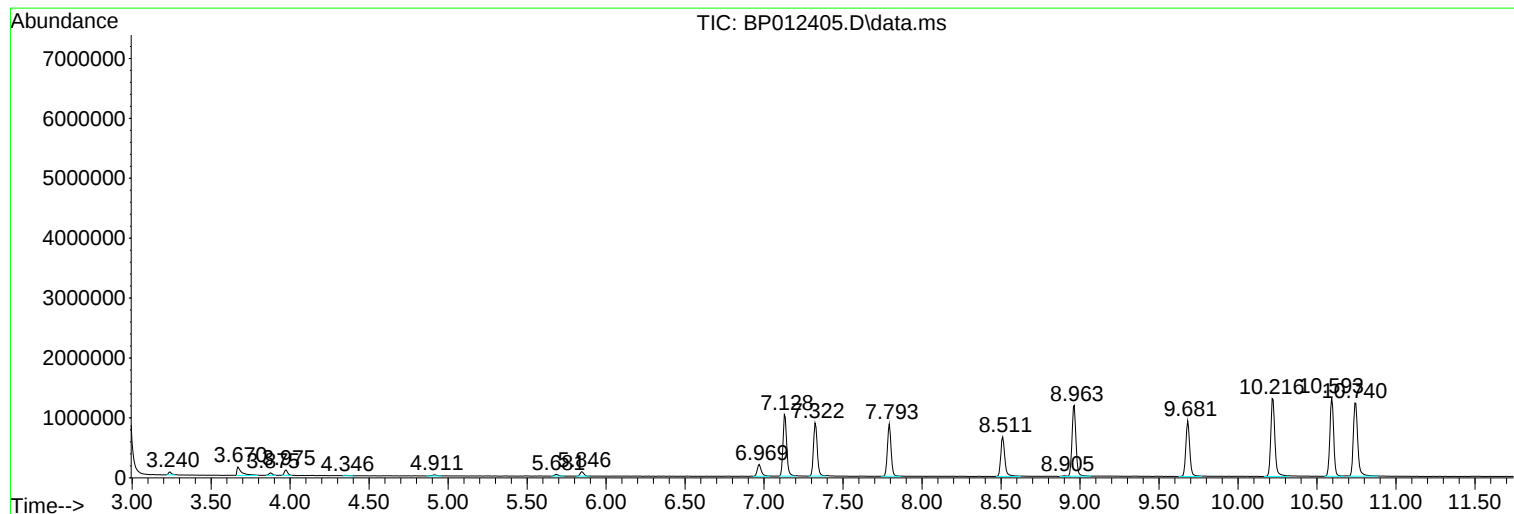

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012405.D
Acq On : 01 Nov 2022 01:51
Operator : CG/JU
Sample : N5216-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012405.D
Acq On : 01 Nov 2022 01:51
Operator : CG/JU
Sample : N5216-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
