

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012413.D
 Acq On : 01 Nov 2022 06:58
 Operator : CG/JU
 Sample : N5216-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	51	rVB	52239	82944	0.73%	0.090%
2	3.534	90	93	103	rVB	16427	33659	0.30%	0.036%
3	3.670	113	116	138	rBV	123686	261339	2.32%	0.283%
4	3.875	146	151	159	rBV	39132	65531	0.58%	0.071%
5	3.969	164	167	175	rVB	23100	35087	0.31%	0.038%
6	6.969	671	677	693	rVB	199468	374162	3.31%	0.405%
7	7.128	697	704	720	rBV	1109812	1840097	16.30%	1.994%
8	7.322	730	737	748	rBV	934567	1548510	13.72%	1.678%
9	7.793	810	817	827	rBV	1107072	1862796	16.50%	2.018%
10	8.510	930	939	956	rBV	672377	1200833	10.64%	1.301%
11	8.957	1007	1015	1033	rBV	1290965	2242132	19.86%	2.429%
12	9.346	1075	1081	1086	rVB	34929	53596	0.47%	0.058%
13	9.681	1130	1138	1157	rBV	977229	1678463	14.87%	1.819%
14	10.216	1222	1229	1254	rBV	1387033	2504563	22.19%	2.714%
15	10.404	1256	1261	1266	rBV3	12851	28842	0.26%	0.031%
16	10.593	1285	1293	1307	rBV	1734266	2949176	26.12%	3.195%
17	10.740	1311	1318	1338	rBV	1096464	2061499	18.26%	2.234%
18	12.193	1558	1565	1573	rBV	26043	49693	0.44%	0.054%
19	13.257	1740	1746	1750	rVV5	6886	12247	0.11%	0.013%
20	13.334	1755	1759	1766	rVB3	12164	20348	0.18%	0.022%
21	13.857	1839	1848	1862	rBV	3192002	4523928	40.07%	4.901%
22	13.945	1862	1863	1870	rVB7	8186	14835	0.13%	0.016%
23	14.134	1885	1895	1912	rBV	3701419	5636970	49.93%	6.107%
24	14.445	1940	1948	1966	rVB	2728192	4181572	37.04%	4.531%
25	14.675	1981	1987	2000	rBV2	116206	299163	2.65%	0.324%
26	14.881	2015	2022	2028	rVB9	14963	32787	0.29%	0.036%
27	15.281	2087	2090	2097	rVB8	7784	12887	0.11%	0.014%
28	15.439	2110	2117	2133	rBV	4900741	7274759	64.44%	7.882%
29	15.575	2133	2140	2152	rVV	1527088	2150372	19.05%	2.330%
30	15.681	2155	2158	2165	rVB	27923	45281	0.40%	0.049%
31	16.228	2247	2251	2256	rVB7	9244	15868	0.14%	0.017%
32	17.204	2410	2417	2427	rBV	3666711	5186920	45.95%	5.620%
33	17.304	2427	2434	2446	rVV	5788823	8301272	73.53%	8.994%
34	17.875	2528	2531	2534	rVB3	13874	12752	0.11%	0.014%
35	18.092	2564	2568	2578	rBV	183423	314941	2.79%	0.341%
36	19.122	2739	2743	2749	rBV3	79146	111538	0.99%	0.121%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012413.D
Acq On : 01 Nov 2022 06:58
Operator : CG/JU
Sample : N5216-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Title : SVOA CALIBRATION

37	19.192	2751	2755	2767	rVV	83687	153966	1.36%	0.167%
38	19.333	2775	2779	2785	rBV2	134150	225882	2.00%	0.245%
39	19.545	2809	2815	2827	rBV	7817184	10345486	91.64%	11.209%
40	21.004	3060	3063	3073	rBV3	256211	462401	4.10%	0.501%
41	21.298	3108	3113	3120	rBV	4983433	6380554	56.52%	6.913%
42	23.533	3486	3493	3506	rVB2	5620948	11288890	100.00%	12.231%
43	23.686	3513	3519	3534	rVB2	3253218	6419606	56.87%	6.955%




Sum of corrected areas: 92298147

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012413.D
Acq On : 01 Nov 2022 06:58
Operator : CG/JU
Sample : N5216-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA68

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

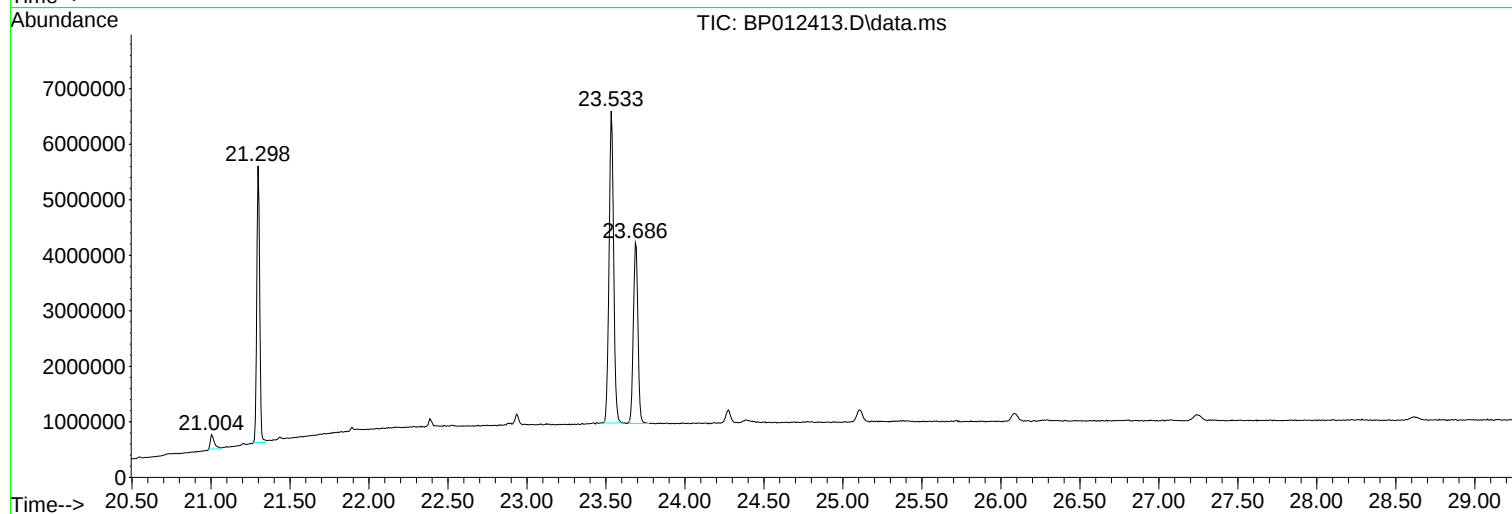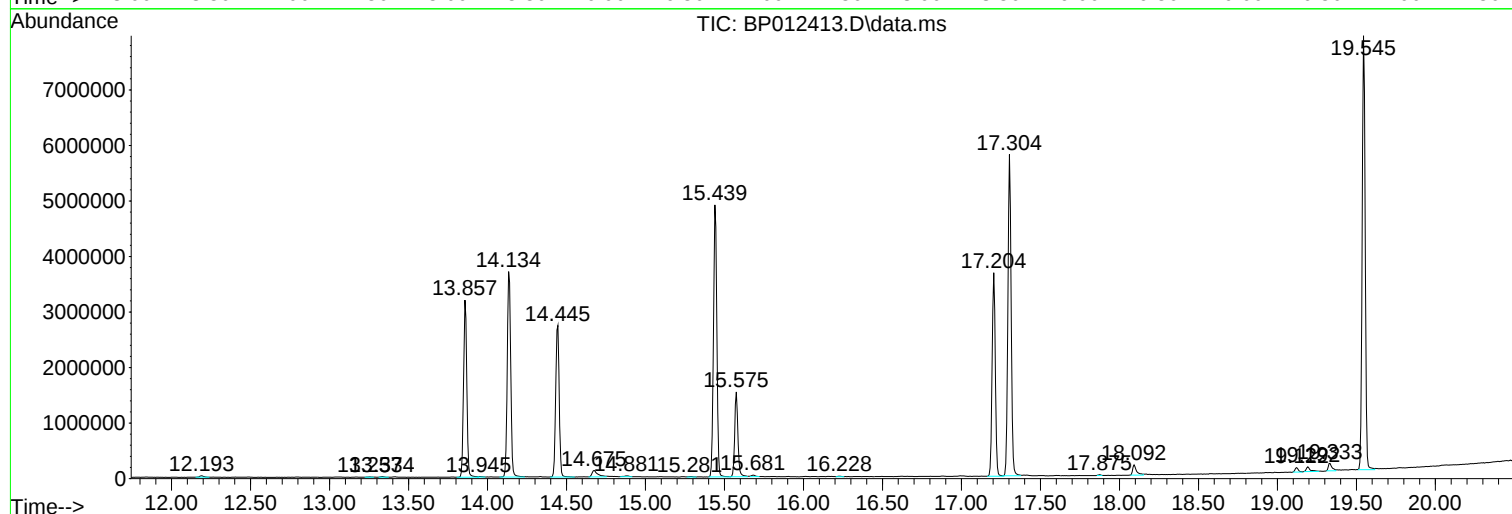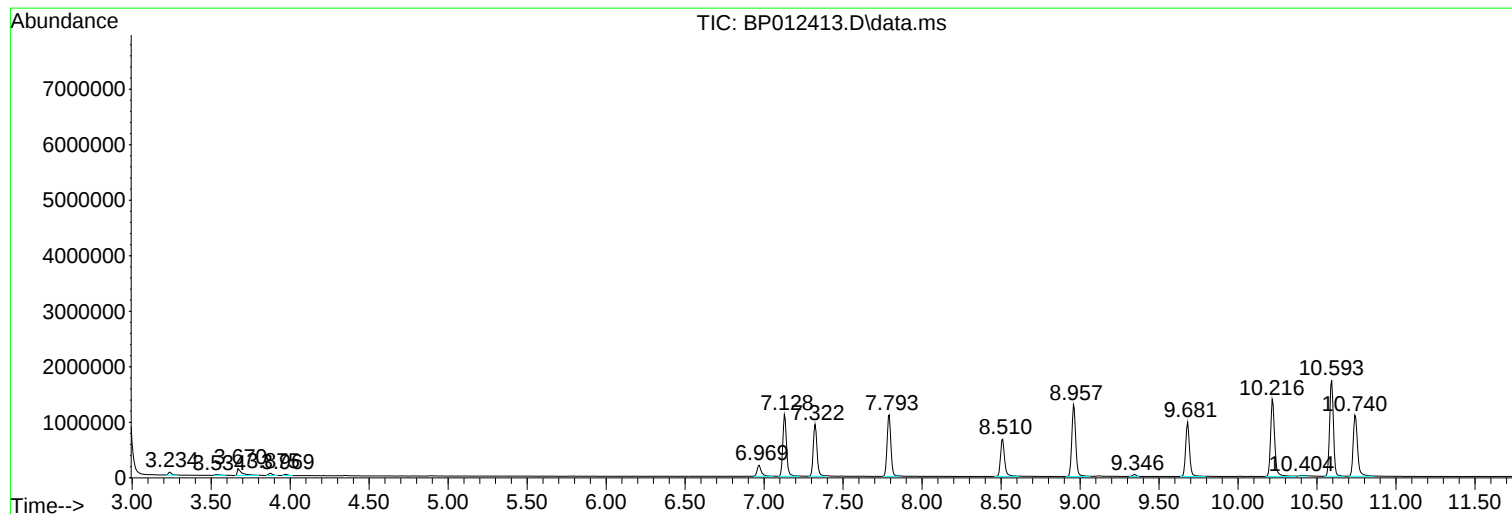

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012413.D
Acq On : 01 Nov 2022 06:58
Operator : CG/JU
Sample : N5216-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA68

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012413.D
Acq On : 01 Nov 2022 06:58
Operator : CG/JU
Sample : N5216-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA68

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc