

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012416.D
 Acq On : 01 Nov 2022 08:41
 Operator : CG/JU
 Sample : N5270-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	53	rVB	72736	111102	0.81%	0.098%
2	3.664	113	115	136	rBV	318421	600983	4.40%	0.528%
3	3.875	146	151	160	rVV	53391	89277	0.65%	0.078%
4	3.970	164	167	173	rVB	22301	31540	0.23%	0.028%
5	4.893	320	324	330	rVB	10670	17397	0.13%	0.015%
6	6.964	669	676	689	rBV	394520	698527	5.11%	0.614%
7	7.128	698	704	718	rBV	1488067	2416762	17.68%	2.125%
8	7.322	730	737	748	rBV	1392388	2270050	16.61%	1.996%
9	7.793	809	817	833	rBV	1208444	2008129	14.69%	1.766%
10	8.505	932	938	954	rBV	1164106	2008667	14.70%	1.766%
11	8.958	1007	1015	1033	rBV	1722546	2950533	21.59%	2.594%
12	9.346	1075	1081	1088	rVB2	16804	29794	0.22%	0.026%
13	9.681	1130	1138	1157	rBV	1374700	2357583	17.25%	2.073%
14	10.216	1221	1229	1251	rBV	2008428	3523464	25.78%	3.098%
15	10.387	1251	1258	1276	rVV2	36435	128336	0.94%	0.113%
16	10.593	1285	1293	1309	rVB	1901551	3159897	23.12%	2.778%
17	10.740	1310	1318	1348	rVV	1802269	3259220	23.84%	2.866%
18	12.187	1558	1564	1573	rBV2	32871	66995	0.49%	0.059%
19	13.063	1705	1713	1721	rBV2	5025	16327	0.12%	0.014%
20	13.251	1739	1745	1754	rVV4	12737	23639	0.17%	0.021%
21	13.416	1767	1773	1779	rBV5	9683	16797	0.12%	0.015%
22	13.857	1841	1848	1861	rBV	4211077	5908776	43.23%	5.195%
23	14.134	1888	1895	1915	rBV	4960314	7277920	53.24%	6.399%
24	14.440	1940	1947	1966	rVB	2964096	4503525	32.95%	3.960%
25	14.669	1980	1986	2005	rBV	285604	628486	4.60%	0.553%
26	14.881	2015	2022	2029	rVB10	19207	44302	0.32%	0.039%
27	15.198	2068	2076	2080	rBV2	15571	24214	0.18%	0.021%
28	15.440	2110	2117	2131	rBV	6308652	9327025	68.24%	8.201%
29	15.575	2133	2140	2153	rVV	2111443	2931451	21.45%	2.577%
30	15.681	2154	2158	2164	rVB	31481	51913	0.38%	0.046%
31	16.228	2245	2251	2257	rVB8	9577	17422	0.13%	0.015%
32	16.986	2377	2380	2384	rBV3	8196	14680	0.11%	0.013%
33	17.122	2399	2403	2408	rVB7	11326	16788	0.12%	0.015%
34	17.204	2410	2417	2427	rBV	3909551	5565648	40.72%	4.894%
35	17.304	2427	2434	2449	rBV2	7350882	10456062	76.50%	9.193%
36	17.598	2480	2484	2489	rBV6	11474	20644	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012416.D
 Acq On : 01 Nov 2022 08:41
 Operator : CG/JU
 Sample : N5270-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.875	2527	2531	2536	rBV	59046	73691	0.54%	0.065%
38	18.092	2563	2568	2578	rBV	173245	304426	2.23%	0.268%
39	19.004	2721	2723	2727	rBV4	17055	17441	0.13%	0.015%
40	19.122	2738	2743	2748	rBV3	96838	148438	1.09%	0.131%
41	19.192	2751	2755	2759	rBV	98257	142359	1.04%	0.125%
42	19.328	2774	2778	2791	rBV2	153434	288491	2.11%	0.254%
43	19.545	2809	2815	2832	rBV	9698431	12848995	94.00%	11.297%
44	21.298	3108	3113	3123	rBV	5685745	6936778	50.75%	6.099%
45	23.533	3485	3493	3505	rVB2	6718961	13668915	100.00%	12.018%
46	23.686	3512	3519	3532	rVB2	3384904	6731913	49.25%	5.919%




Sum of corrected areas: 113735322

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012416.D
Acq On : 01 Nov 2022 08:41
Operator : CG/JU
Sample : N5270-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

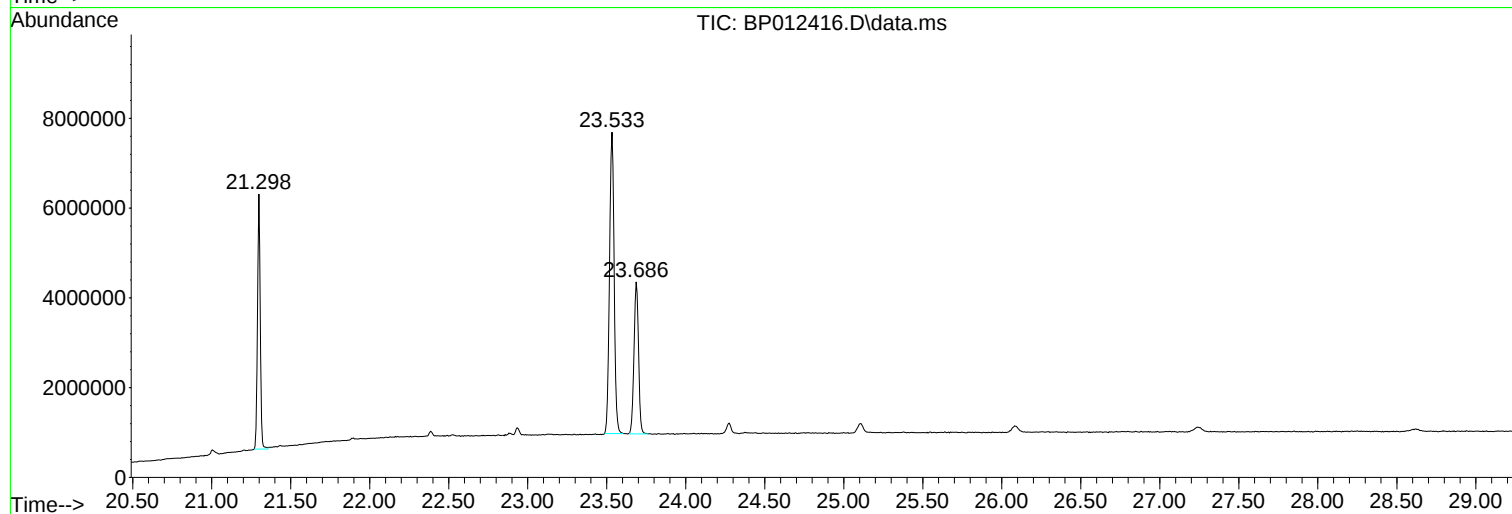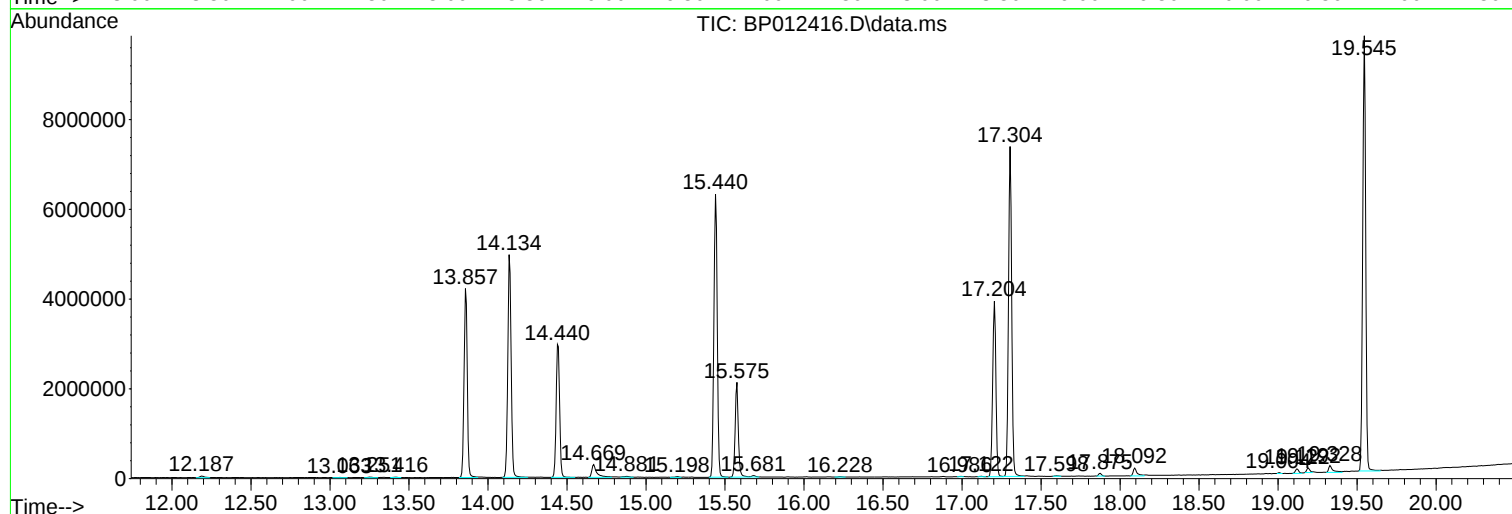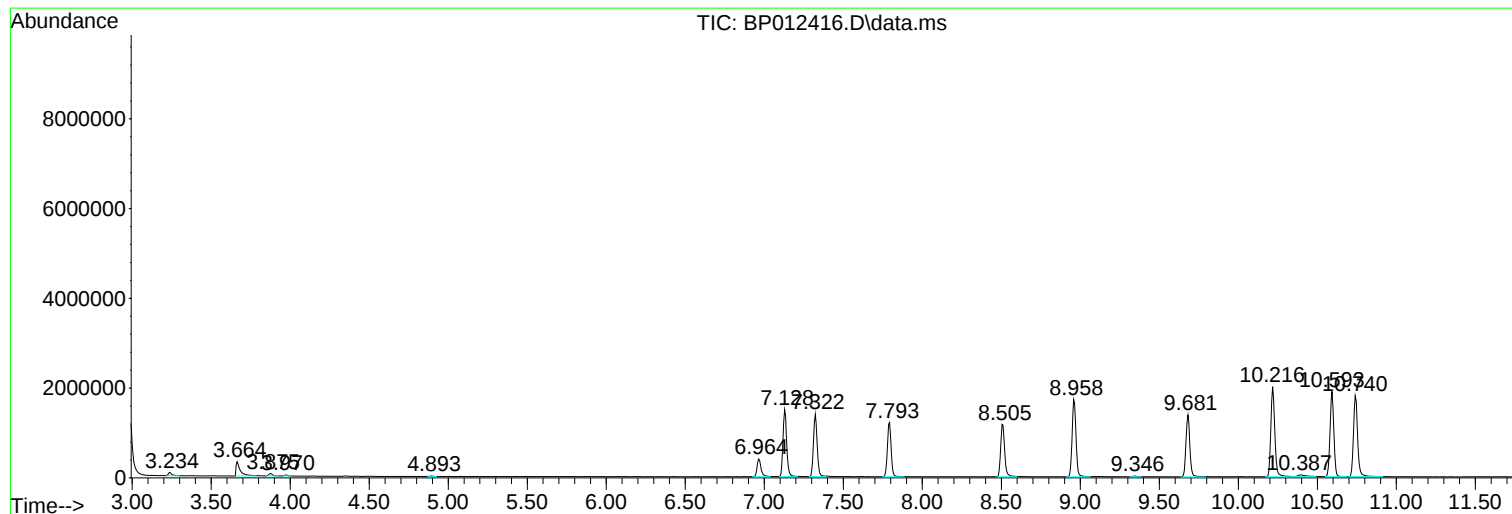

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012416.D
Acq On : 01 Nov 2022 08:41
Operator : CG/JU
Sample : N5270-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012416.D
Acq On : 01 Nov 2022 08:41
Operator : CG/JU
Sample : N5270-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc