

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012417.D
 Acq On : 01 Nov 2022 09:15
 Operator : CG/JU
 Sample : N5270-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	54	rVB	78118	124433	0.86%	0.103%
2	3.669	115	116	139	rBV	108784	233668	1.61%	0.193%
3	3.875	146	151	159	rVV	48735	76717	0.53%	0.063%
4	3.975	163	168	173	rBV	30360	42050	0.29%	0.035%
5	4.887	320	323	333	rVB2	9889	22487	0.15%	0.019%
6	6.963	670	676	696	rBV	420034	754525	5.19%	0.622%
7	7.128	697	704	723	rBV	1630669	2647588	18.20%	2.184%
8	7.322	730	737	748	rBV	1481309	2401013	16.51%	1.981%
9	7.787	807	816	825	rBV	1180383	1967586	13.53%	1.623%
10	7.852	825	827	836	rVB5	13287	27953	0.19%	0.023%
11	8.504	931	938	956	rBV	1230235	2137174	14.69%	1.763%
12	8.957	1008	1015	1028	rBV	1889730	3206226	22.04%	2.645%
13	9.340	1074	1080	1086	rVB	30199	51728	0.36%	0.043%
14	9.681	1130	1138	1154	rBV	1506622	2578266	17.73%	2.127%
15	10.216	1220	1229	1248	rBV	2215902	3828754	26.32%	3.158%
16	10.381	1251	1257	1279	rVV	204634	527566	3.63%	0.435%
17	10.593	1285	1293	1310	rVB	1849273	3104153	21.34%	2.561%
18	10.740	1311	1318	1340	rVB	1311539	2331815	16.03%	1.924%
19	12.187	1557	1564	1573	rBV2	39116	71103	0.49%	0.059%
20	13.040	1706	1709	1716	rBV7	7695	14874	0.10%	0.012%
21	13.257	1738	1746	1750	rBV2	27234	44623	0.31%	0.037%
22	13.334	1755	1759	1764	rVV6	11622	20846	0.14%	0.017%
23	13.416	1768	1773	1778	rVB3	10406	17889	0.12%	0.015%
24	13.857	1838	1848	1861	rBV	4645633	6675518	45.90%	5.507%
25	13.969	1862	1867	1876	rVB7	20337	45242	0.31%	0.037%
26	14.134	1884	1895	1912	rBV	5132750	8144962	56.00%	6.719%
27	14.257	1912	1916	1923	rVV2	15088	36151	0.25%	0.030%
28	14.328	1926	1928	1933	rVB3	12939	15698	0.11%	0.013%
29	14.439	1940	1947	1959	rBV	2871648	4380513	30.12%	3.614%
30	14.669	1980	1986	2004	rBV	320151	698573	4.80%	0.576%
31	14.881	2014	2022	2031	rVV4	49519	101891	0.70%	0.084%
32	14.957	2031	2035	2043	rVB10	8509	21871	0.15%	0.018%
33	15.198	2071	2076	2080	rBV	36472	51312	0.35%	0.042%
34	15.286	2086	2091	2095	rVB4	15380	23526	0.16%	0.019%
35	15.439	2110	2117	2130	rBV	7199557	10389102	71.43%	8.570%
36	15.575	2133	2140	2154	rBV	2350103	3403480	23.40%	2.808%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012417.D
 Acq On : 01 Nov 2022 09:15
 Operator : CG/JU
 Sample : N5270-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.681	2154	2158	2164	rVB	35369	53183	0.37%	0.044%
38	15.898	2191	2195	2199	rBV6	13152	17547	0.12%	0.014%
39	16.881	2358	2362	2369	rBV9	9994	17765	0.12%	0.015%
40	16.998	2377	2382	2389	rVB4	10412	26582	0.18%	0.022%
41	17.116	2399	2402	2410	rBV3	31823	42855	0.29%	0.035%
42	17.204	2410	2417	2427	rBV	3851671	5441946	37.42%	4.489%
43	17.304	2427	2434	2446	rBV2	8126928	11842120	81.42%	9.769%
44	17.598	2480	2484	2489	rBV6	16874	30566	0.21%	0.025%
45	17.692	2497	2500	2503	rBV5	11986	16510	0.11%	0.014%
46	17.875	2526	2531	2537	rBV	133968	171820	1.18%	0.142%
47	18.092	2563	2568	2578	rBV	286571	491009	3.38%	0.405%
48	19.122	2738	2743	2749	rBV2	119105	177875	1.22%	0.147%
49	19.192	2750	2755	2759	rBV	132164	199397	1.37%	0.164%
50	19.327	2774	2778	2787	rBV2	218528	363991	2.50%	0.300%
51	19.545	2809	2815	2828	rBV	10717759	14511859	99.78%	11.971%
52	21.004	3060	3063	3072	rBV4	198043	377141	2.59%	0.311%
53	21.298	3108	3113	3124	rBV	5239677	6606523	45.42%	5.450%
54	23.533	3486	3493	3506	rVB2	7041807	14544450	100.00%	11.998%
55	23.686	3513	3519	3533	rVB2	3044434	6069267	41.73%	5.007%




Sum of corrected areas: 121223282

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012417.D
Acq On : 01 Nov 2022 09:15
Operator : CG/JU
Sample : N5270-09
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA94

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

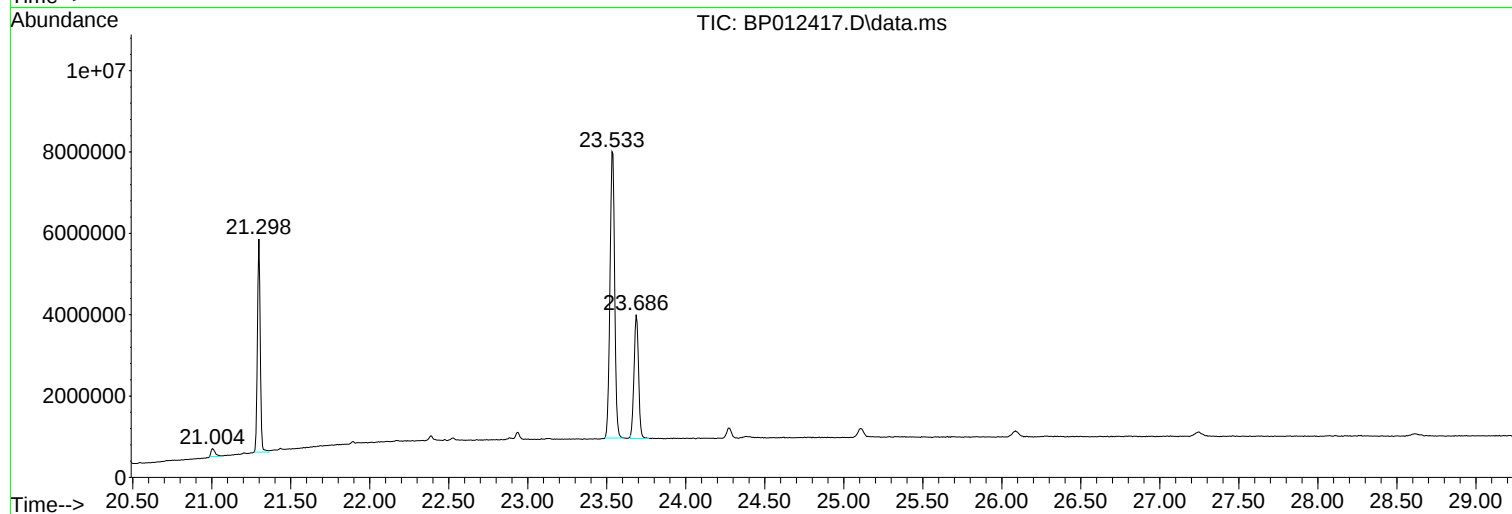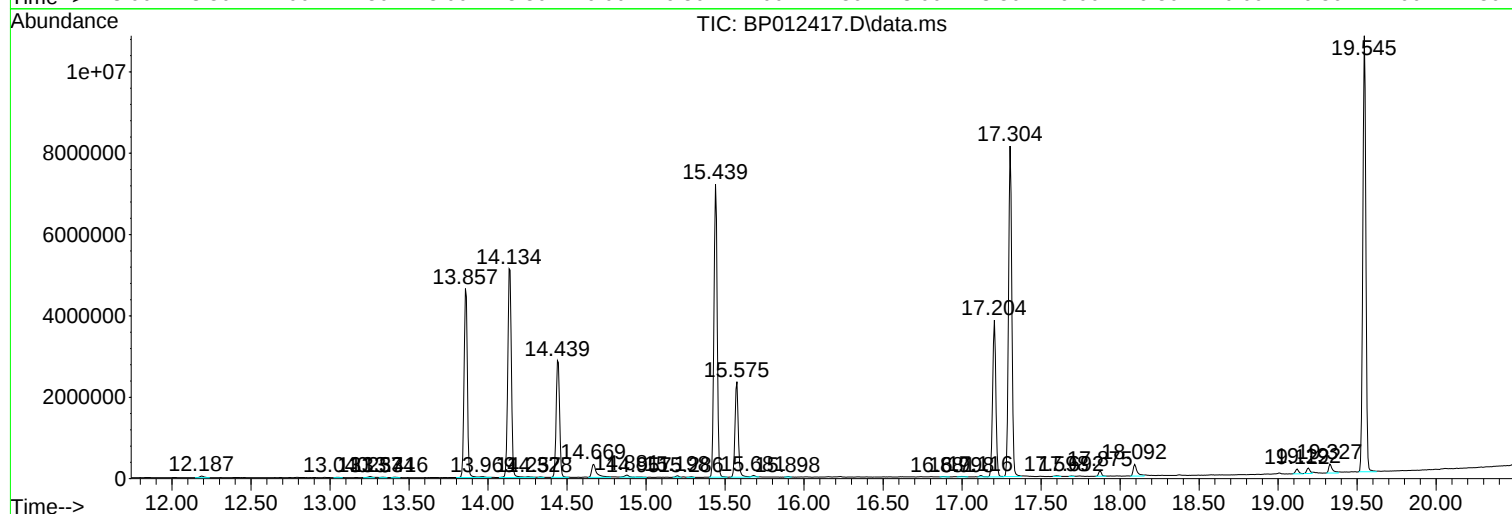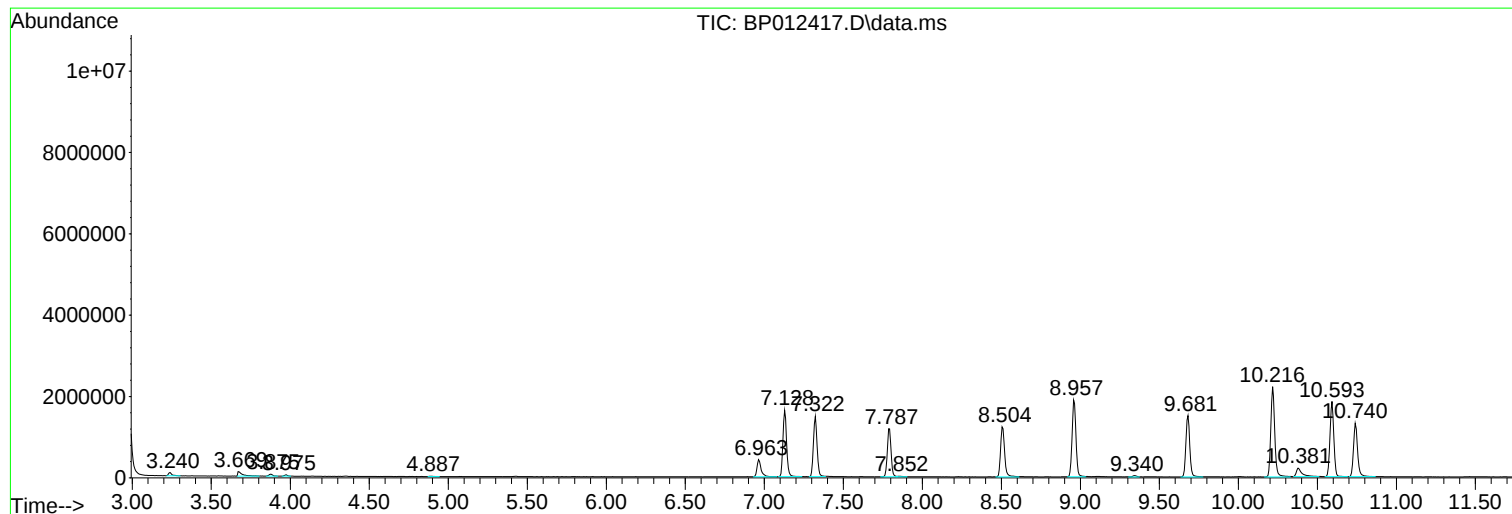

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012417.D
Acq On : 01 Nov 2022 09:15
Operator : CG/JU
Sample : N5270-09
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA94










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.381	3.40 ng/ul	527566	Naphthalene-d8	10.593

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

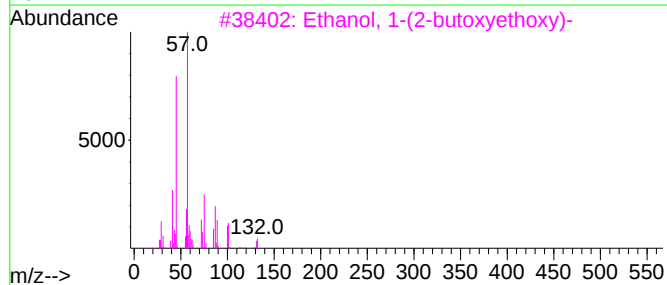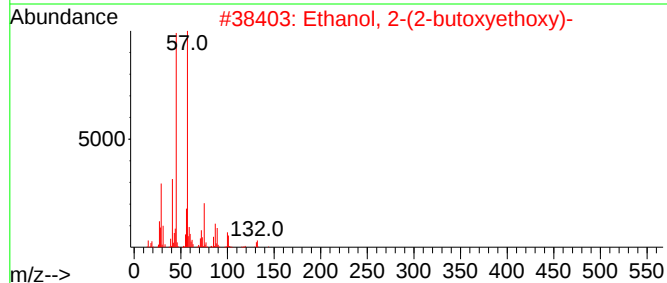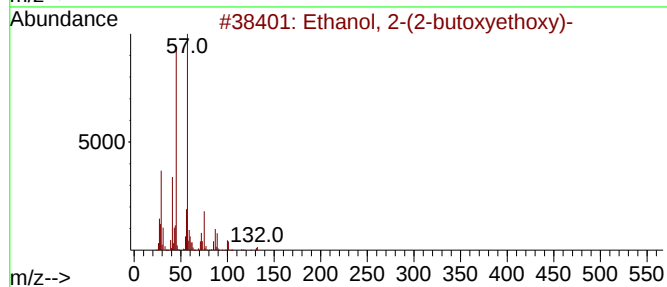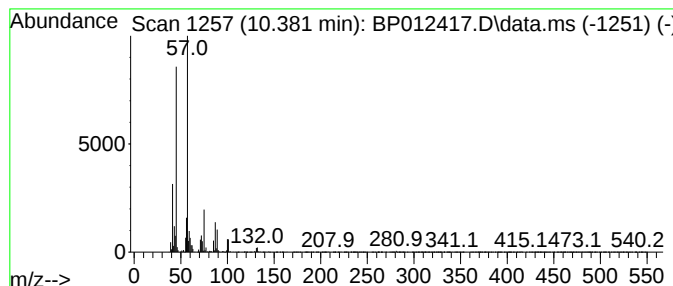

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012417.D
Acq On : 01 Nov 2022 09:15
Operator : CG/JU
Sample : N5270-09
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA94

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.381	3.4	ng/u1	527566	2	10.593	3104150	20.0