

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012420.D
 Acq On : 01 Nov 2022 10:58
 Operator : CG/JU
 Sample : N5270-13
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	50	rBV	66161	95417	0.63%	0.080%
2	3.664	112	115	142	rBV	336279	661901	4.39%	0.553%
3	3.875	146	151	163	rVV	49519	91652	0.61%	0.077%
4	3.970	163	167	174	rVB	26945	40170	0.27%	0.034%
5	6.964	670	676	690	rBV	338470	648530	4.30%	0.542%
6	7.128	697	704	721	rBV	1419874	2316372	15.35%	1.935%
7	7.322	730	737	749	rBV	1263136	2067714	13.70%	1.727%
8	7.793	807	817	826	rBV	1256392	2085848	13.82%	1.742%
9	8.505	932	938	956	rBV	1081675	1908696	12.65%	1.594%
10	8.958	1006	1015	1031	rBV	1635909	2824868	18.72%	2.359%
11	9.346	1076	1081	1086	rVB	27860	41731	0.28%	0.035%
12	9.681	1129	1138	1156	rBV	1317424	2243631	14.87%	1.874%
13	10.216	1221	1229	1251	rBV	1938638	3425168	22.70%	2.861%
14	10.381	1251	1257	1275	rVV	175430	437335	2.90%	0.365%
15	10.593	1283	1293	1306	rVB	1913717	3275536	21.71%	2.736%
16	10.740	1311	1318	1340	rBV	1861671	3280112	21.74%	2.740%
17	12.187	1557	1564	1571	rBV	34286	64319	0.43%	0.054%
18	12.534	1614	1623	1632	rBV2	13599	33909	0.22%	0.028%
19	13.040	1704	1709	1718	rVB10	12585	22717	0.15%	0.019%
20	13.251	1740	1745	1749	rBV2	21329	31808	0.21%	0.027%
21	13.299	1749	1753	1756	rVV3	21210	33080	0.22%	0.028%
22	13.334	1756	1759	1765	rVB3	13003	21687	0.14%	0.018%
23	13.410	1765	1772	1779	rVB6	11607	26954	0.18%	0.023%
24	13.857	1840	1848	1861	rBV	4508622	6254640	41.45%	5.224%
25	13.951	1862	1864	1870	rVB7	10035	16843	0.11%	0.014%
26	14.134	1888	1895	1914	rVB	5007575	7380114	48.91%	6.164%
27	14.334	1924	1929	1935	rVB4	13342	21704	0.14%	0.018%
28	14.440	1937	1947	1959	rBV	3073409	4649808	30.81%	3.884%
29	14.669	1980	1986	2008	rBV	297432	662946	4.39%	0.554%
30	14.875	2015	2021	2030	rVB	21502	50317	0.33%	0.042%
31	15.287	2087	2091	2096	rVB3	14148	20543	0.14%	0.017%
32	15.440	2110	2117	2133	rBV	6757243	9792133	64.89%	8.179%
33	15.575	2133	2140	2154	rBV	2267265	3249956	21.54%	2.714%
34	15.681	2154	2158	2165	rVB2	34911	59111	0.39%	0.049%
35	15.898	2191	2195	2200	rVB5	14418	19407	0.13%	0.016%
36	16.228	2248	2251	2255	rVB4	11523	16997	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012420.D
 Acq On : 01 Nov 2022 10:58
 Operator : CG/JU
 Sample : N5270-13
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.881	2357	2362	2367	rBV6	10129	19476	0.13%	0.016%
38	17.004	2377	2383	2389	rVB5	10289	25720	0.17%	0.021%
39	17.122	2399	2403	2409	rVB2	27953	35308	0.23%	0.029%
40	17.204	2410	2417	2427	rBV	4012441	5661603	37.52%	4.729%
41	17.304	2427	2434	2445	rBV2	7888372	11410893	75.62%	9.531%
42	17.598	2480	2484	2491	rBV6	17765	31174	0.21%	0.026%
43	17.875	2527	2531	2535	rBV	76982	93743	0.62%	0.078%
44	18.092	2563	2568	2578	rBV	295330	503918	3.34%	0.421%
45	19.122	2739	2743	2748	rBV	117198	154546	1.02%	0.129%
46	19.192	2750	2755	2758	rBV	129182	180885	1.20%	0.151%
47	19.328	2774	2778	2788	rBV	207200	324954	2.15%	0.271%
48	19.545	2809	2815	2827	rBV	10182450	14093575	93.40%	11.772%
49	21.010	3060	3064	3074	rBV	324490	603846	4.00%	0.504%
50	21.298	3108	3113	3122	rBV	5376455	6945354	46.03%	5.801%
51	23.533	3486	3493	3508	rVB2	7450801	15090148	100.00%	12.604%
52	23.686	3513	3519	3529	rVB2	3405448	6677150	44.25%	5.577%




Sum of corrected areas: 119725967

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012420.D
Acq On : 01 Nov 2022 10:58
Operator : CG/JU
Sample : N5270-13
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

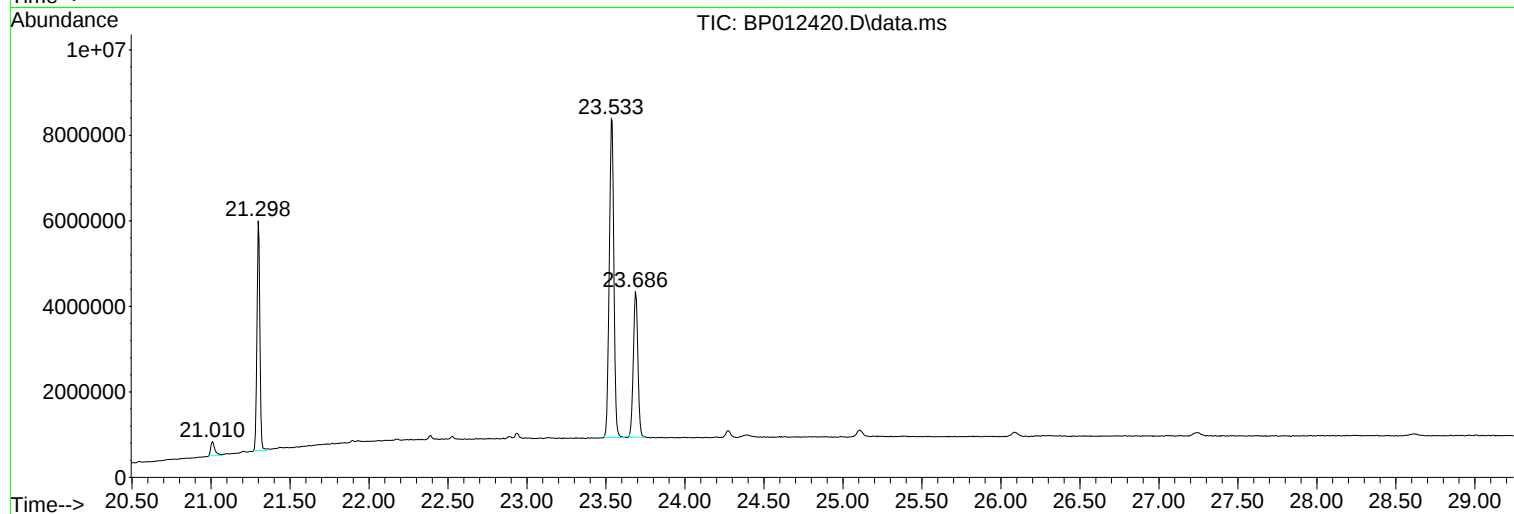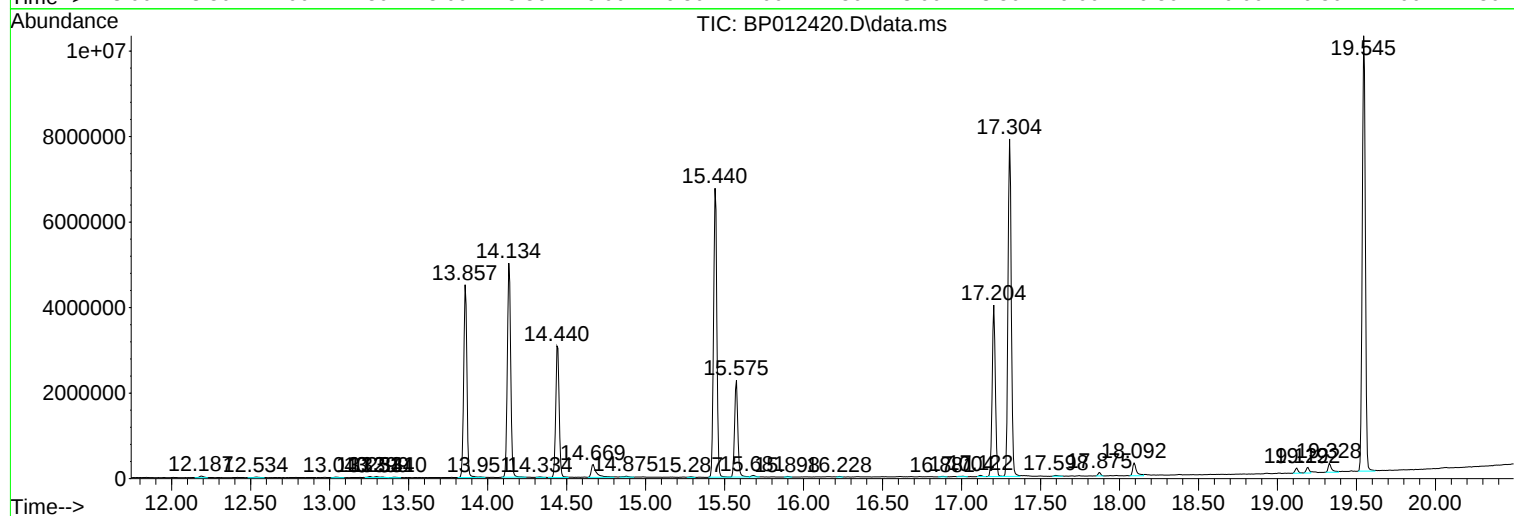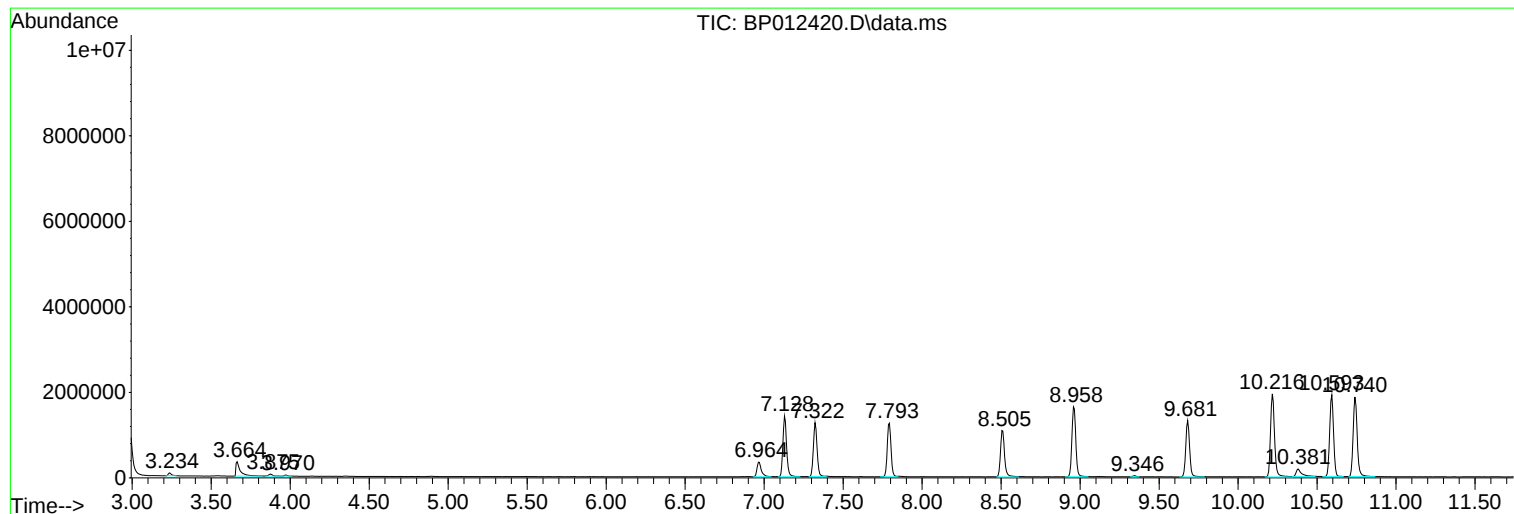

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012420.D
Acq On : 01 Nov 2022 10:58
Operator : CG/JU
Sample : N5270-13
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA69










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.381	2.67 ng/ul	437335	Naphthalene-d8	10.593

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83

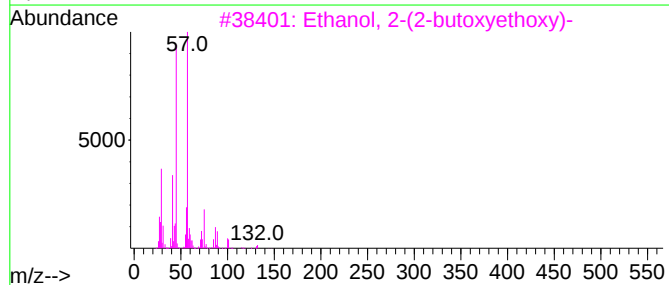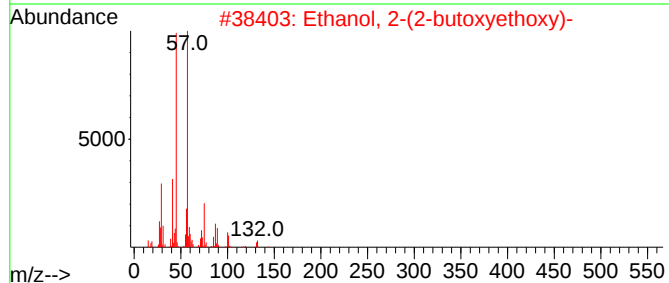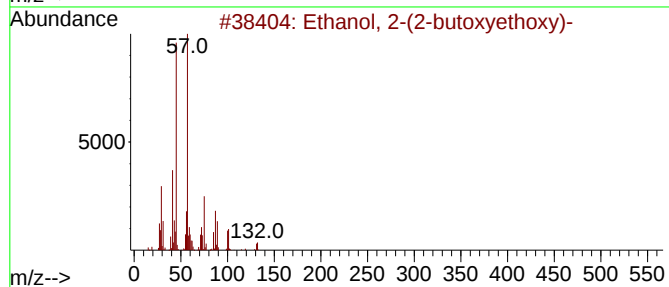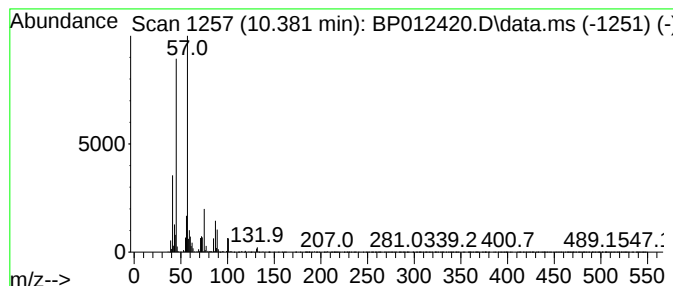

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012420.D
Acq On : 01 Nov 2022 10:58
Operator : CG/JU
Sample : N5270-13
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA69

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.381	2.7	ng/u1	437335	2	10.593	3275540	20.0