

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012427.D
 Acq On : 01 Nov 2022 14:59
 Operator : CG/JU
 Sample : PB148496BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK496

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	50	rVB	80479	111481	1.24%	0.125%
2	3.658	110	114	147	rBV	931086	1614512	18.03%	1.810%
3	3.969	163	167	173	rVB	34523	46727	0.52%	0.052%
4	6.963	669	676	690	rBV	1263899	2101462	23.47%	2.356%
5	7.128	698	704	716	rBV	1093121	1764492	19.70%	1.979%
6	7.322	730	737	748	rBV	1271947	2073349	23.15%	2.325%
7	7.793	810	817	833	rBV	1034885	1766811	19.73%	1.981%
8	8.505	931	938	955	rBV	1554518	2718580	30.36%	3.048%
9	8.957	1008	1015	1034	rBV	1263876	2162540	24.15%	2.425%
10	9.681	1131	1138	1154	rBV	1031703	1765545	19.72%	1.980%
11	10.216	1222	1229	1248	rBV	1526573	2714558	30.31%	3.044%
12	10.593	1285	1293	1304	rBV	1649442	2768767	30.92%	3.105%
13	10.740	1311	1318	1343	rBV	1486053	2822581	31.52%	3.165%
14	12.193	1559	1565	1577	rBV2	18160	46439	0.52%	0.052%
15	13.857	1840	1848	1861	rBV	2957902	4258359	47.55%	4.775%
16	14.134	1888	1895	1909	rBV	3497494	5261371	58.76%	5.900%
17	14.440	1940	1947	1964	rBV	2719483	3905715	43.62%	4.379%
18	14.663	1978	1985	2007	rBV	1138415	2140141	23.90%	2.400%
19	14.857	2015	2018	2030	rVB	9936	27194	0.30%	0.030%
20	15.439	2110	2117	2132	rBV	4600295	6601545	73.72%	7.402%
21	15.575	2134	2140	2154	rVV	1374548	1991872	22.24%	2.233%
22	15.681	2154	2158	2165	rVB	27230	46727	0.52%	0.052%
23	16.228	2247	2251	2257	rVB8	6624	10446	0.12%	0.012%
24	16.881	2359	2362	2368	rVB7	6338	9888	0.11%	0.011%
25	16.998	2376	2382	2385	rBV5	9052	19274	0.22%	0.022%
26	17.204	2410	2417	2427	rBV	3343147	4803450	53.64%	5.386%
27	17.304	2427	2434	2453	rVV	5006388	7337898	81.95%	8.228%
28	19.122	2739	2743	2748	rBV2	64560	87922	0.98%	0.099%
29	19.192	2751	2755	2759	rVV	56787	81724	0.91%	0.092%
30	19.545	2809	2815	2827	rBV	6797065	8954623	100.00%	10.041%
31	21.298	3108	3113	3122	rBV	4290851	5643562	63.02%	6.328%
32	23.533	3486	3493	3507	rVB2	4241552	8476561	94.66%	9.505%
33	23.686	3513	3519	3531	rVB2	2504096	5045684	56.35%	5.658%




Sum of corrected areas: 89181800

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012427.D
Acq On : 01 Nov 2022 14:59
Operator : CG/JU
Sample : PB148496BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

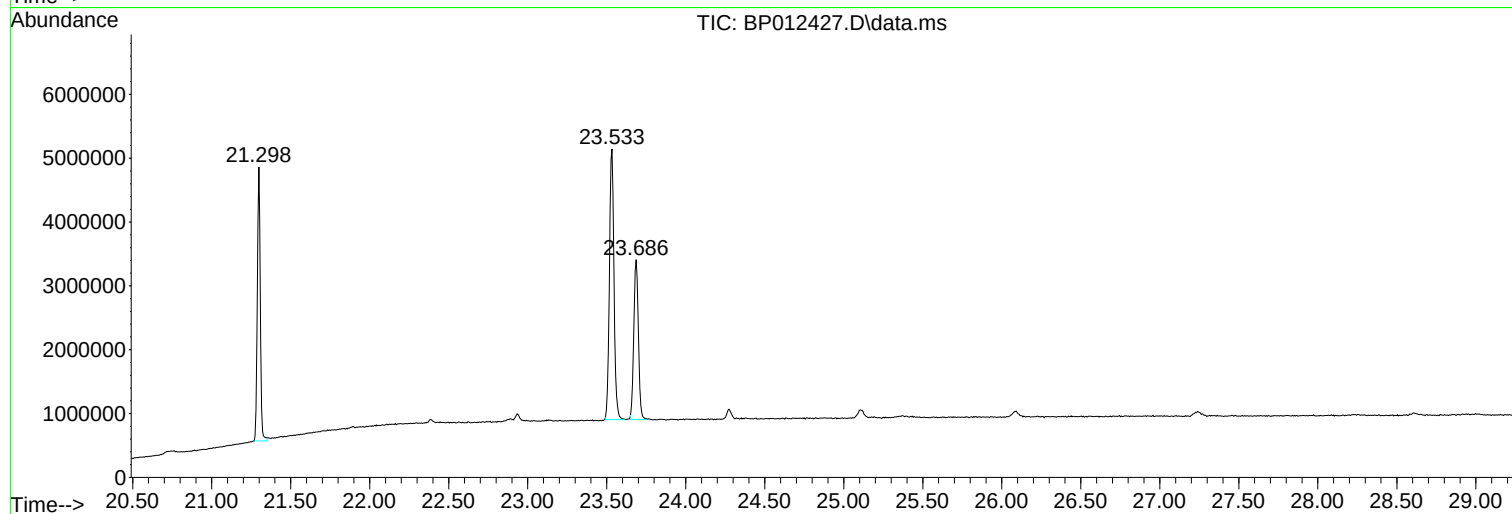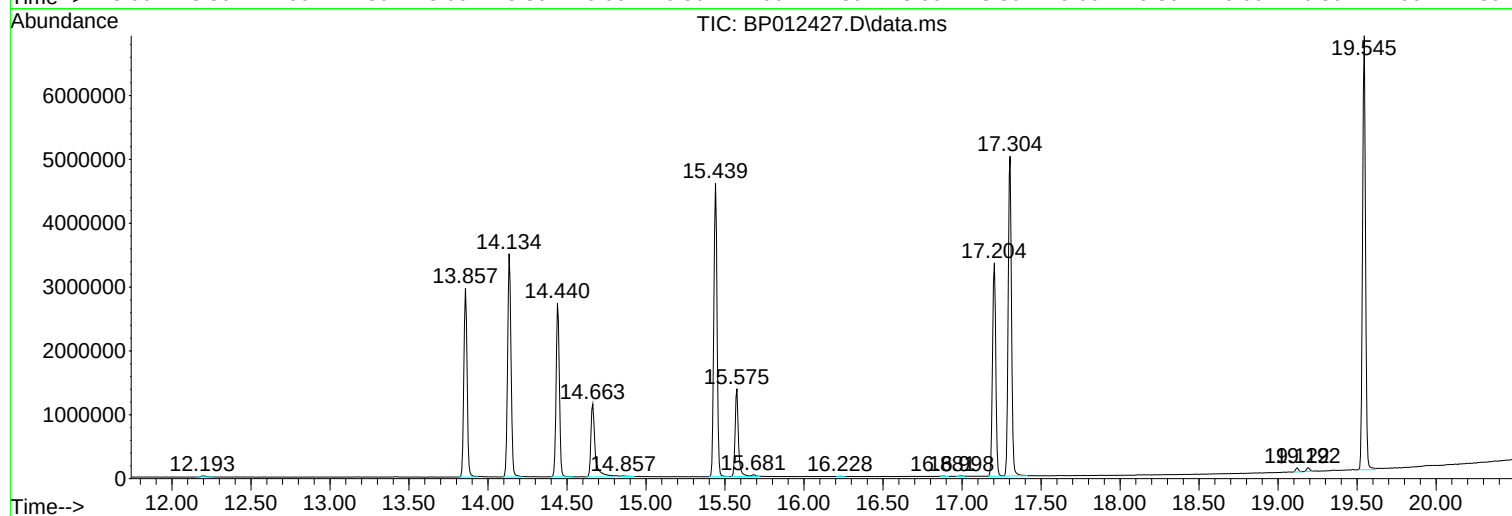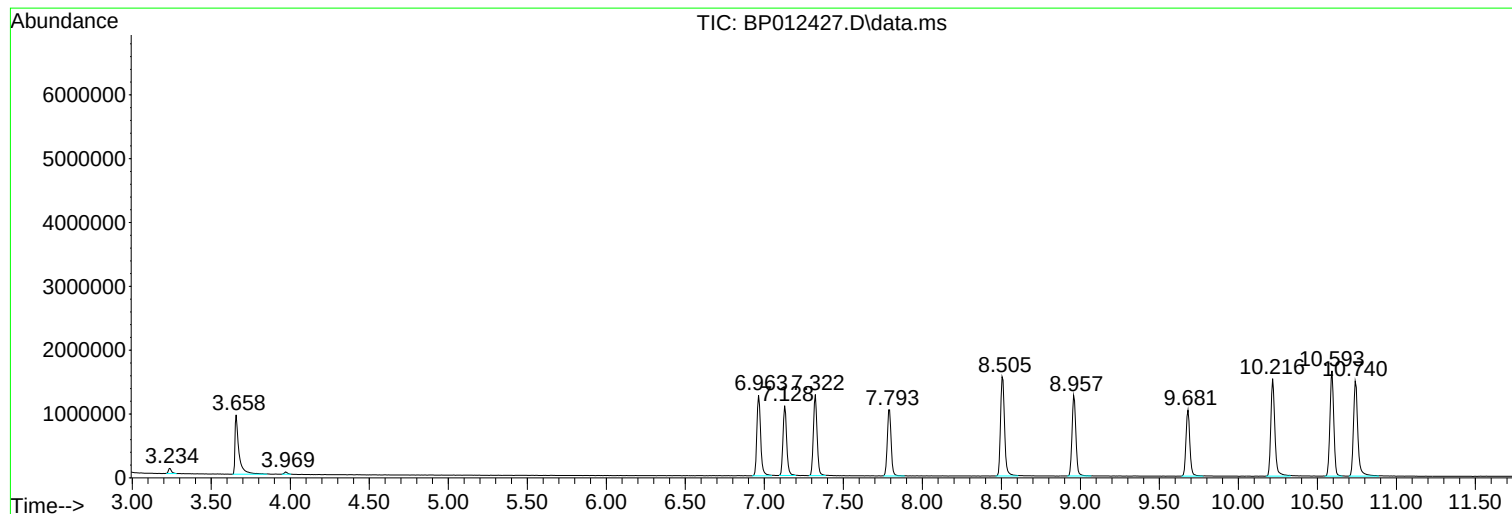

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012427.D
Acq On : 01 Nov 2022 14:59
Operator : CG/JU
Sample : PB148496BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012427.D
Acq On : 01 Nov 2022 14:59
Operator : CG/JU
Sample : PB148496BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK496

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc