

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012428.D
 Acq On : 01 Nov 2022 15:34
 Operator : CG/JU
 Sample : PB148597BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	51	rVB	91405	126481	1.29%	0.134%
2	3.658	110	114	141	rBV	1079382	1835308	18.65%	1.938%
3	3.970	164	167	179	rVB	38145	61296	0.62%	0.065%
4	6.963	669	676	693	rBV	1415470	2334333	23.72%	2.465%
5	7.128	698	704	718	rVB	1228509	1967488	19.99%	2.078%
6	7.322	729	737	751	rBV	1422230	2316251	23.53%	2.446%
7	7.793	810	817	832	rBV	1017636	1688856	17.16%	1.784%
8	8.505	931	938	959	rBV	1773006	3036606	30.85%	3.207%
9	8.957	1007	1015	1029	rBV	1420521	2413766	24.53%	2.549%
10	9.681	1130	1138	1156	rBV	1172921	1971534	20.03%	2.082%
11	10.216	1221	1229	1250	rBV	1697858	3036705	30.86%	3.207%
12	10.593	1284	1293	1307	rBV	1577288	2685412	27.29%	2.836%
13	10.740	1311	1318	1343	rBV	1687120	3148291	31.99%	3.325%
14	12.193	1560	1565	1575	rBV2	19688	44333	0.45%	0.047%
15	13.334	1754	1759	1765	rBV8	6388	11073	0.11%	0.012%
16	13.857	1839	1848	1861	rBV	3374268	4806205	48.83%	5.076%
17	14.134	1888	1895	1915	rBV	4026882	5902776	59.98%	6.234%
18	14.440	1940	1947	1959	rBV	2495719	3808930	38.70%	4.023%
19	14.663	1978	1985	2008	rBV	1355746	2432952	24.72%	2.570%
20	14.851	2015	2017	2026	rVB10	10943	22558	0.23%	0.024%
21	15.440	2110	2117	2129	rBV	5131158	7428529	75.48%	7.846%
22	15.575	2133	2140	2153	rBV	1535443	2261117	22.97%	2.388%
23	15.681	2154	2158	2164	rVB	28324	48193	0.49%	0.051%
24	16.881	2353	2362	2366	rBV	9208	19129	0.19%	0.020%
25	16.986	2376	2380	2385	rBV2	7865	12463	0.13%	0.013%
26	17.204	2410	2417	2426	rBV	3286052	4692463	47.68%	4.956%
27	17.304	2427	2434	2455	rVV	5650911	8230976	83.63%	8.693%
28	19.122	2739	2743	2749	rBV3	72797	103518	1.05%	0.109%
29	19.192	2751	2755	2759	rBV	66578	92751	0.94%	0.098%
30	19.545	2809	2815	2824	rBV	7441963	9841769	100.00%	10.395%
31	21.298	3108	3113	3122	rBV	4043287	5205545	52.89%	5.498%
32	23.533	3486	3493	3506	rVB2	4196271	8687987	88.28%	9.176%
33	23.686	3513	3519	3532	rVB	2259412	4406015	44.77%	4.654%




Sum of corrected areas: 94681609

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012428.D
Acq On : 01 Nov 2022 15:34
Operator : CG/JU
Sample : PB148597BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

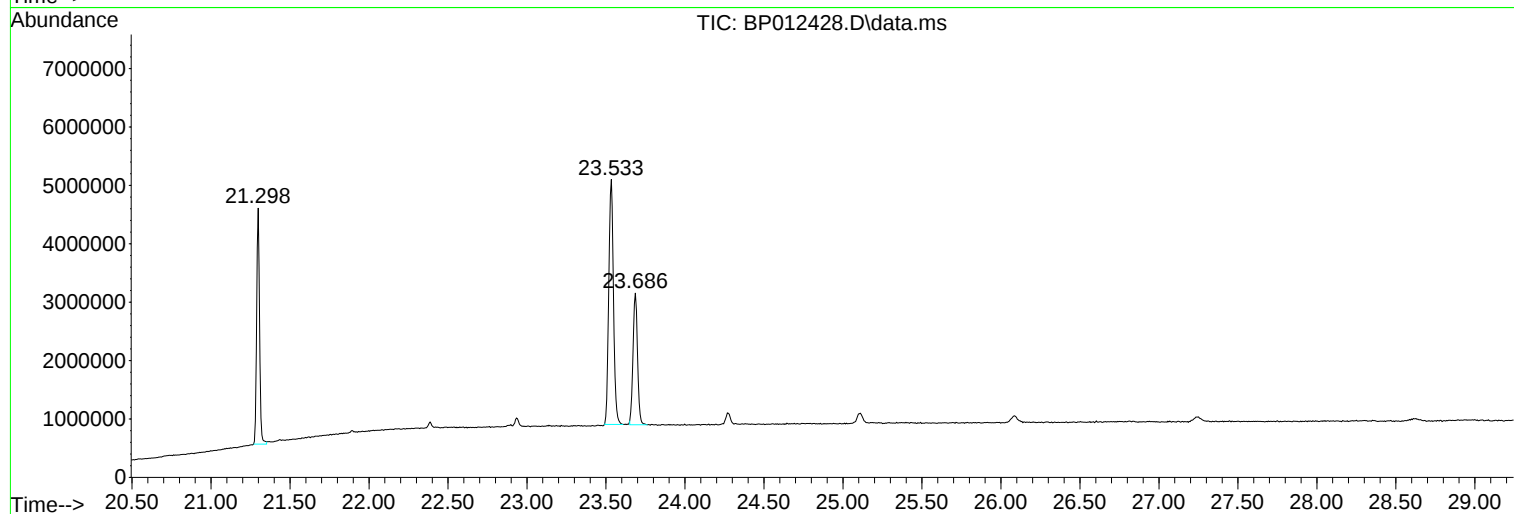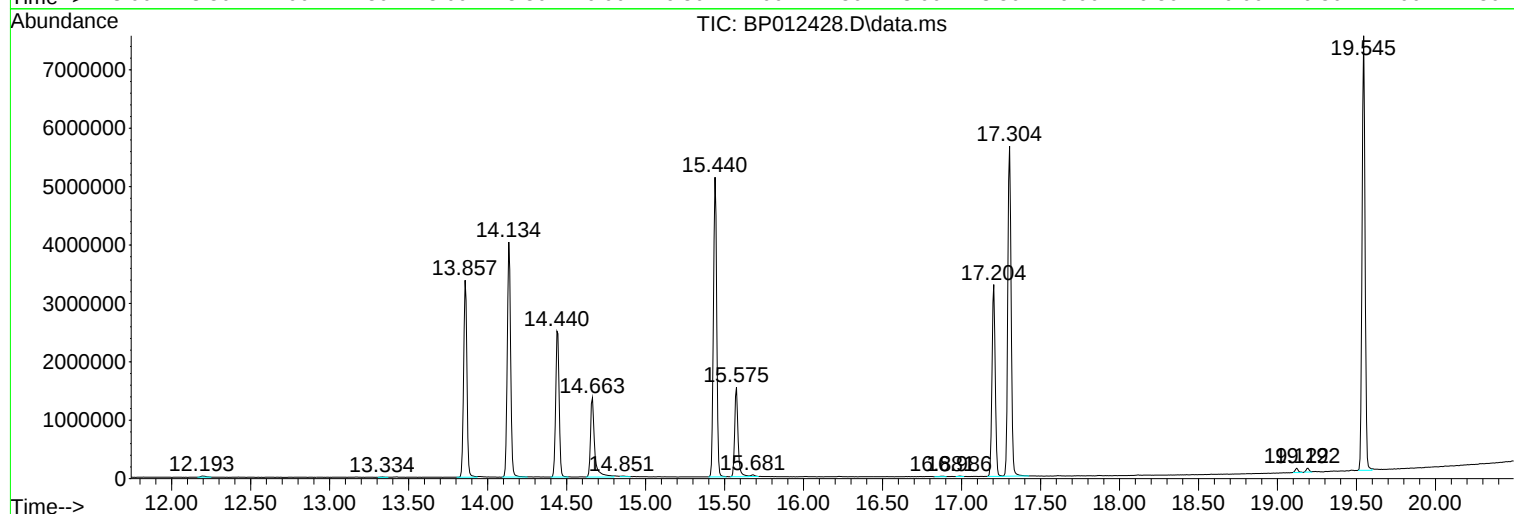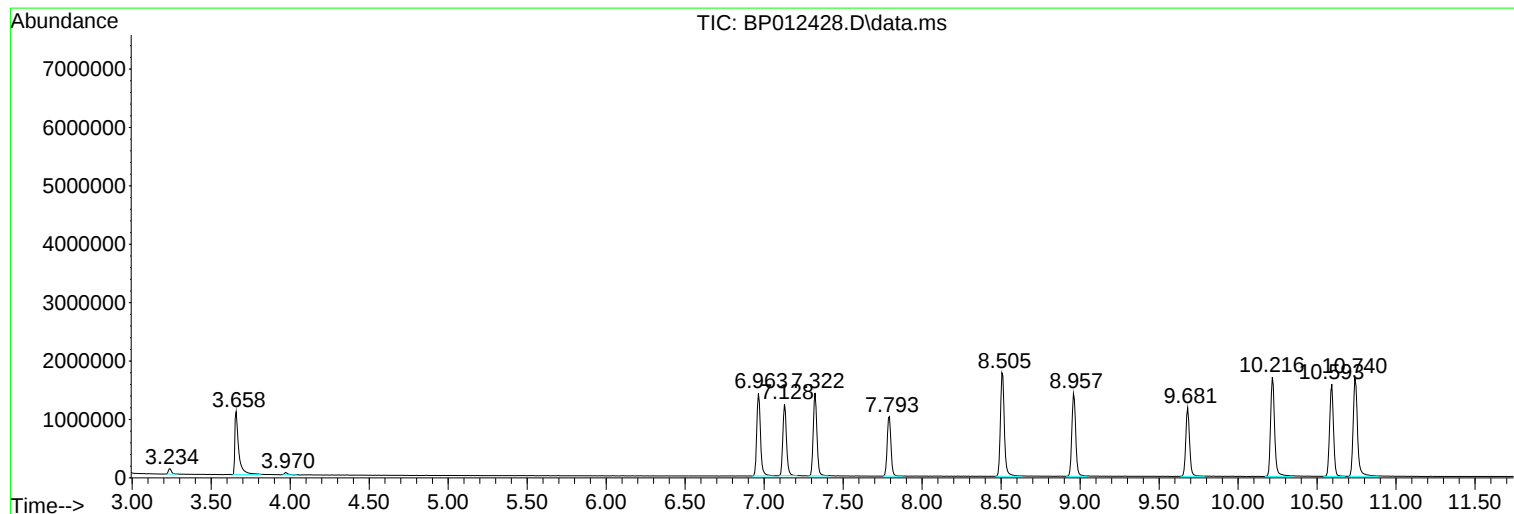

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012428.D
Acq On : 01 Nov 2022 15:34
Operator : CG/JU
Sample : PB148597BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012428.D
Acq On : 01 Nov 2022 15:34
Operator : CG/JU
Sample : PB148597BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc