

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012433.D
 Acq On : 01 Nov 2022 18:27
 Operator : CG/JU
 Sample : N5270-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	52	rVB	64887	101689	0.95%	0.106%
2	3.663	112	115	134	rBV	329225	609891	5.71%	0.634%
3	3.875	146	151	157	rVB	48384	74680	0.70%	0.078%
4	3.969	164	167	174	rVB	23301	35332	0.33%	0.037%
5	6.963	670	676	693	rBV	291708	543026	5.08%	0.564%
6	7.128	697	704	718	rBV	1279676	2068724	19.37%	2.150%
7	7.322	730	737	747	rBV	1114355	1802338	16.88%	1.873%
8	7.793	809	817	826	rBV	1148012	1945809	18.22%	2.022%
9	8.504	932	938	954	rBV	911631	1600839	14.99%	1.663%
10	8.957	1007	1015	1029	rBV	1504404	2565321	24.02%	2.666%
11	9.345	1074	1081	1086	rBV2	17107	27941	0.26%	0.029%
12	9.681	1128	1138	1156	rBV	1135632	1946396	18.22%	2.023%
13	10.216	1221	1229	1251	rBV	1628458	2898620	27.14%	3.012%
14	10.398	1253	1260	1280	rVB3	30276	128604	1.20%	0.134%
15	10.592	1285	1293	1309	rVB	1806020	3109265	29.11%	3.231%
16	10.739	1310	1318	1343	rBV	1583955	2882903	26.99%	2.996%
17	12.186	1558	1564	1574	rBV	27462	53546	0.50%	0.056%
18	13.063	1705	1713	1719	rBV4	12205	28975	0.27%	0.030%
19	13.251	1741	1745	1750	rVV4	12035	18422	0.17%	0.019%
20	13.410	1767	1772	1778	rBV7	6660	13158	0.12%	0.014%
21	13.857	1840	1848	1862	rBV	3626971	5182069	48.52%	5.385%
22	14.133	1888	1895	1914	rVB	4337747	6345872	59.42%	6.594%
23	14.333	1924	1929	1933	rVB6	8555	13163	0.12%	0.014%
24	14.439	1941	1947	1966	rVB	2980421	4437104	41.54%	4.611%
25	14.669	1981	1986	2007	rBV2	154810	412974	3.87%	0.429%
26	14.880	2019	2022	2030	rVB8	13371	22324	0.21%	0.023%
27	15.286	2086	2091	2097	rVB6	11075	17895	0.17%	0.019%
28	15.439	2110	2117	2133	rBV	5718925	8098453	75.82%	8.415%
29	15.574	2133	2140	2152	rBV	1551569	2301197	21.55%	2.391%
30	15.680	2154	2158	2164	rVB3	30163	51835	0.49%	0.054%
31	16.227	2248	2251	2256	rVB6	8125	11239	0.11%	0.012%
32	16.516	2293	2300	2302	rBV8	4646	10903	0.10%	0.011%
33	16.992	2378	2381	2388	rVB4	8633	16216	0.15%	0.017%
34	17.121	2398	2403	2407	rBV8	9587	16579	0.16%	0.017%
35	17.204	2409	2417	2427	rBV	3634549	5432195	50.86%	5.645%
36	17.304	2427	2434	2446	rVV	6329302	8925084	83.56%	9.274%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012433.D
 Acq On : 01 Nov 2022 18:27
 Operator : CG/JU
 Sample : N5270-01
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.874	2527	2531	2537	rVB	21916	29320	0.27%	0.030%
38	18.092	2563	2568	2577	rBV	199465	325607	3.05%	0.338%
39	19.121	2739	2743	2748	rBV2	80757	115603	1.08%	0.120%
40	19.192	2750	2755	2759	rBV	90486	146375	1.37%	0.152%
41	19.327	2774	2778	2787	rBV	125161	211076	1.98%	0.219%
42	19.545	2809	2815	2825	rBV	7918184	10680457	100.00%	11.098%
43	20.545	2982	2985	2989	rBV	92328	109884	1.03%	0.114%
44	21.004	3059	3063	3071	rBV	288815	506690	4.74%	0.527%
45	21.298	3108	3113	3121	rBV	4810426	5933016	55.55%	6.165%
46	21.433	3134	3136	3141	rVB2	159460	152749	1.43%	0.159%
47	23.533	3486	3493	3504	rVB2	4502404	9204126	86.18%	9.564%
48	23.686	3512	3519	3527	rVB2	2562641	5069906	47.47%	5.268%




Sum of corrected areas: 96235390

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012432\
Data File : BP012433.D
Acq On : 01 Nov 2022 18:27
Operator : CG/JU
Sample : N5270-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

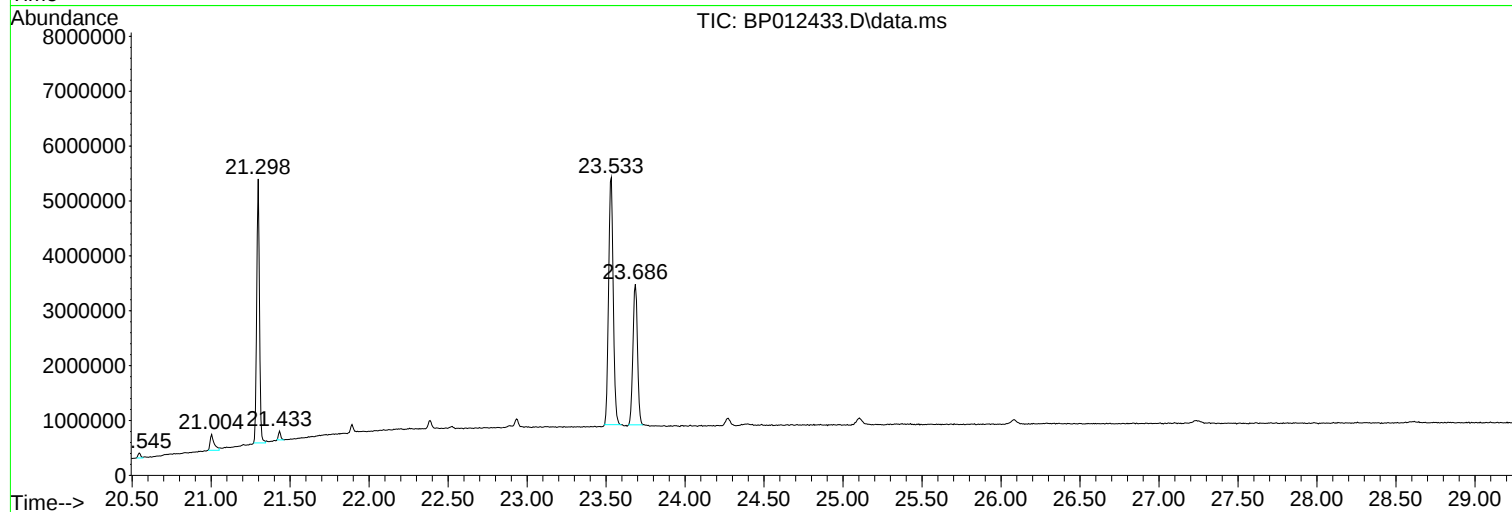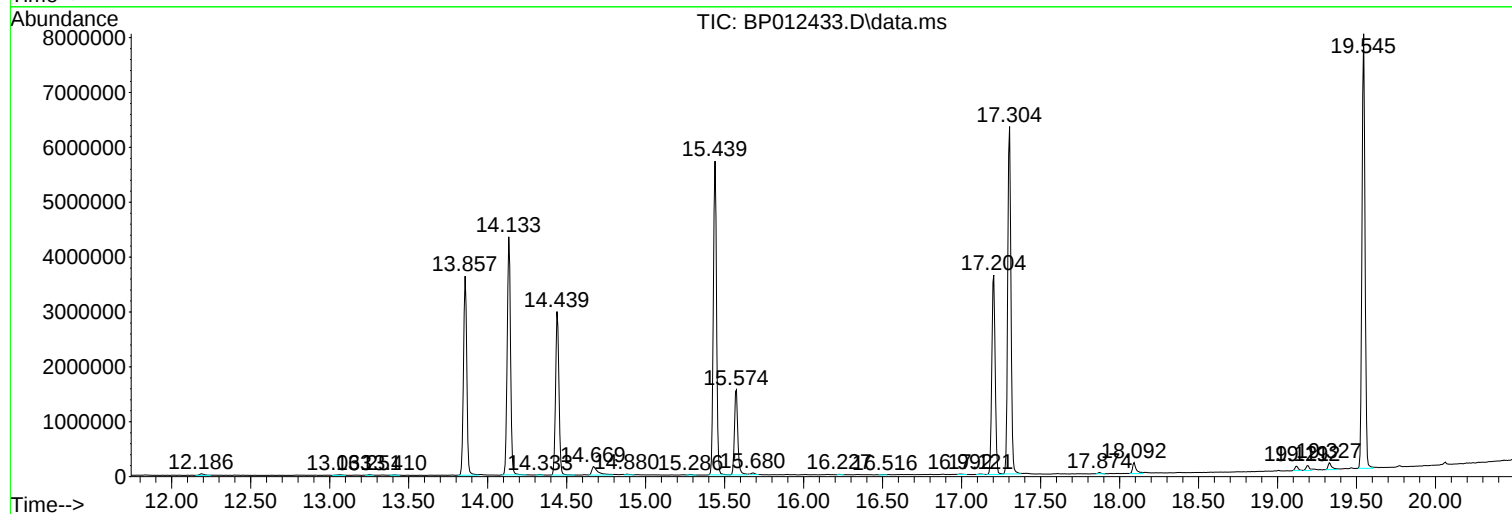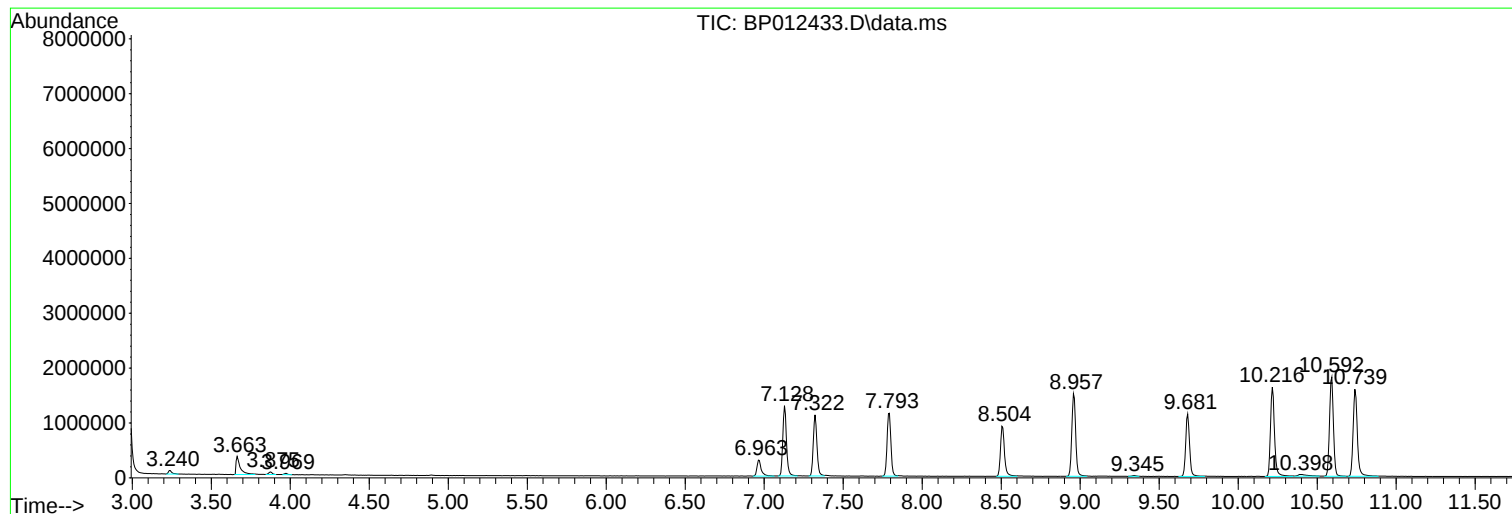

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012433.D
Acq On : 01 Nov 2022 18:27
Operator : CG/JU
Sample : N5270-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012433.D
Acq On : 01 Nov 2022 18:27
Operator : CG/JU
Sample : N5270-01
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc