

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012435.D
 Acq On : 01 Nov 2022 19:36
 Operator : CG/JU
 Sample : N5270-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	52	rVB	69789	102765	0.86%	0.099%
2	3.670	114	116	132	rBV	141667	280493	2.35%	0.270%
3	3.875	146	151	156	rVB	46681	71385	0.60%	0.069%
4	3.969	163	167	173	rVB	26934	38077	0.32%	0.037%
5	4.893	321	324	328	rVB3	8728	12498	0.10%	0.012%
6	6.963	670	676	692	rBV	415392	757866	6.34%	0.729%
7	7.128	697	704	719	rBV	1422960	2336577	19.54%	2.248%
8	7.322	730	737	747	rBV	1344279	2178722	18.22%	2.096%
9	7.787	809	816	825	rBV	1087185	1751916	14.65%	1.686%
10	8.505	931	938	955	rBV	1225585	2077691	17.38%	1.999%
11	8.957	1007	1015	1030	rBV	1737407	2897546	24.23%	2.788%
12	9.340	1074	1080	1086	rVB2	22401	35920	0.30%	0.035%
13	9.681	1129	1138	1155	rBV	1341762	2313479	19.35%	2.226%
14	10.216	1222	1229	1247	rBV	2024292	3537085	29.58%	3.403%
15	10.375	1249	1256	1281	rVV	556945	1252169	10.47%	1.205%
16	10.587	1285	1292	1310	rVB	1593274	2819237	23.58%	2.713%
17	10.740	1310	1318	1338	rBV	1255999	2277102	19.05%	2.191%
18	12.187	1558	1564	1571	rBV2	33847	65332	0.55%	0.063%
19	12.287	1575	1581	1589	rBV8	11330	25439	0.21%	0.024%
20	13.057	1710	1712	1723	rVB5	9844	21572	0.18%	0.021%
21	13.251	1738	1745	1752	rBV4	16269	28455	0.24%	0.027%
22	13.334	1752	1759	1766	rVV	61287	102430	0.86%	0.099%
23	13.410	1766	1772	1778	rVB4	8816	17979	0.15%	0.017%
24	13.857	1841	1848	1861	rBV	4138868	5892993	49.29%	5.670%
25	14.134	1884	1895	1906	rBV2	4838834	7272663	60.83%	6.998%
26	14.328	1921	1928	1932	rBV6	21383	46196	0.39%	0.044%
27	14.440	1940	1947	1960	rVB	2723140	3986117	33.34%	3.836%
28	14.669	1980	1986	2006	rBV	269249	641323	5.36%	0.617%
29	14.875	2015	2021	2028	rVB9	19240	48566	0.41%	0.047%
30	15.234	2078	2082	2086	rBV4	8886	13585	0.11%	0.013%
31	15.287	2086	2091	2095	rVB4	13179	17532	0.15%	0.017%
32	15.439	2110	2117	2131	rBV	6441202	9161438	76.62%	8.815%
33	15.569	2133	2139	2154	rVV	1976659	2924978	24.46%	2.814%
34	15.681	2154	2158	2165	rVB	32988	58451	0.49%	0.056%
35	15.898	2191	2195	2202	rVB3	17902	25236	0.21%	0.024%
36	16.010	2207	2214	2218	rBV8	8992	18594	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
 Data File : BP012435.D
 Acq On : 01 Nov 2022 19:36
 Operator : CG/JU
 Sample : N5270-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHA67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.157	2235	2239	2244	rVB8	8387	13039	0.11%	0.013%
38	16.228	2248	2251	2255	rVB6	9048	12868	0.11%	0.012%
39	16.345	2265	2271	2277	rBV6	8288	21916	0.18%	0.021%
40	16.992	2378	2381	2388	rVB8	10263	23069	0.19%	0.022%
41	17.204	2410	2417	2427	rBV	3387533	4876346	40.78%	4.692%
42	17.304	2427	2434	2445	rBV	6933830	10215454	85.44%	9.830%
43	17.604	2480	2485	2490	rBV8	8393	17307	0.14%	0.017%
44	17.869	2526	2530	2536	rBV	188265	247367	2.07%	0.238%
45	18.092	2563	2568	2578	rBV	215967	382685	3.20%	0.368%
46	18.975	2716	2718	2719	rBV2	20613	16898	0.14%	0.016%
47	19.004	2719	2723	2727	rVV	273940	311279	2.60%	0.300%
48	19.122	2738	2743	2749	rBV2	103338	178385	1.49%	0.172%
49	19.192	2751	2755	2765	rVV	93008	166054	1.39%	0.160%
50	19.328	2774	2778	2786	rBV	141056	235502	1.97%	0.227%
51	19.545	2809	2815	2827	rBV	8857132	11956357	100.00%	11.505%
52	21.010	3060	3064	3072	rBV4	206184	384208	3.21%	0.370%
53	21.298	3108	3113	3120	rBV	4107425	5217329	43.64%	5.020%
54	23.527	3486	3492	3507	rVB2	5046997	10117523	84.62%	9.735%
55	23.680	3512	3518	3531	rVB2	2180965	4422435	36.99%	4.255%




Sum of corrected areas: 103925428

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012435.D
Acq On : 01 Nov 2022 19:36
Operator : CG/JU
Sample : N5270-03
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA67

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

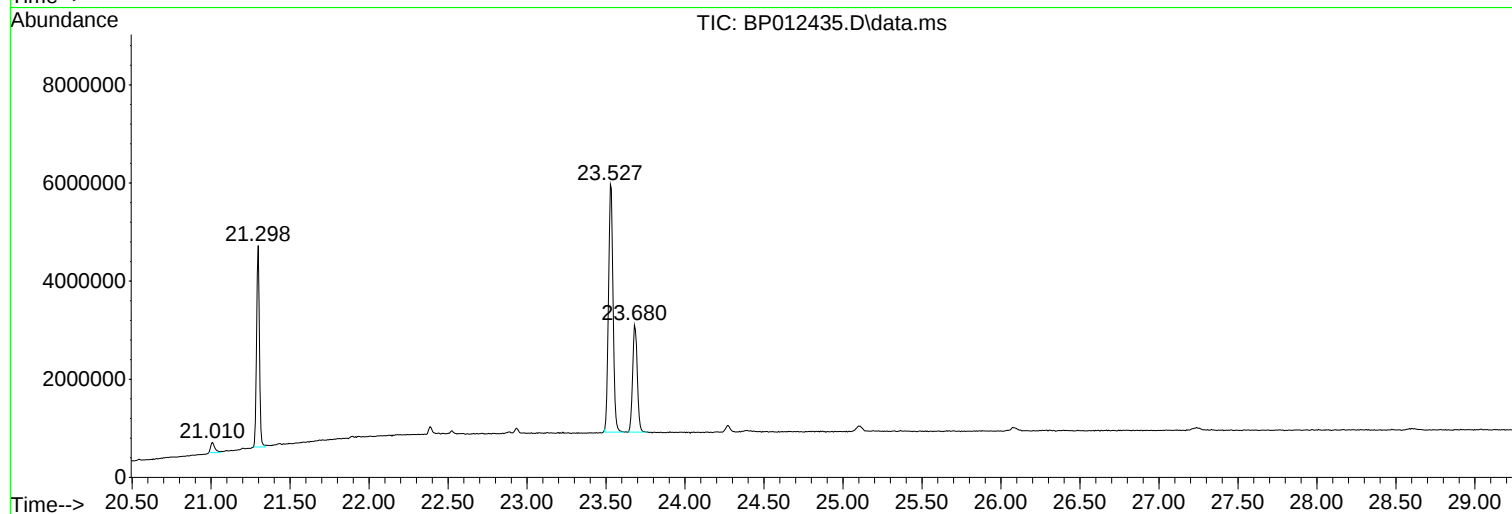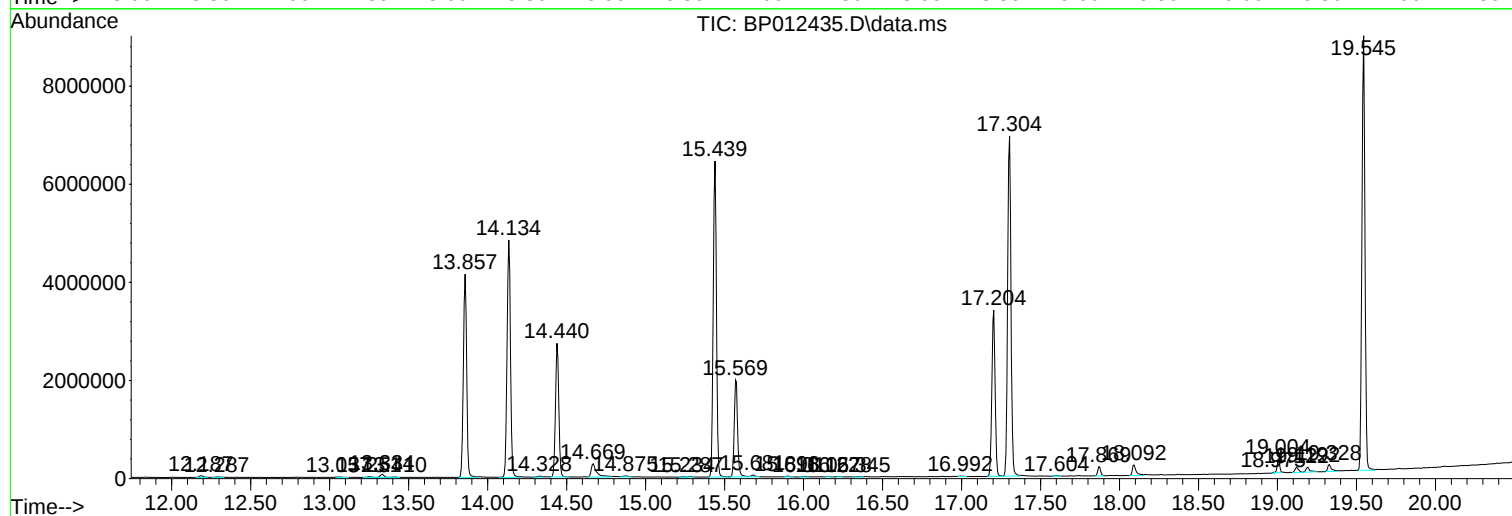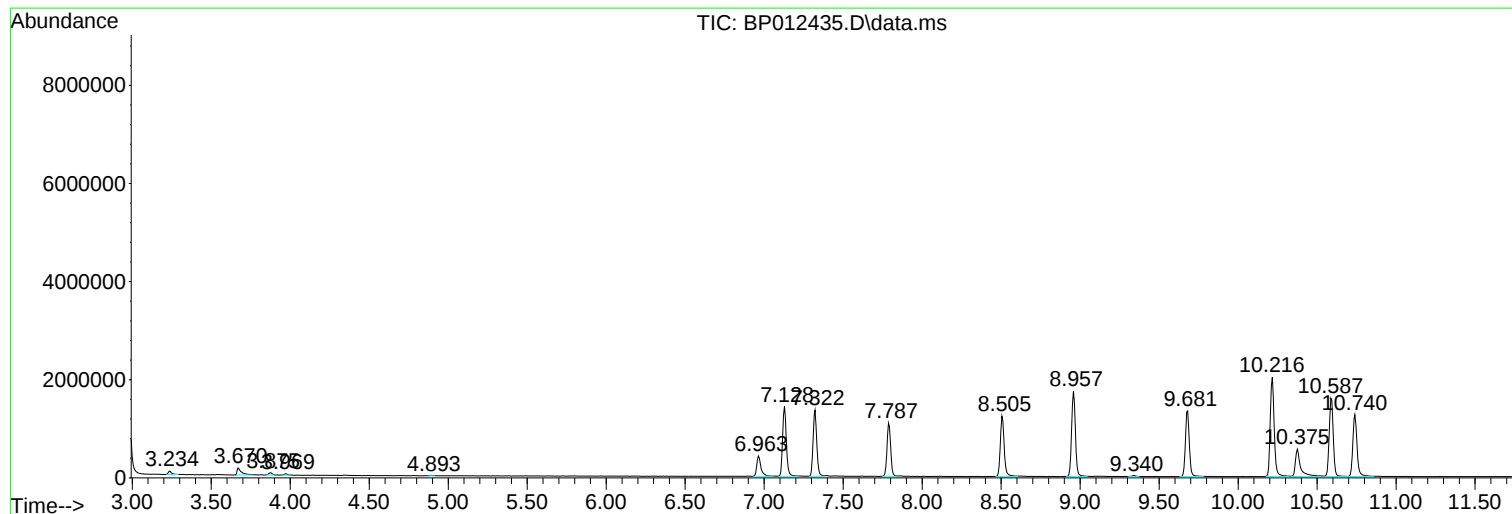

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012435.D
Acq On : 01 Nov 2022 19:36
Operator : CG/JU
Sample : N5270-03
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA67










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.375	8.88 ng/ul	1252170	Naphthalene-d8	10.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

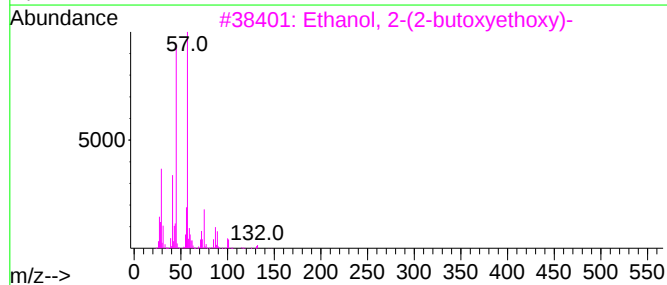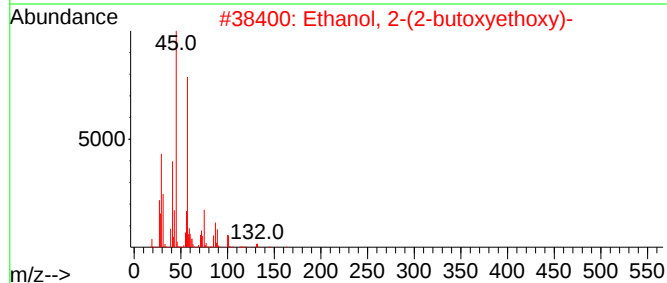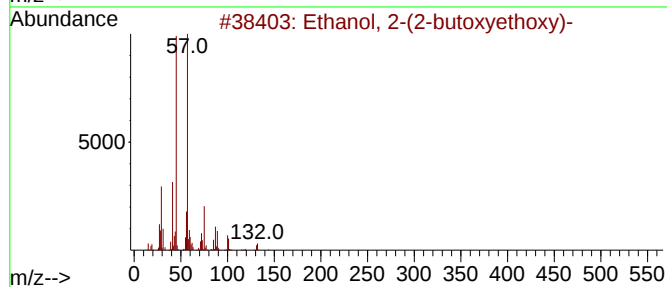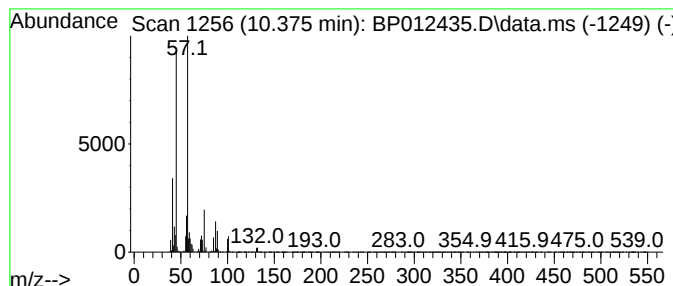

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP103122\
Data File : BP012435.D
Acq On : 01 Nov 2022 19:36
Operator : CG/JU
Sample : N5270-03
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHA67

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.375	8.9	ng/ul	1252170	2	10.587	2819240	20.0