
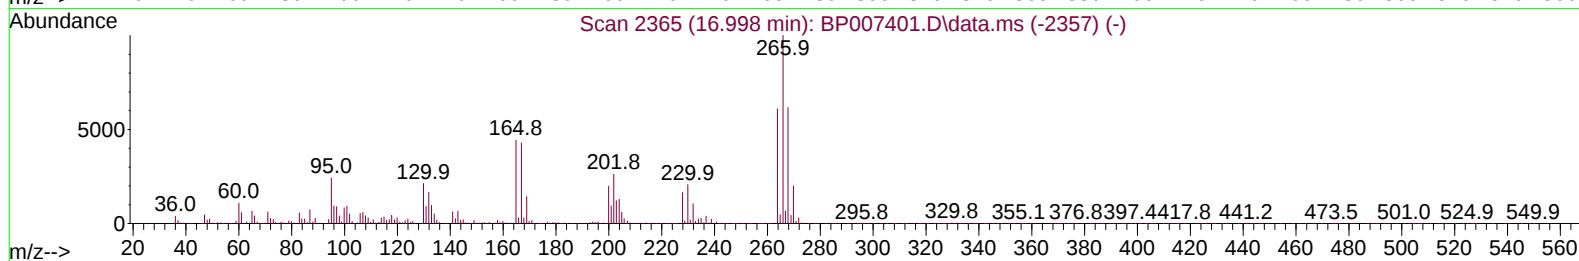
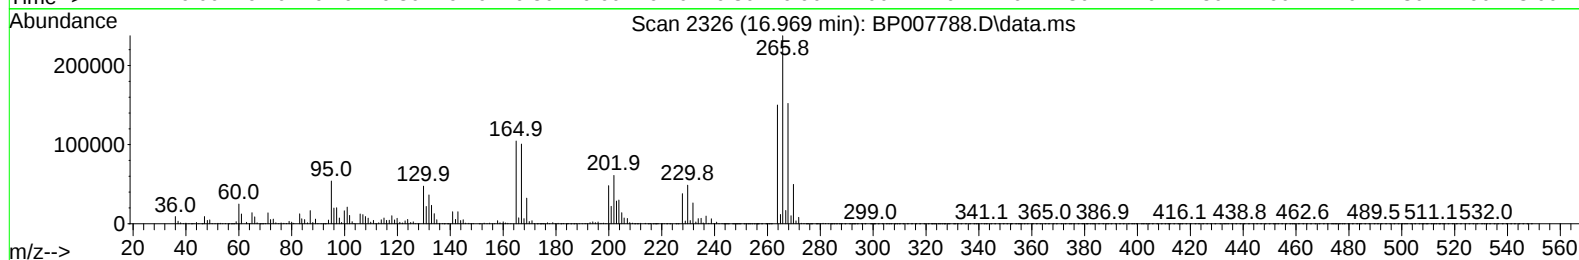


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110121\  
Data File : BP007788.D  
Acq On : 01 Nov 2021 12:40  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:34:08 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP101321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 13 14:54:20 2021  
Response via : Initial Calibration

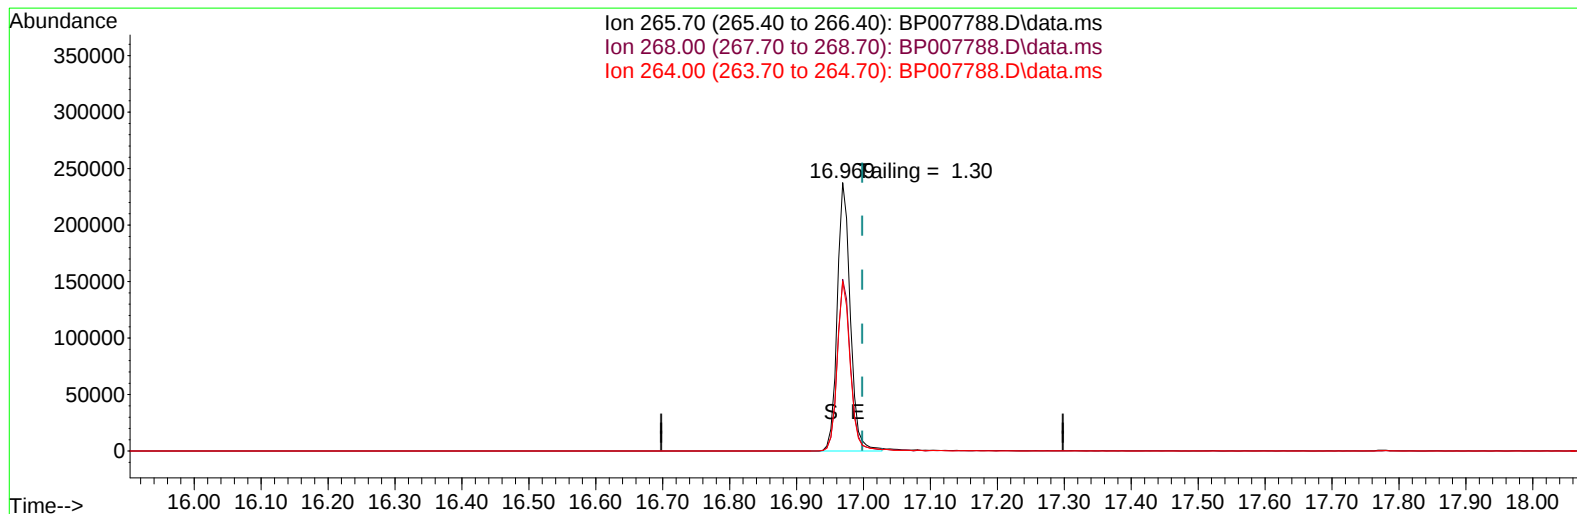

TIC: BP007788.D\data.ms

**(70) Pentachlorophenol (C)**




16.969min (-0.029) 2876622.33 ng

response 324598

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.60  | 63.98  |
| 264.00 | 60.90  | 63.15  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP110121\  
Data File : BP007788.D  
Acq On : 01 Nov 2021 12:40  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:34:08 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP101321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 13 14:54:20 2021  
Response via : Initial Calibration

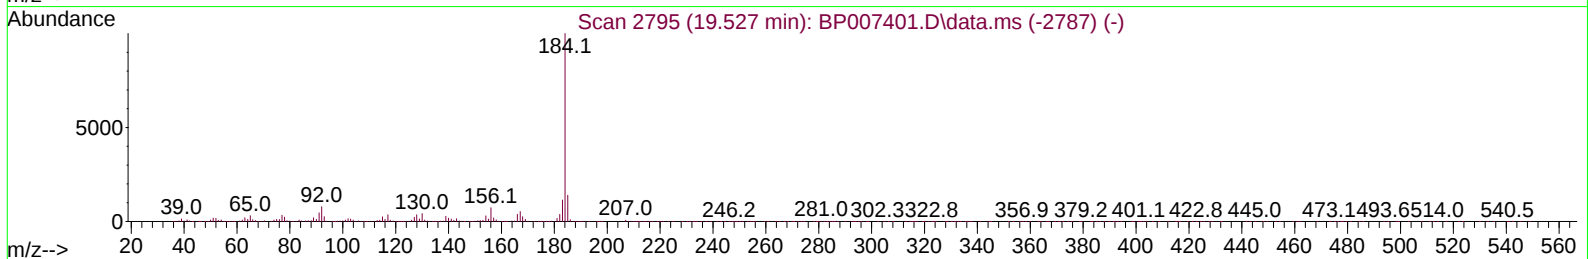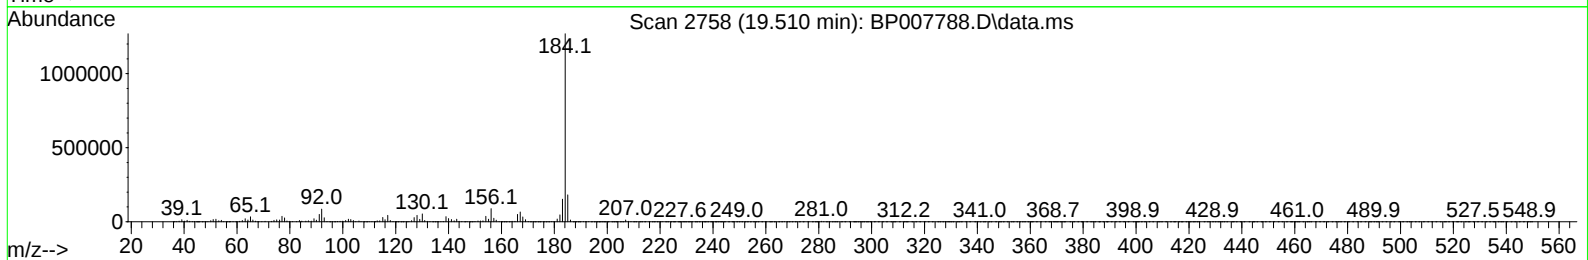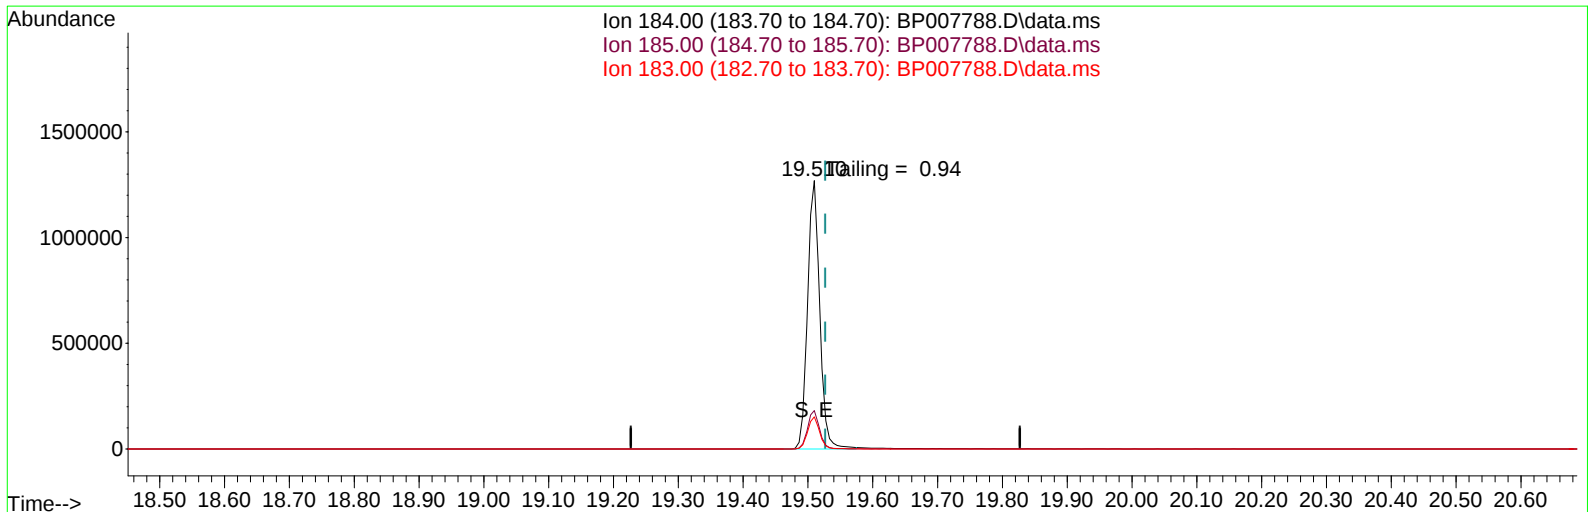

TIC: BP007788.D\data.ms

**(77) Benzidine****19.510min (-0.017) 594839.03 ng****response 1678411**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 14.34  |
| 183.00 | 11.40  | 11.98  |
| 0.00   | 0.00   | 0.00   |