


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110121\
 Data File : BP007788.D
 Acq On : 01 Nov 2021 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 01:43:06 2021

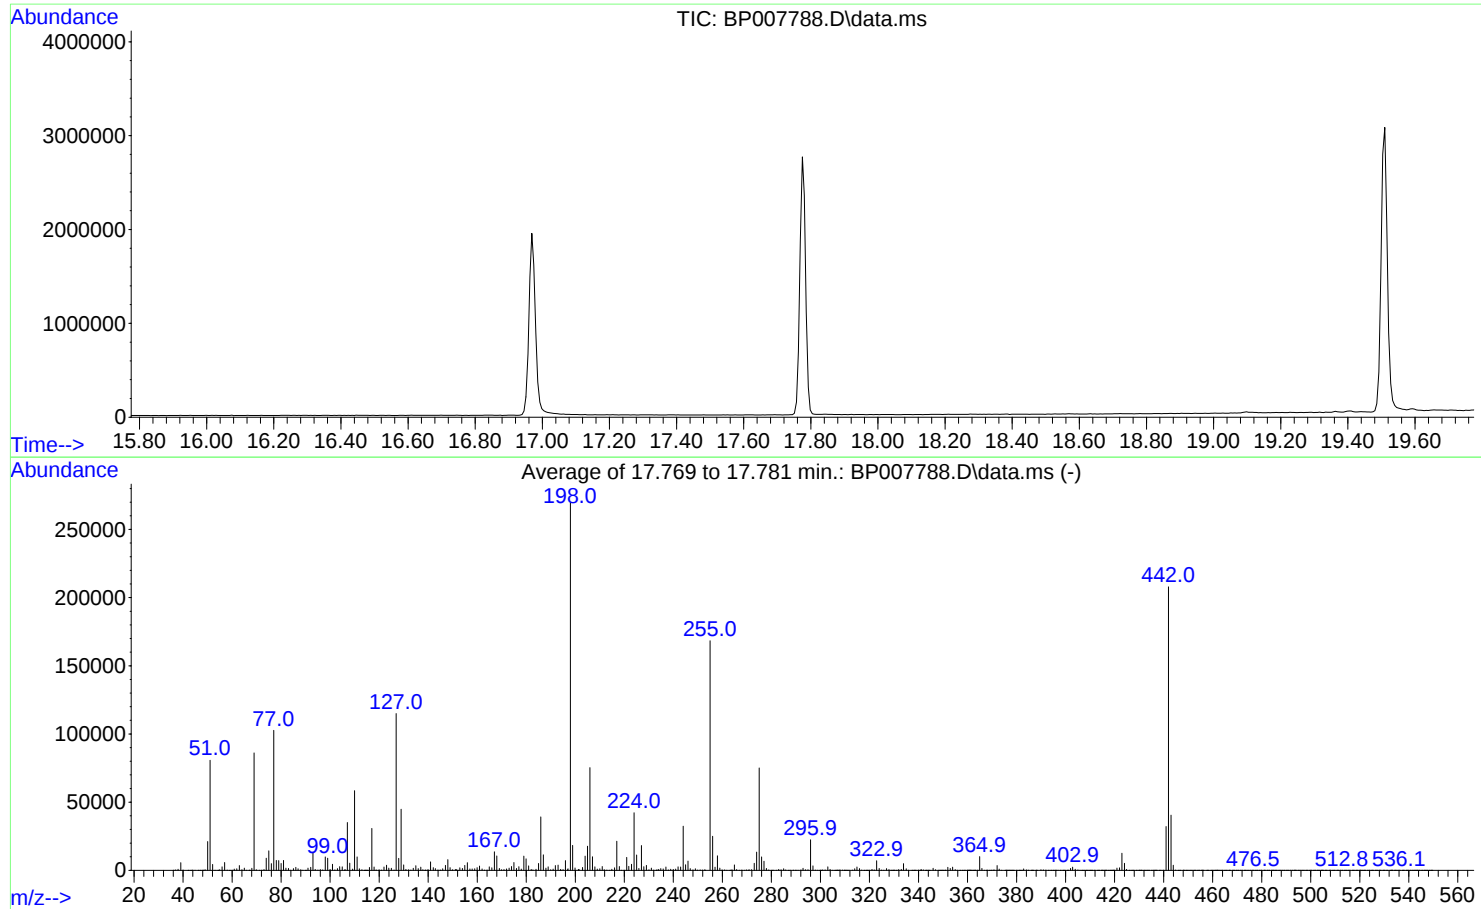


AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	80748	PASS
68	69	0.00	2	1.7	1506	PASS
69	198	0.00	100	31.9	86109	PASS
70	69	0.00	2	0.6	497	PASS
127	198	10	80	42.6	115045	PASS
197	198	0.00	2	0.4	1131	PASS
198	198	100	100	100.0	269750	PASS
199	198	5	9	6.8	18328	PASS
275	198	10	60	27.9	75155	PASS
365	198	1	100	3.8	10128	PASS
441	198	0.01	100	11.9	32147	PASS
442	442	100	100	100.0	207909	PASS
443	442	15	24	19.5	40496	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110121\
 Data File : BP007788.D
 Acq On : 01 Nov 2021 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 01 14:34:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 14:54:20 2021
 Response via : Initial Calibration

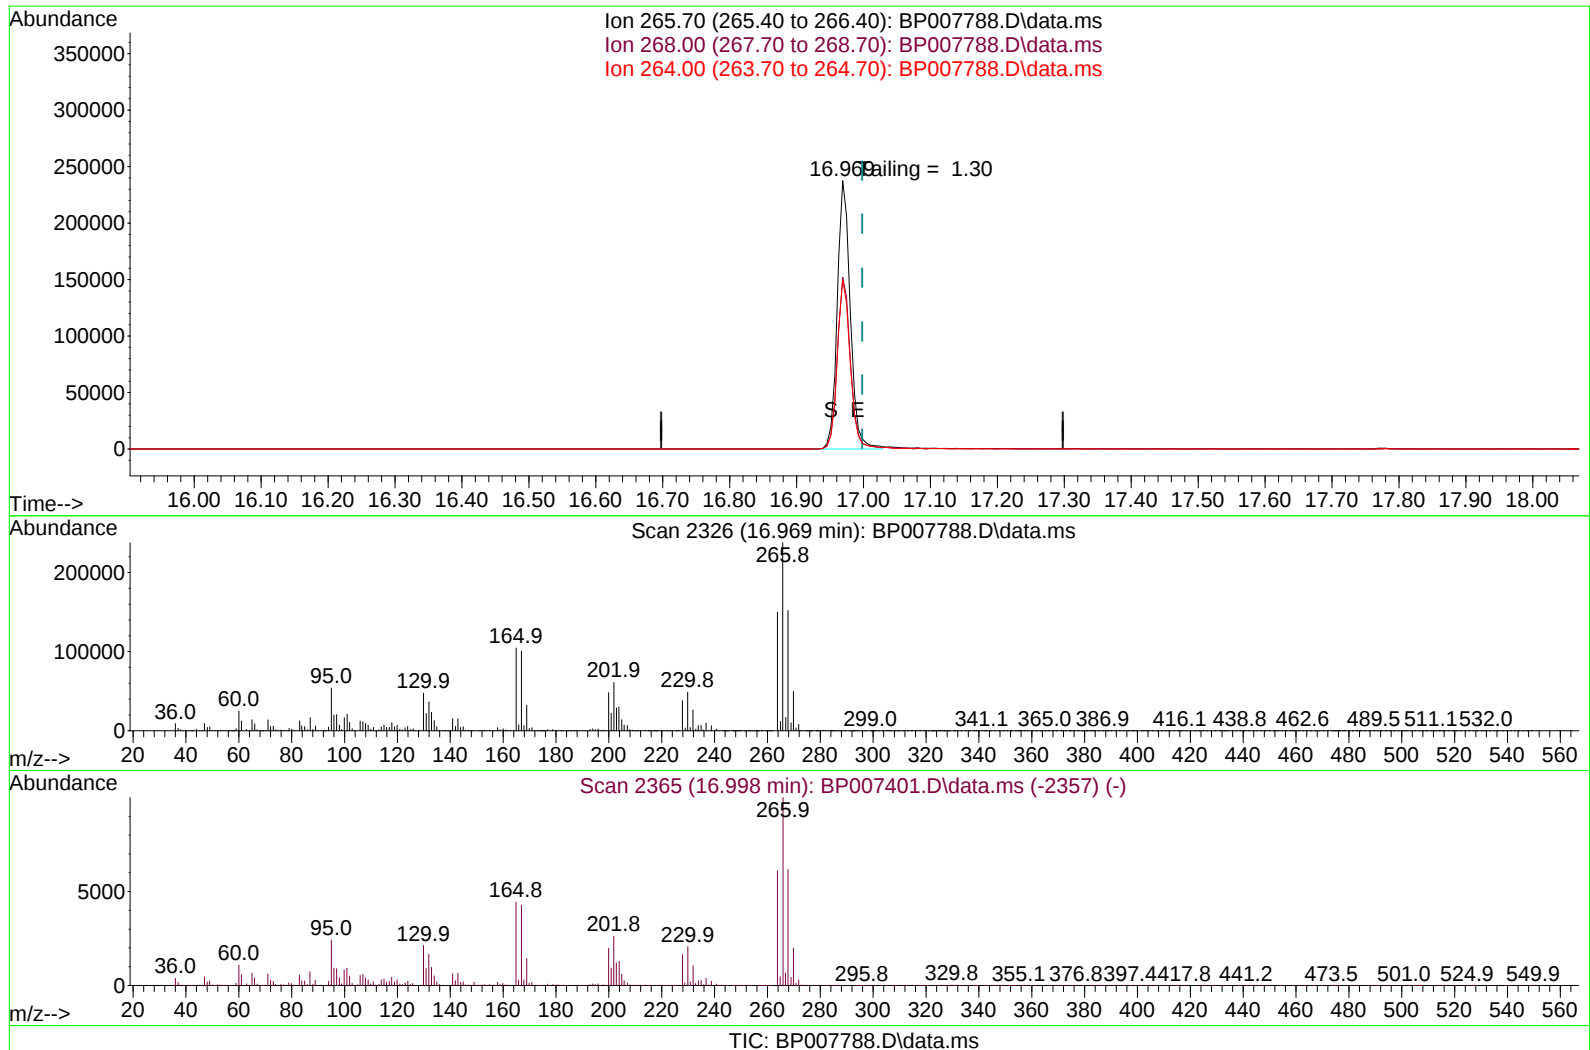

TIC: BP007788.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.029) 2876622.33 ng




response 324598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.98
264.00	60.90	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110121\
 Data File : BP007788.D
 Acq On : 01 Nov 2021 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 01 14:34:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 14:54:20 2021
 Response via : Initial Calibration

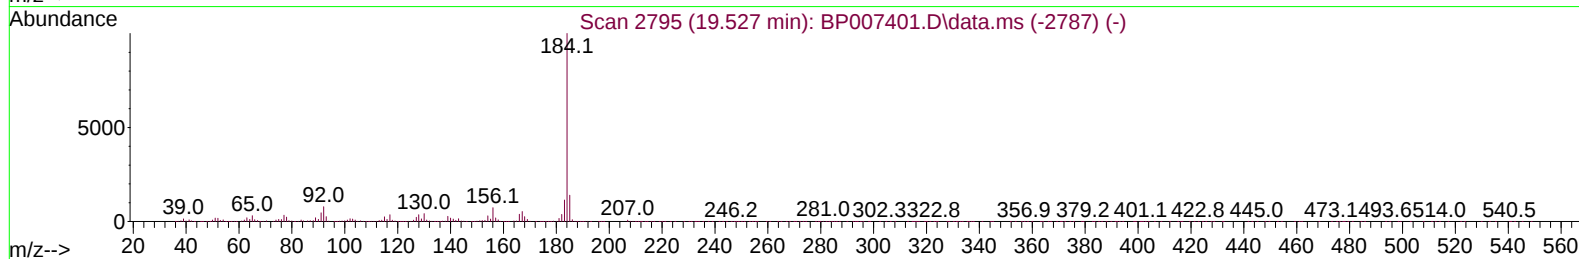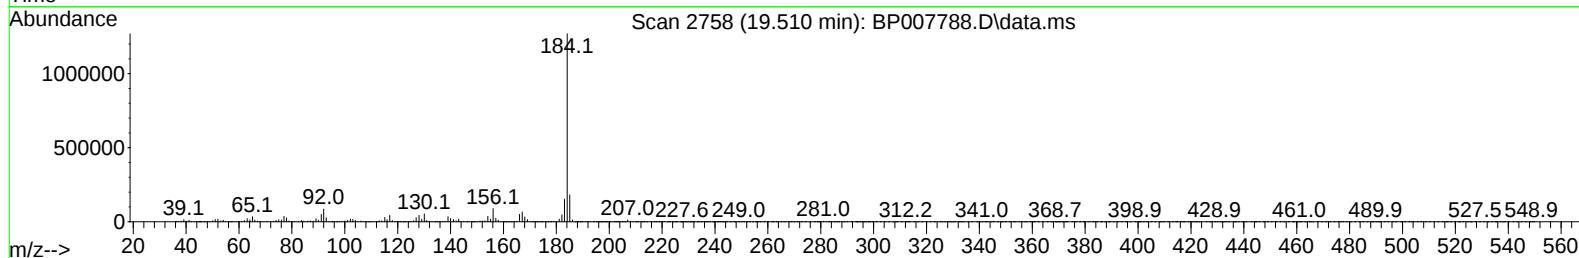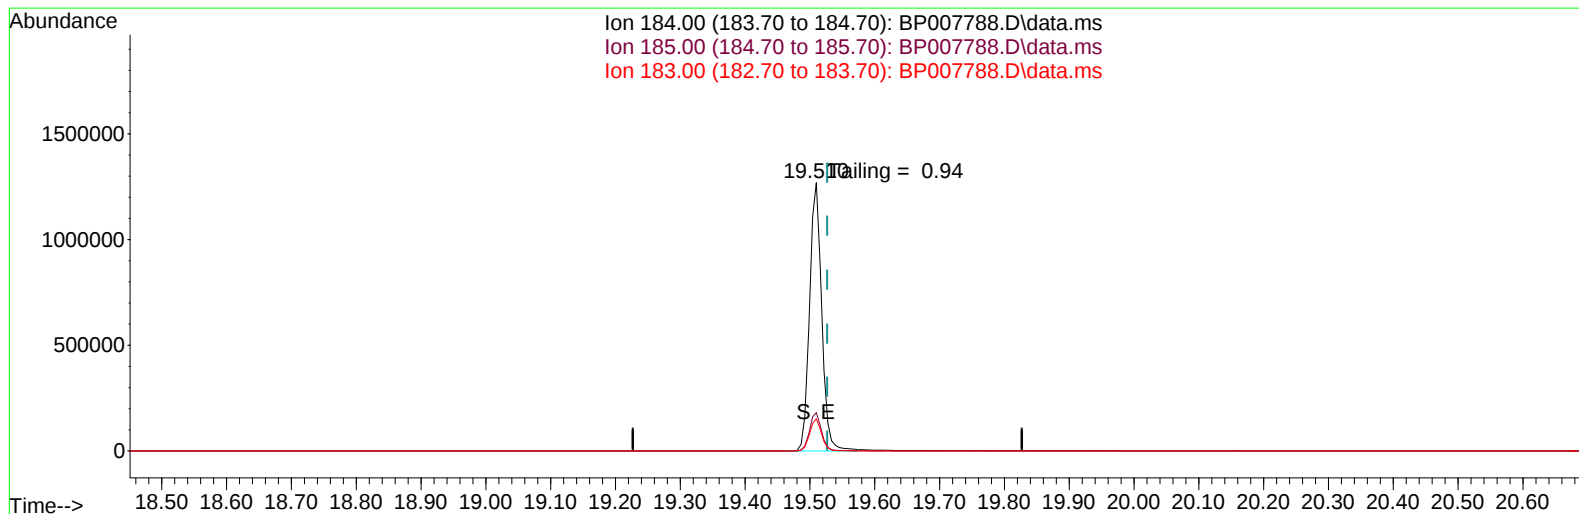

TIC: BP007788.D\data.ms

(77) Benzidine

19.510min (-0.017) 594839.03 ng

response 1678411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.34
183.00	11.40	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2021	BNA_P	<u>BP007788.D</u>
Compound Name	Response	Retention Time
DDT	915938	20.71
DDD	50861	20.28
DDE	7789	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
58650	974588	6.02

Instrument :
BNA_P
ClientSampleId :
DFTPP