
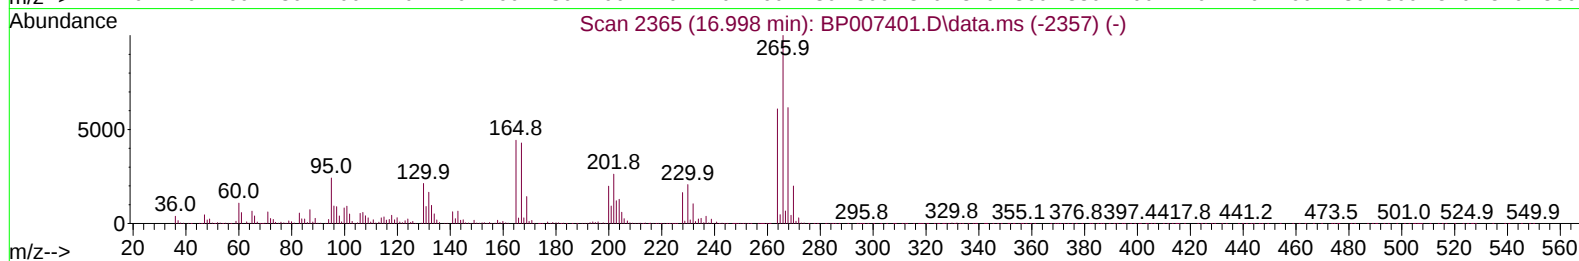
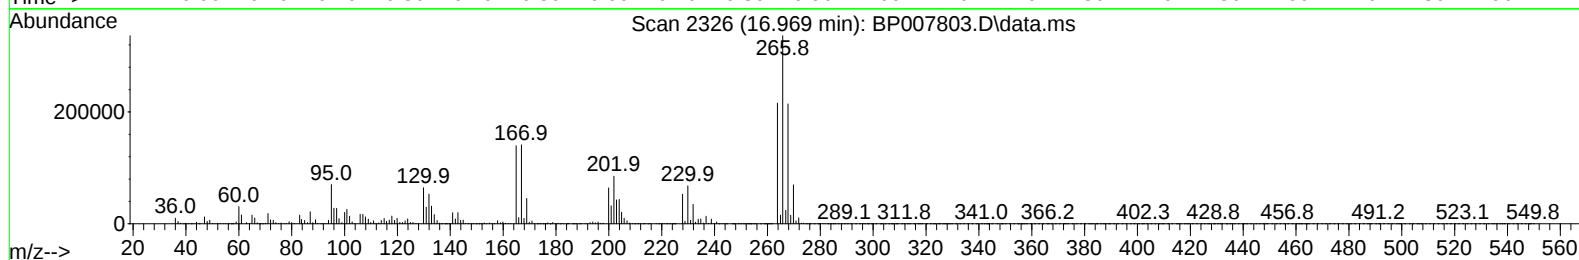


Quant Time: Nov 02 11:56:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 11:49:47 2021
Response via : Initial Calibration

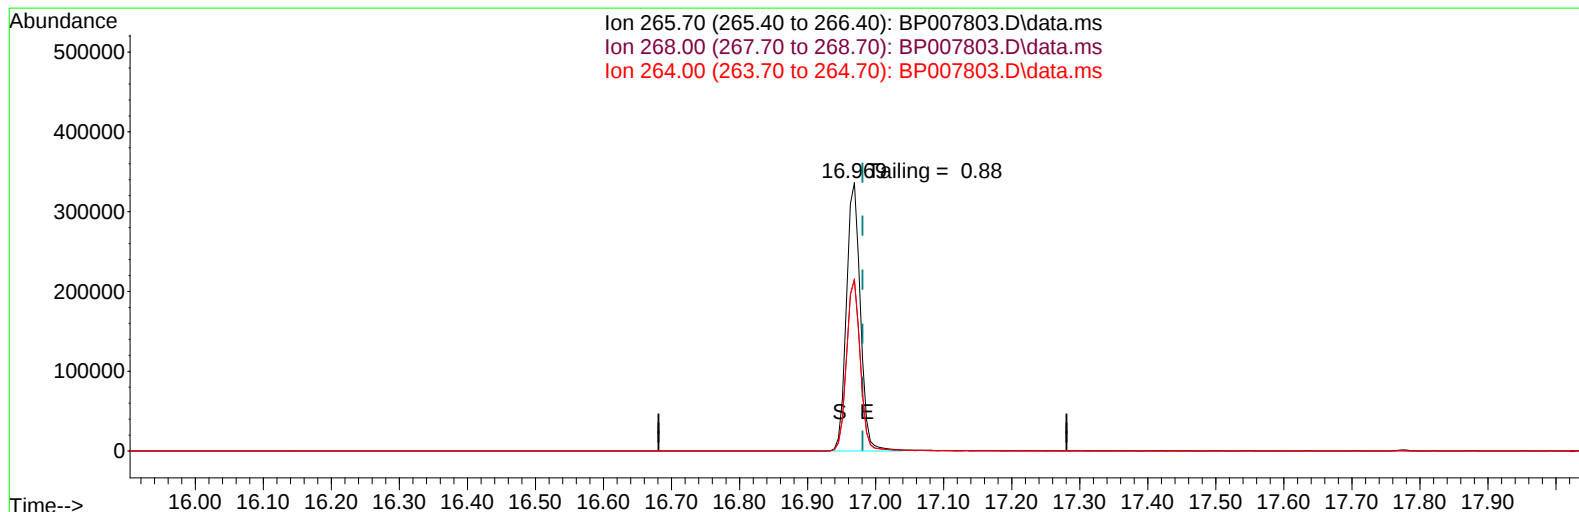

TIC: BP007803.D\data.ms

(70) Pentachlorophenol (C)




16.969min (-0.012) 3798353.28 ng

response **476229**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.77
264.00	60.90	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110221\
 Data File : BP007803.D
 Acq On : 02 Nov 2021 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 11:56:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 11:49:47 2021
 Response via : Initial Calibration

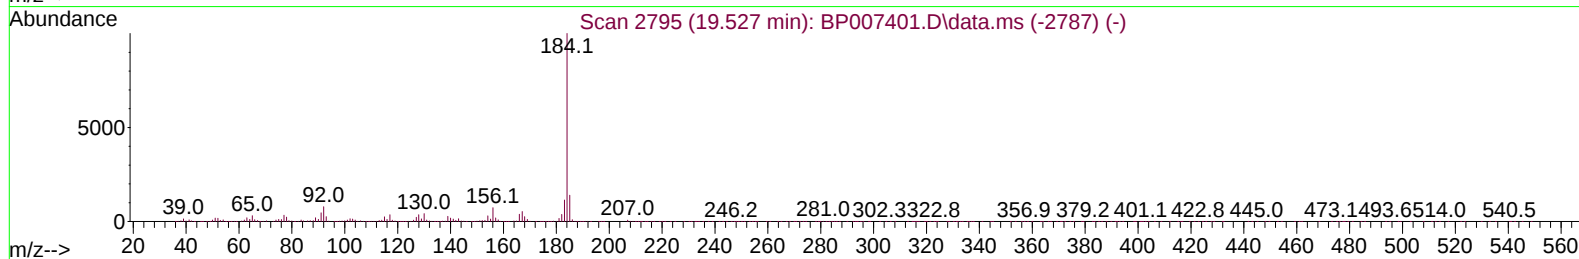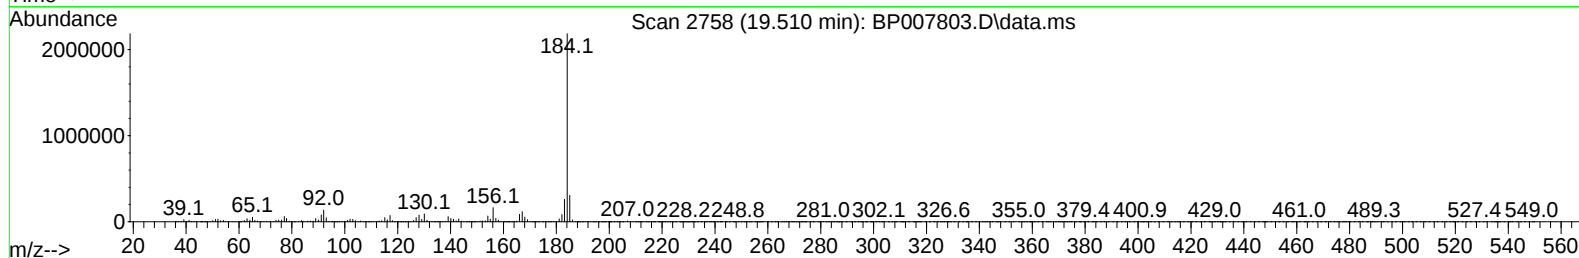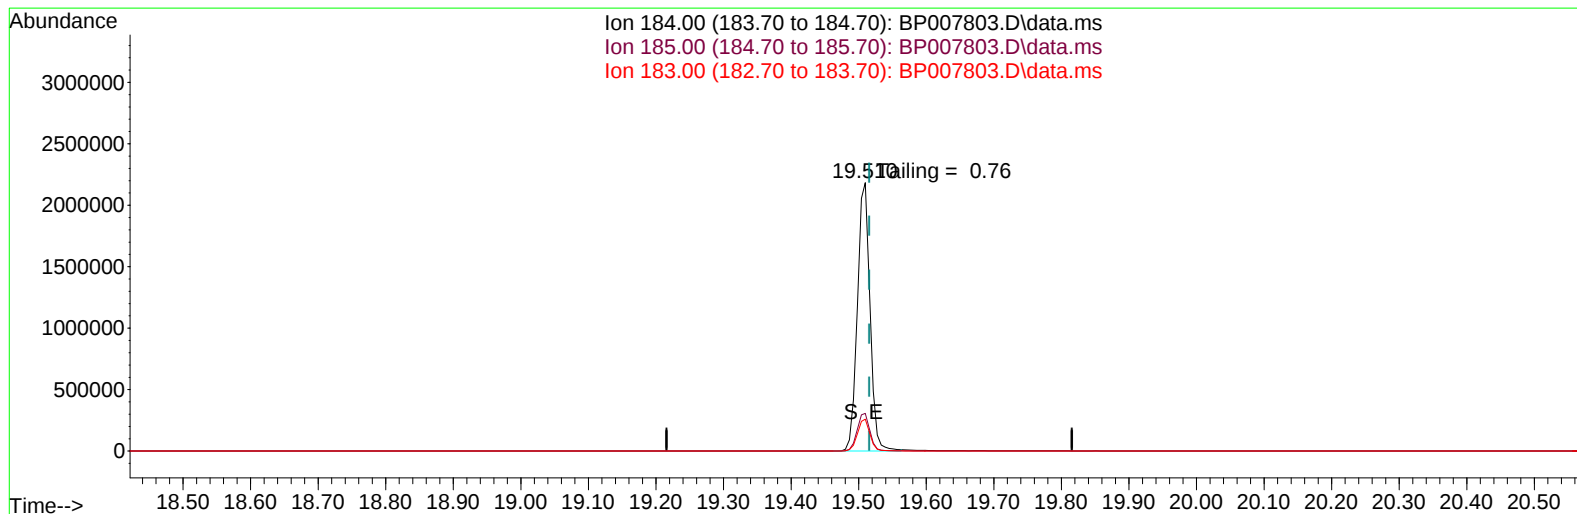

TIC: BP007803.D\data.ms

(77) Benzidine**19.510min (-0.006) 8179829.50 ng****response 2826170**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.06
183.00	11.40	11.89
0.00	0.00	0.00