
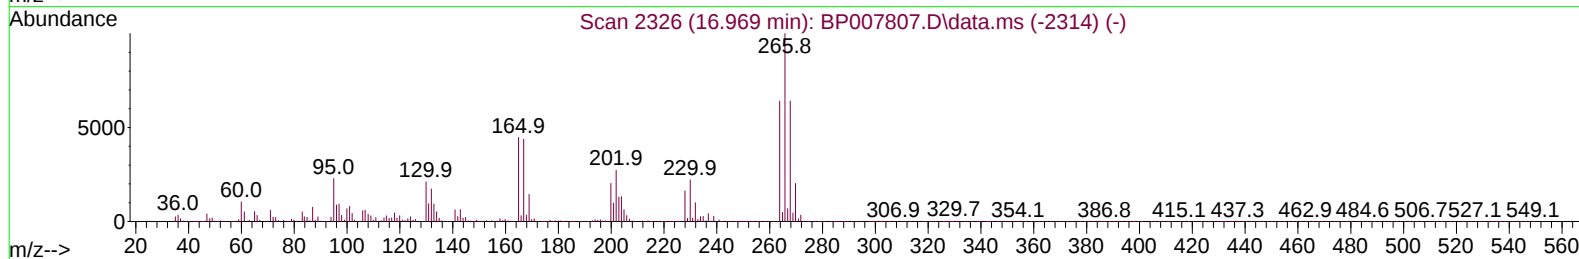
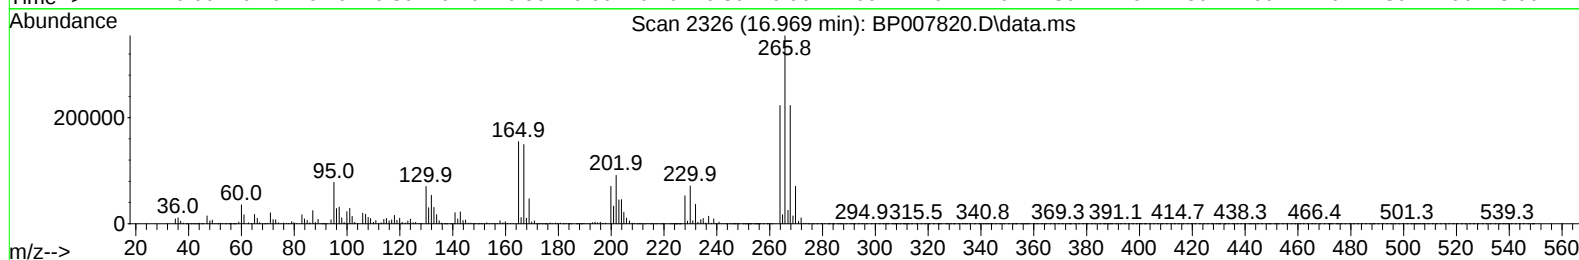


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007820.D
 Acq On : 03 Nov 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 14:21:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 19:18:55 2021
 Response via : Initial Calibration

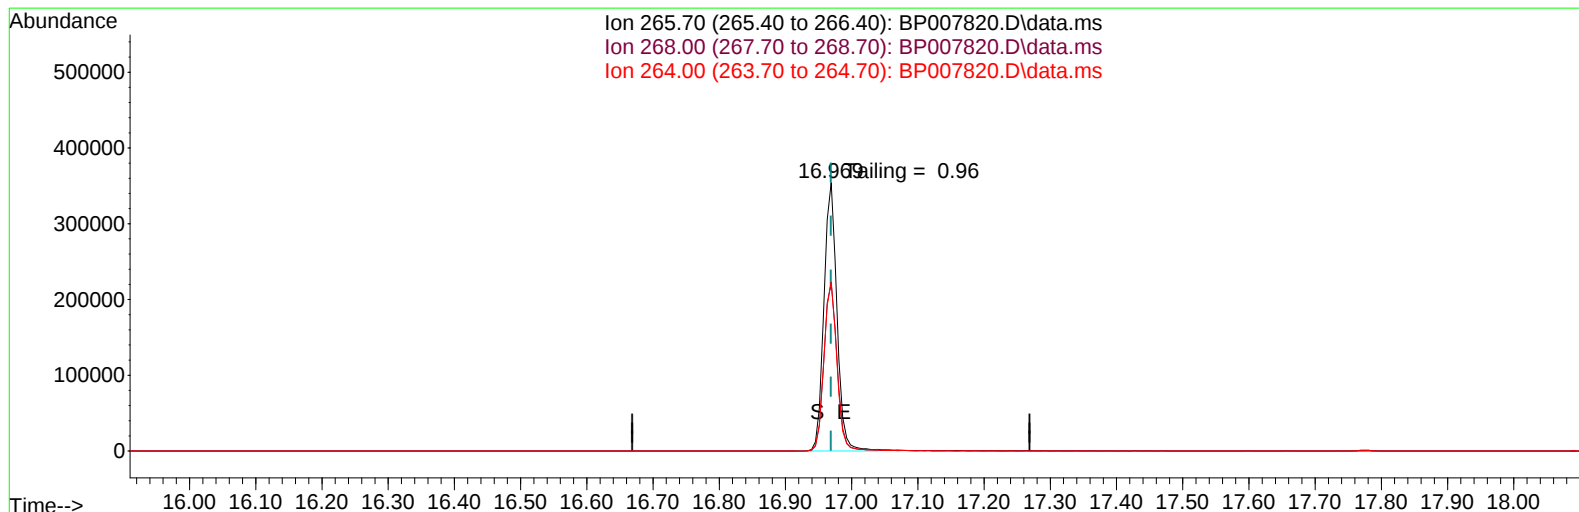

TIC: BP007820.D\data.ms

(70) Pentachlorophenol (C)




16.969min (+ 0.000) 2915970.10 ng

response 486526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	62.86
264.00	60.90	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007820.D
 Acq On : 03 Nov 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 14:21:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 19:18:55 2021
 Response via : Initial Calibration

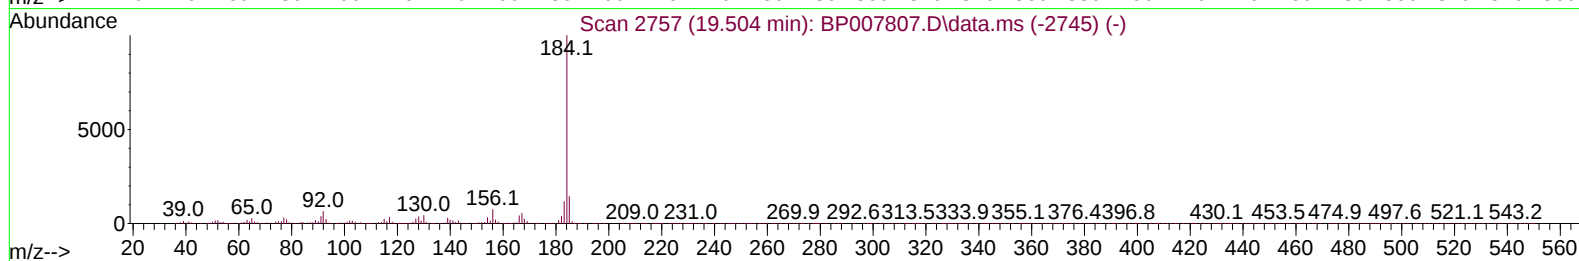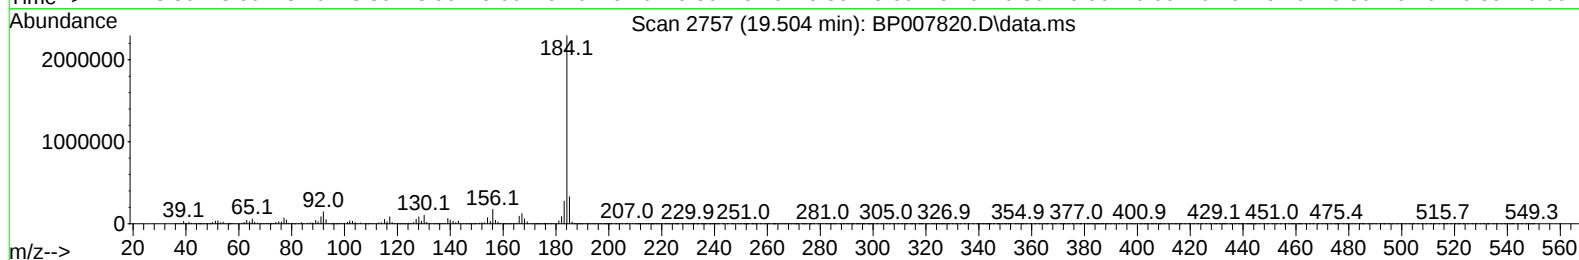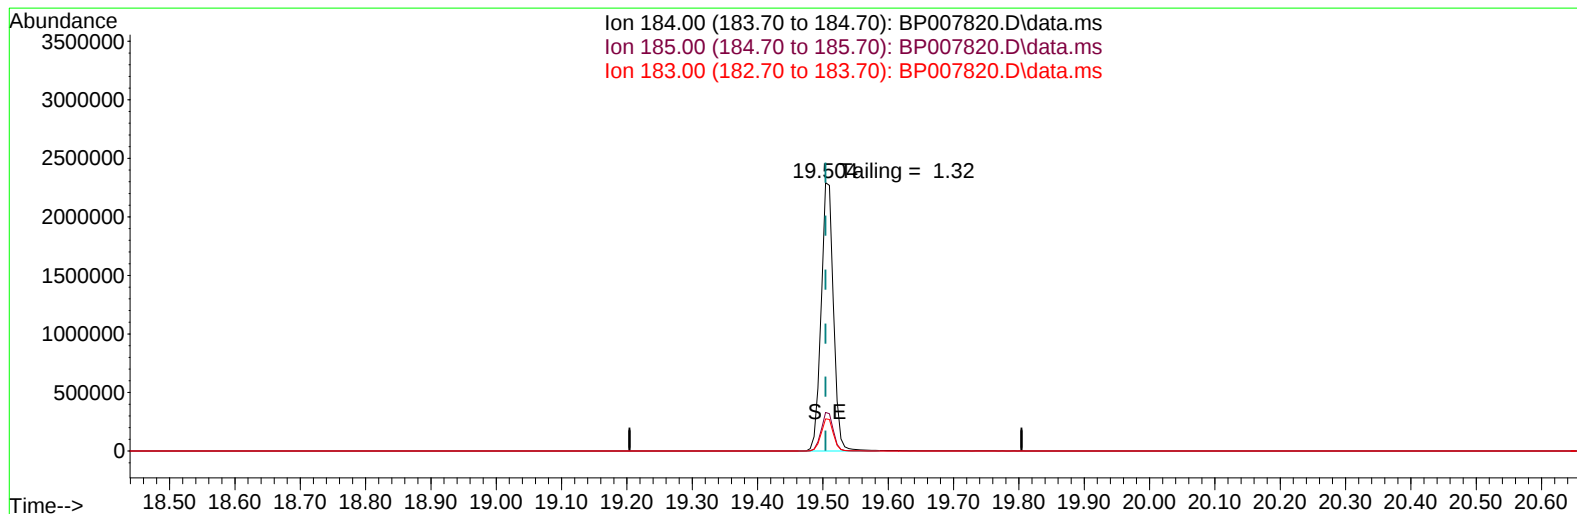

TIC: BP007820.D\data.ms

(77) Benzidine**19.504min (+ 0.000) 208811.15 ng****response 3026023**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	11.40	11.98
0.00	0.00	0.00