

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007822.D
 Acq On : 03 Nov 2021 14:44
 Operator : CG/JU
 Sample : PB140419BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140419BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.499	369	376	386	rBV	3056502	4496378	30.49%	8.145%
2	7.093	639	647	656	rBV	2984198	4720889	32.01%	8.552%
3	7.922	781	788	797	rVB	527817	835369	5.66%	1.513%
4	9.081	974	985	1000	rBV	1709557	2869597	19.46%	5.198%
5	10.722	1256	1264	1279	rBV	717313	1227867	8.33%	2.224%
6	13.187	1673	1683	1700	rBV	5026127	7416305	50.29%	13.435%
7	14.557	1909	1916	1931	rBV	1253962	1884021	12.77%	3.413%
8	16.051	2162	2170	2192	rBV	4654027	6720246	45.57%	12.174%
9	17.316	2378	2385	2398	rBV	1771051	2582411	17.51%	4.678%
10	19.881	2815	2821	2826	rBV	12117301	14747984	100.00%	26.717%
11	21.404	3075	3080	3092	rVB	2748987	3686040	24.99%	6.677%
12	23.839	3487	3494	3506	rVB2	1901061	4014265	27.22%	7.272%




Sum of corrected areas: 55201372

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
Data File : BP007822.D
Acq On : 03 Nov 2021 14:44
Operator : CG/JU
Sample : PB140419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140419BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

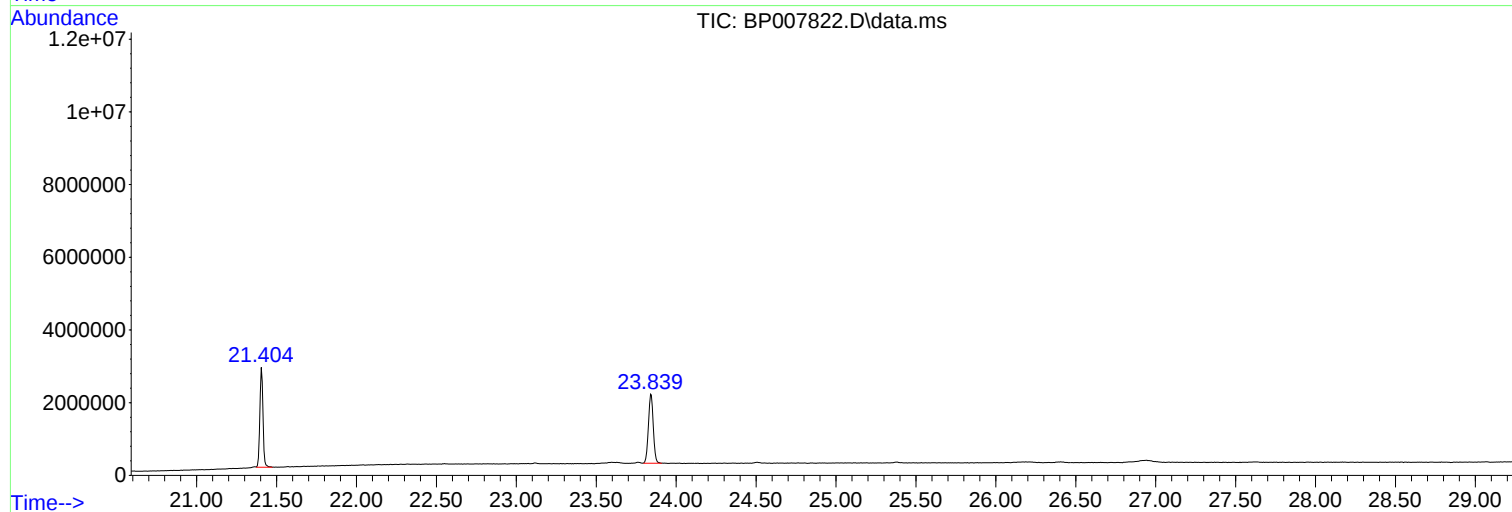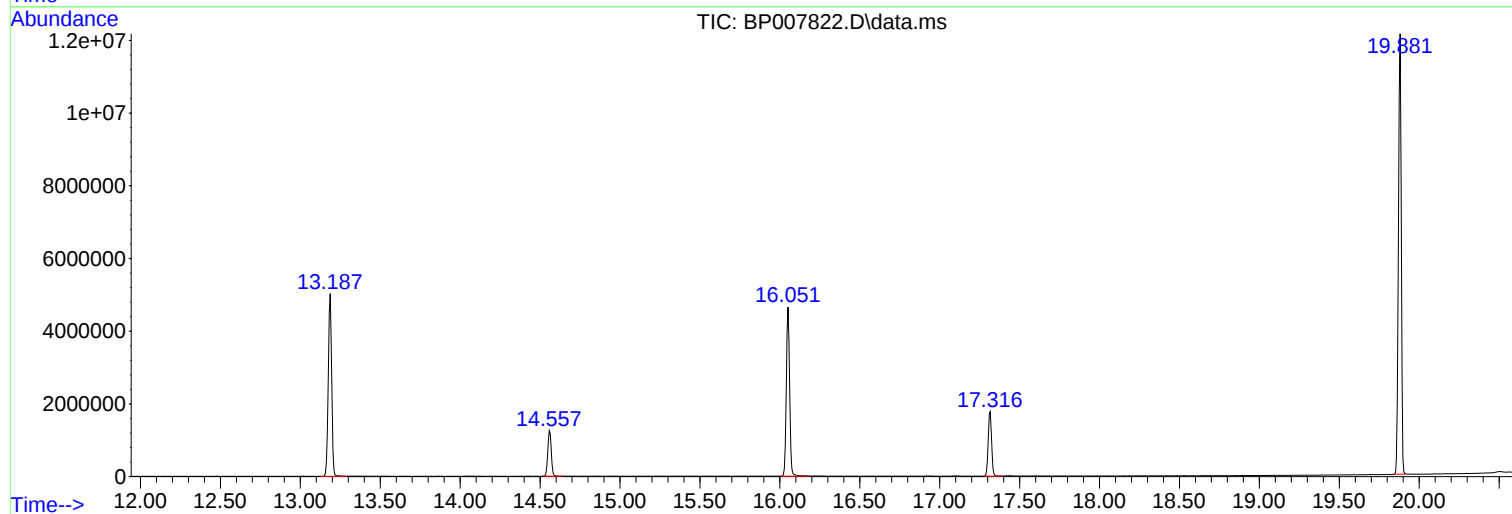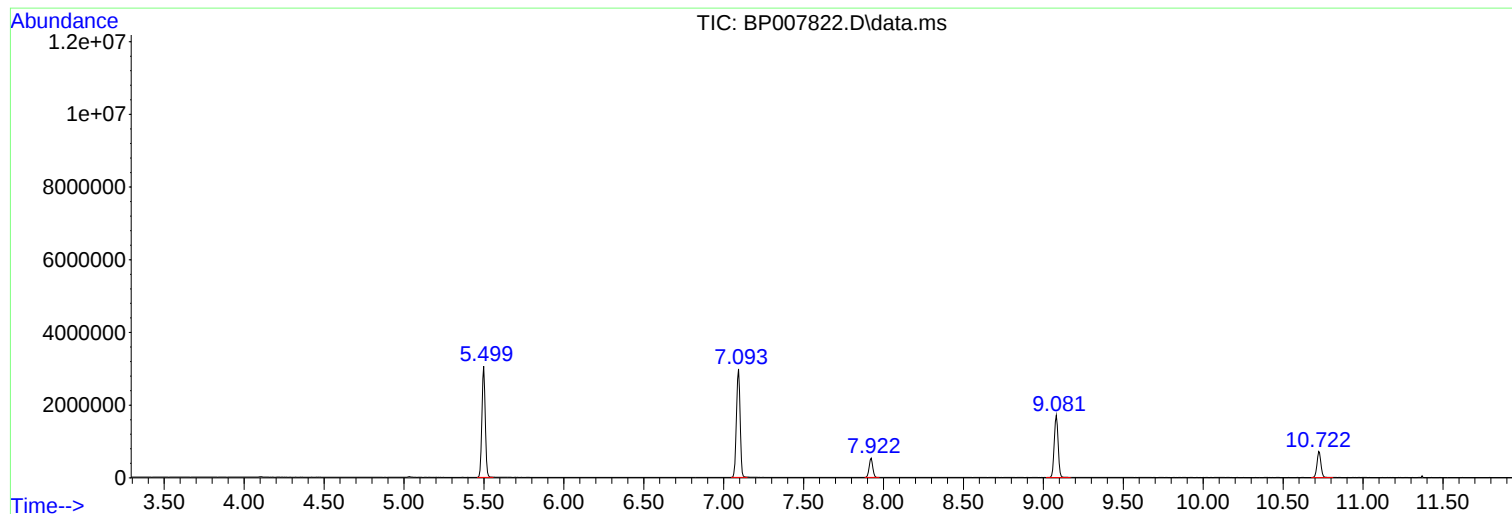

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
Data File : BP007822.D
Acq On : 03 Nov 2021 14:44
Operator : CG/JU
Sample : PB140419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140419BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
Data File : BP007822.D
Acq On : 03 Nov 2021 14:44
Operator : CG/JU
Sample : PB140419BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140419BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------