
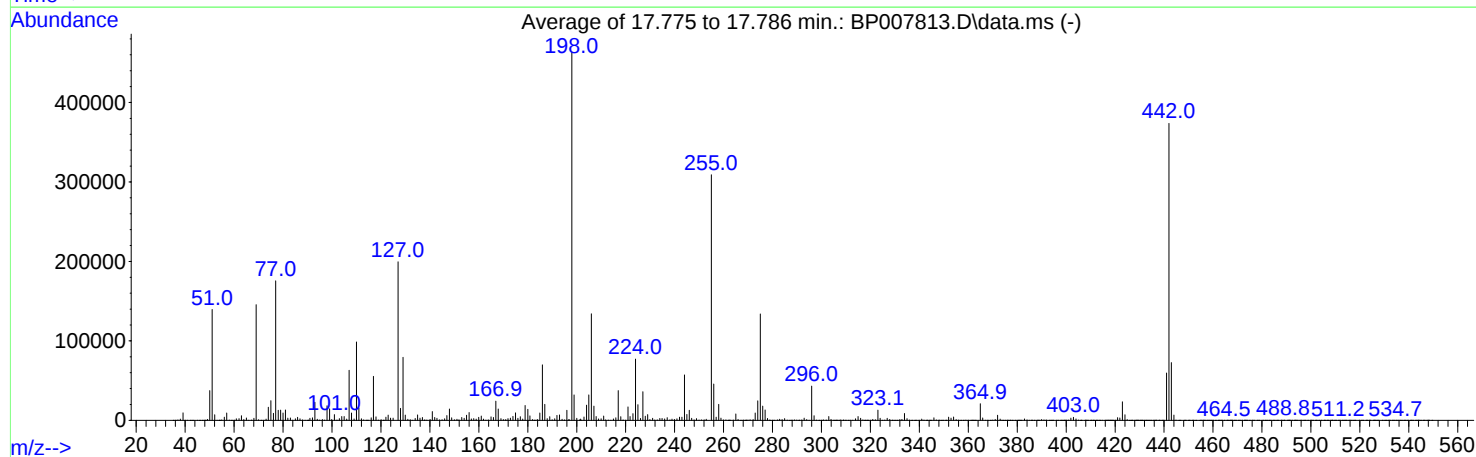


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007813.D
 Acq On : 03 Nov 2021 08:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 19:18:55 2021

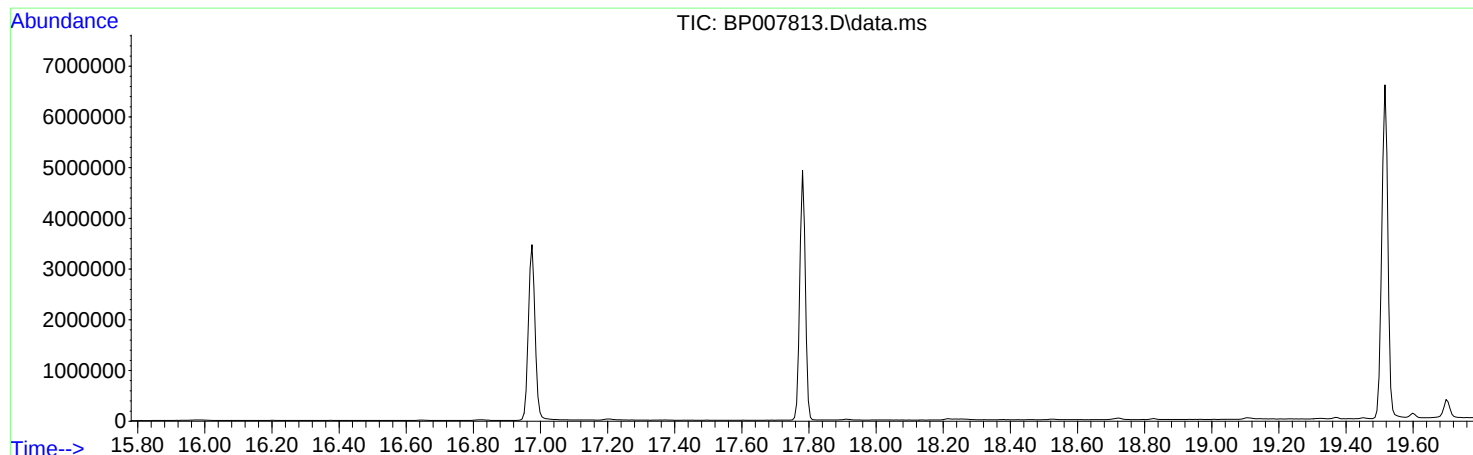

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	139485	PASS
68	69	0.00	2	1.7	2533	PASS
69	198	0.00	100	31.5	145600	PASS
70	69	0.00	2	0.6	806	PASS
127	198	10	80	43.1	199637	PASS
197	198	0.00	2	0.2	770	PASS
198	198	100	100	100.0	462917	PASS
199	198	5	9	6.9	32008	PASS
275	198	10	60	28.9	133957	PASS
365	198	1	100	4.5	21036	PASS
441	198	0.01	100	12.9	59709	PASS
442	442	100	100	100.0	373781	PASS
443	442	15	24	19.5	72754	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/3/2021	BNA_P	<u>BP007813.D</u>
Compound Name	Response	Retention Time
DDT	1775406	20.72
DDD	10637	20.29
DDE	1068	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11705	1787111	0.65

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007813.D
 Acq On : 03 Nov 2021 08:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 11:25:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 19:18:55 2021
 Response via : Initial Calibration

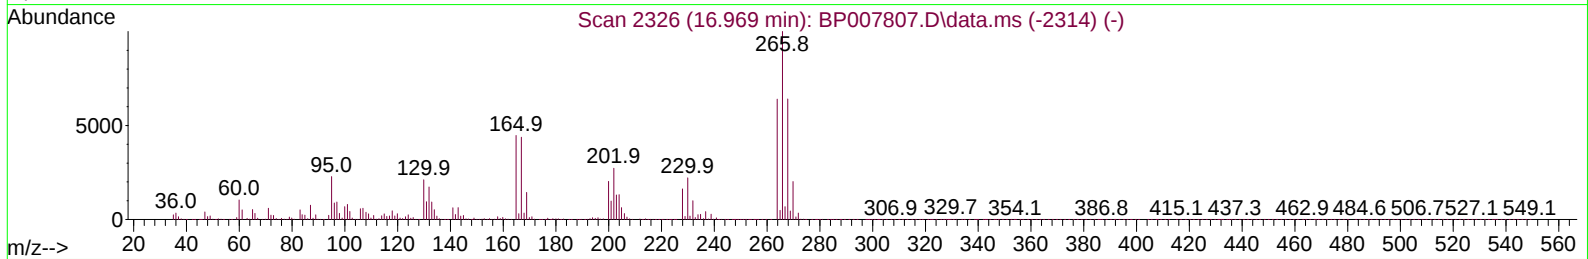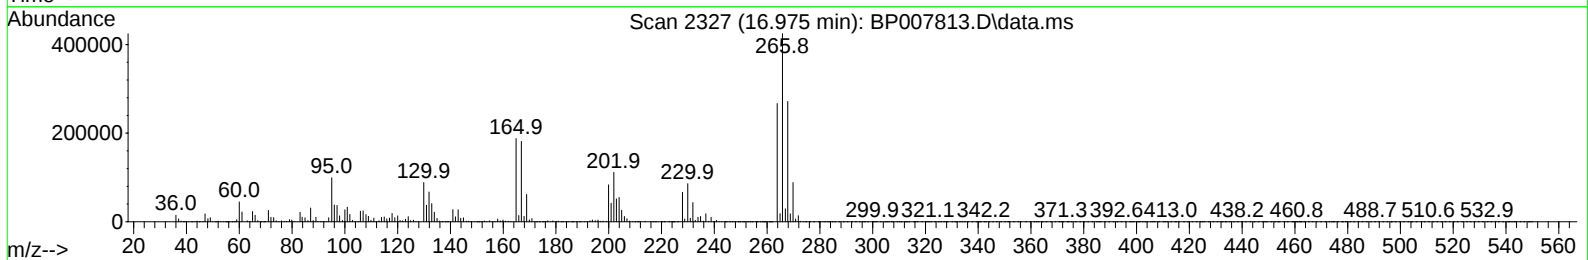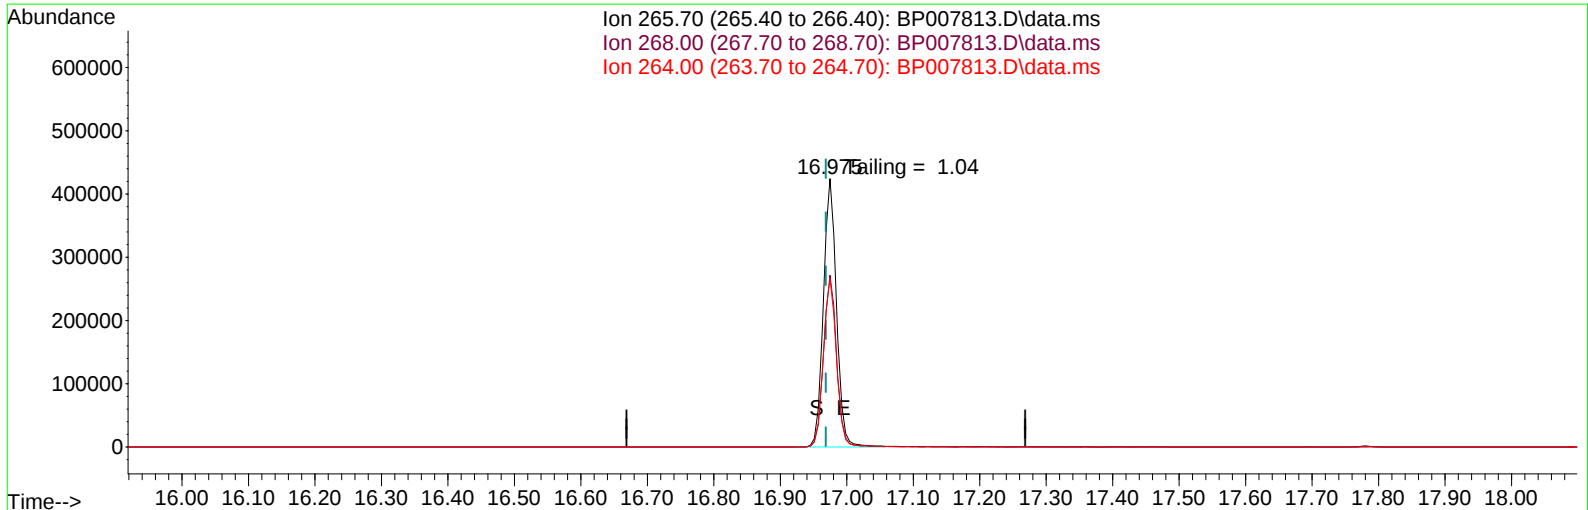

TIC: BP007813.D\data.ms

(70) Pentachlorophenol (C)

16.975min (+ 0.006) 146531.26 ng




response 584437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.99
264.00	60.90	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
Data File : BP007813.D
Acq On : 03 Nov 2021 08:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 03 11:25:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 19:18:55 2021
Response via : Initial Calibration

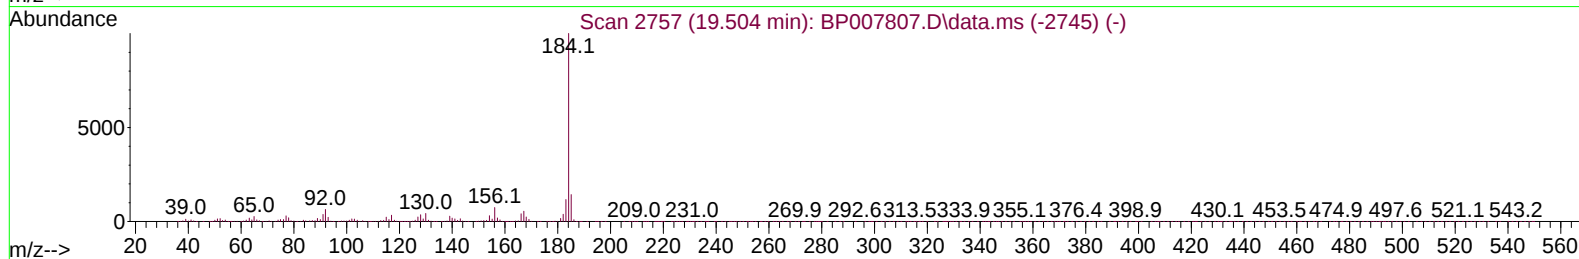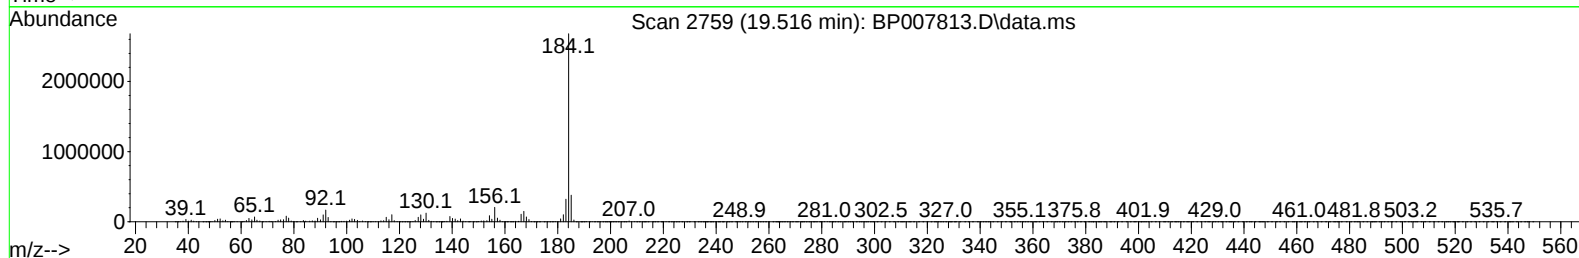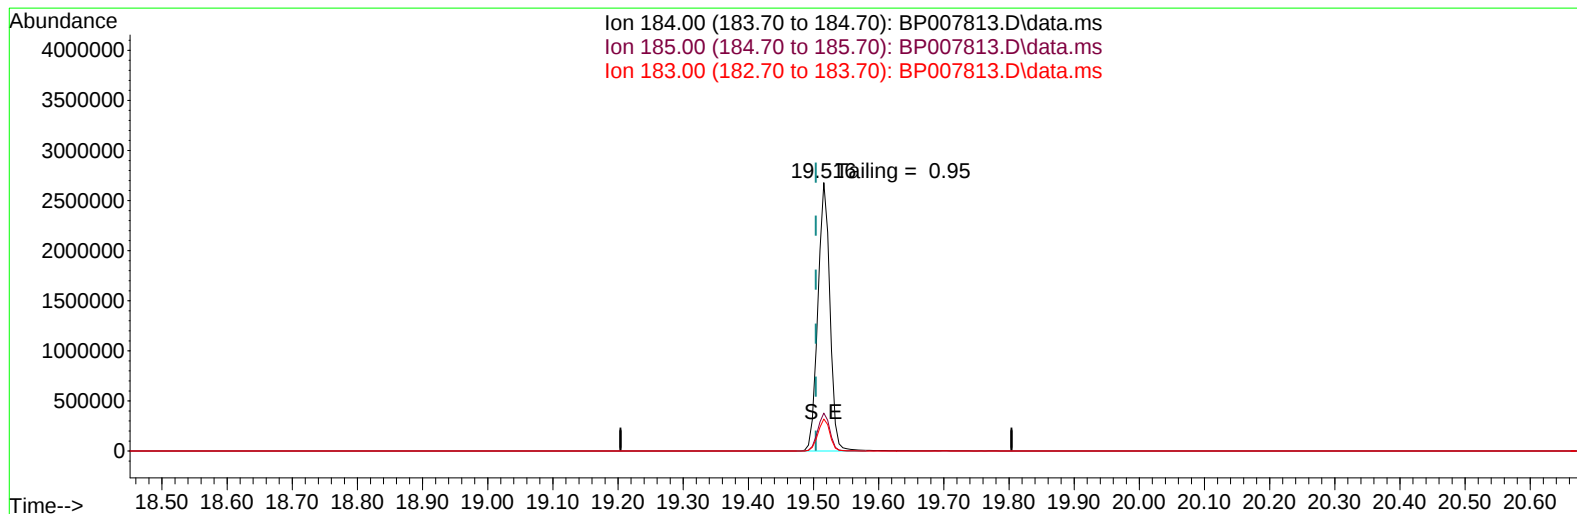

TIC: BP007813.D\data.ms

(77) Benzidine

19.516min (+ 0.012) 42141.34 ng

response 3454961

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.15
183.00	11.40	11.97
0.00	0.00	0.00