


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007820.D
 Acq On : 03 Nov 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 19:18:55 2021

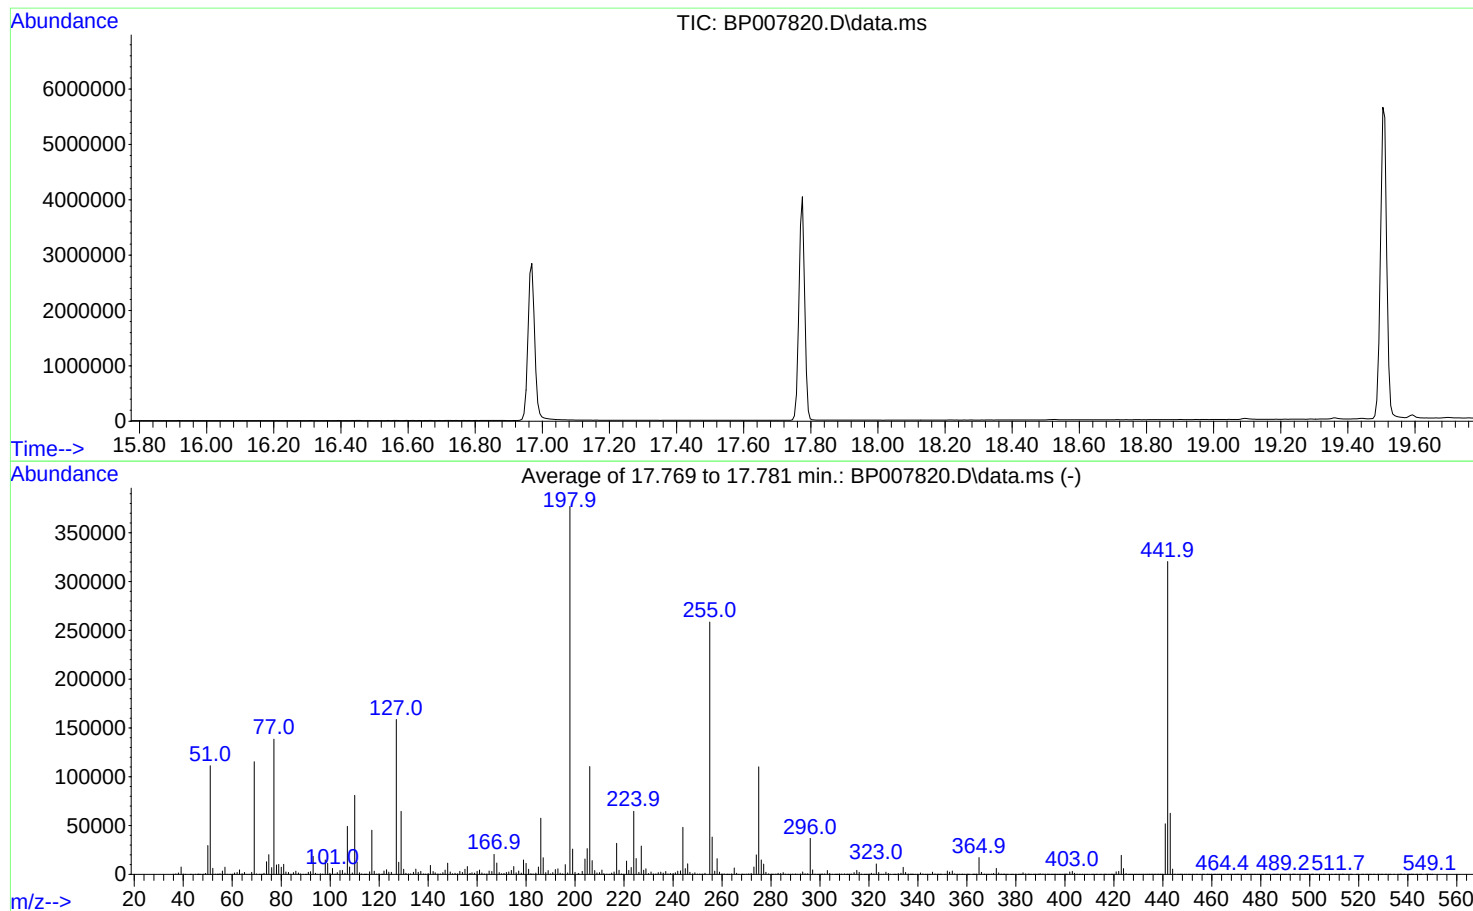




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	111273	PASS
68	69	0.00	2	1.8	2098	PASS
69	198	0.00	100	30.6	115410	PASS
70	69	0.00	2	0.5	564	PASS
127	198	10	80	42.1	158739	PASS
197	198	0.00	2	0.4	1441	PASS
198	198	100	100	100.0	376970	PASS
199	198	5	9	6.9	25848	PASS
275	198	10	60	29.2	110146	PASS
365	198	1	100	4.6	17158	PASS
441	198	0.01	100	13.7	51824	PASS
442	442	100	100	100.0	320482	PASS
443	442	15	24	19.5	62565	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
 Data File : BP007820.D
 Acq On : 03 Nov 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 14:21:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 19:18:55 2021
 Response via : Initial Calibration

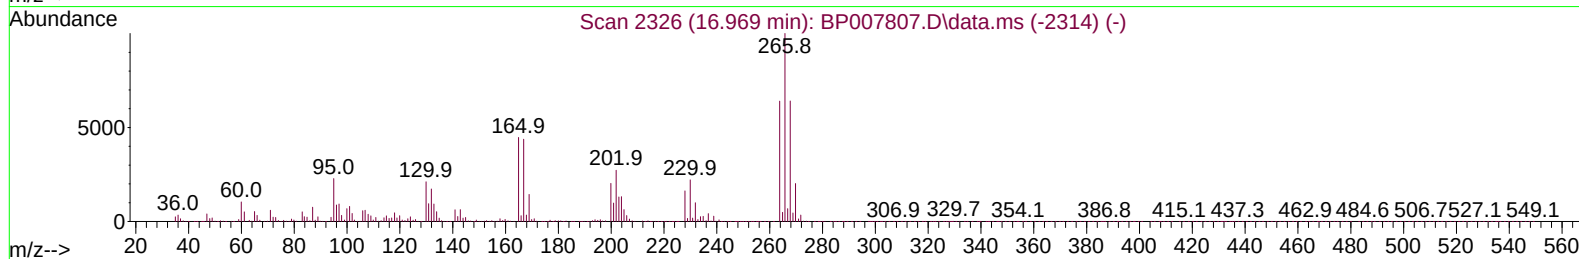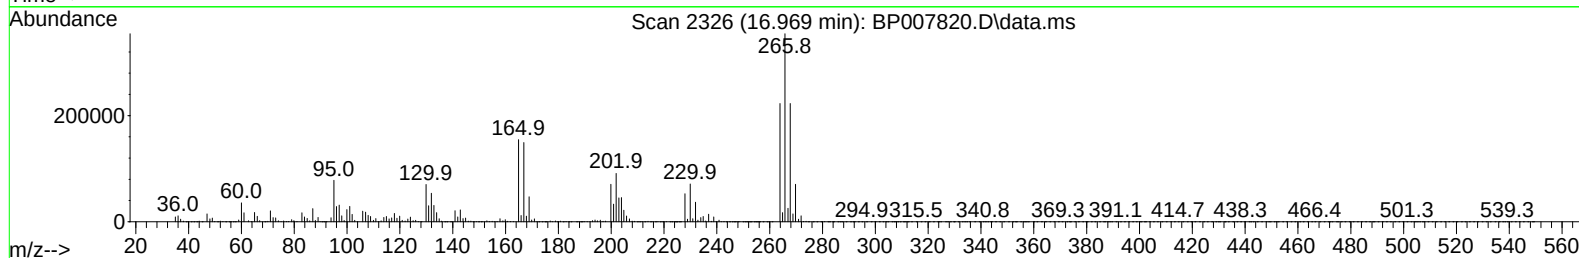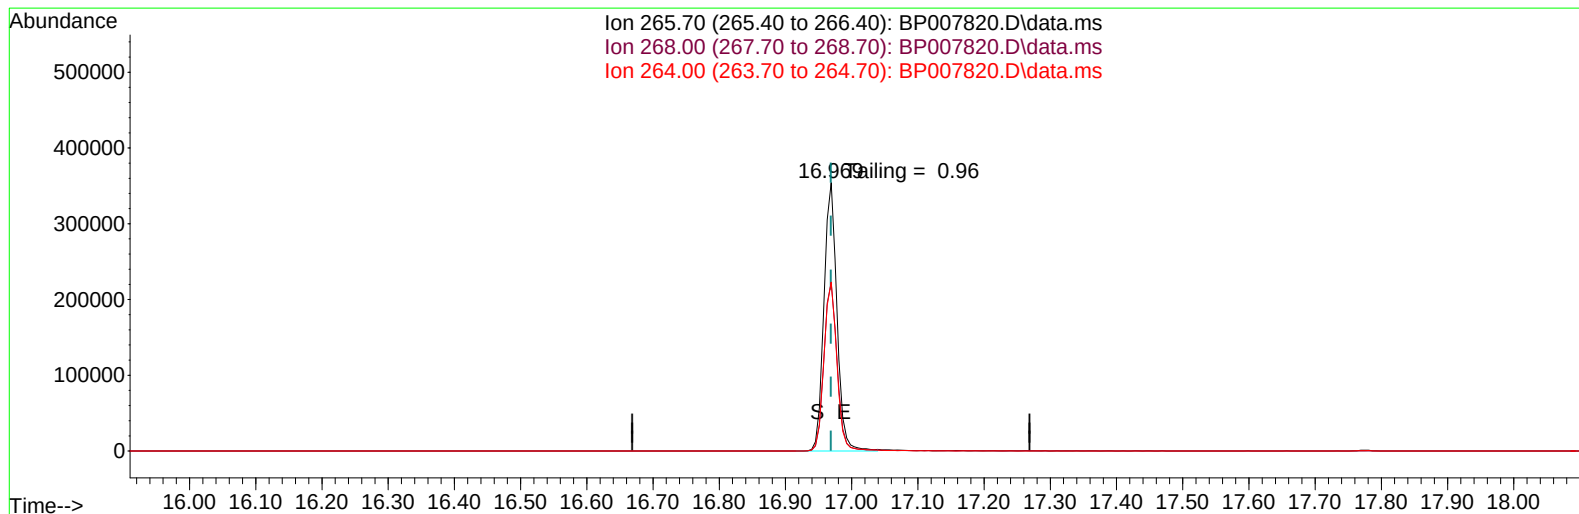

TIC: BP007820.D\data.ms

(70) Pentachlorophenol (C)

16.969min (+ 0.000) 2915970.10 ng




response 486526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	62.86
264.00	60.90	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110321\
Data File : BP007820.D
Acq On : 03 Nov 2021 13:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 03 14:21:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 19:18:55 2021
Response via : Initial Calibration

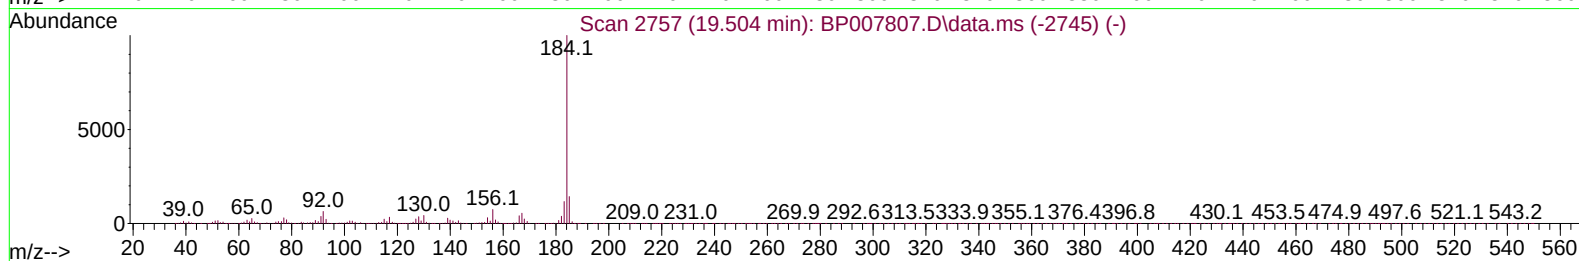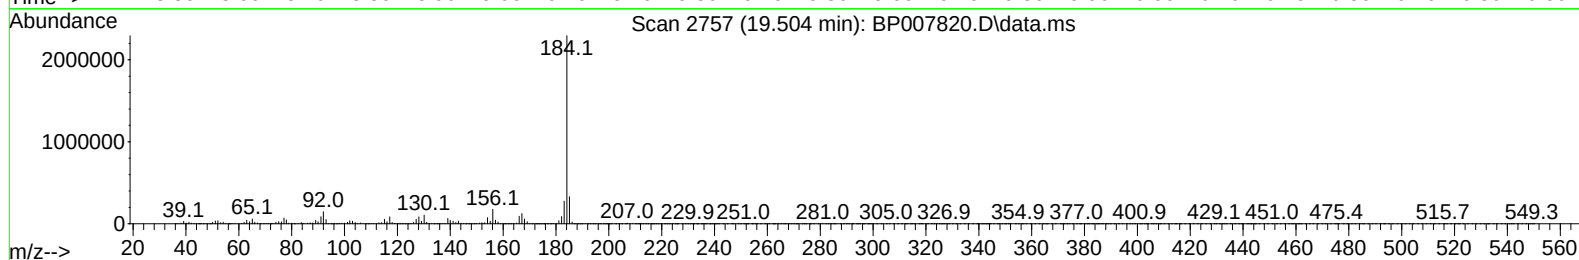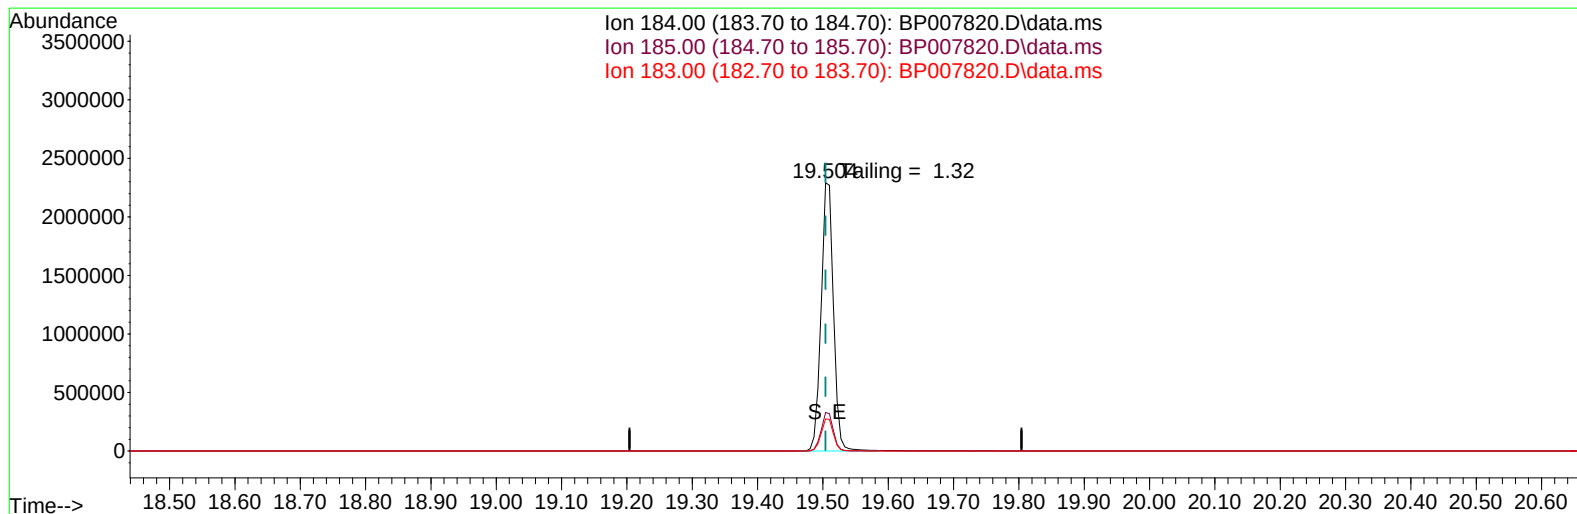

TIC: BP007820.D\data.ms

(77) Benzidine

19.504min (+ 0.000) 208811.15 ng

response 3026023

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	11.40	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2021	BNA_P	<u>BP007820.D</u>
Compound Name	Response	Retention Time
DDT	1509873	20.71
DDD	13205	20.28
DDE	1832	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15037	1524910	0.99

Instrument :
BNA_P
ClientSampleId :
DFTPP