
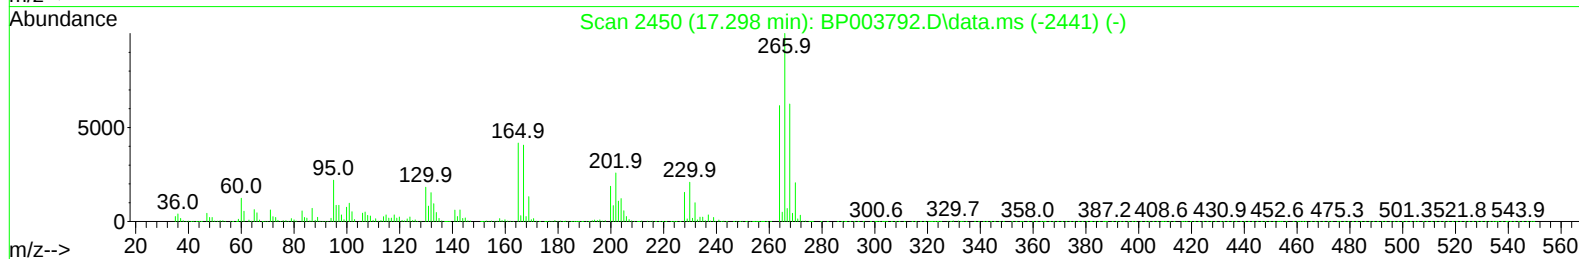
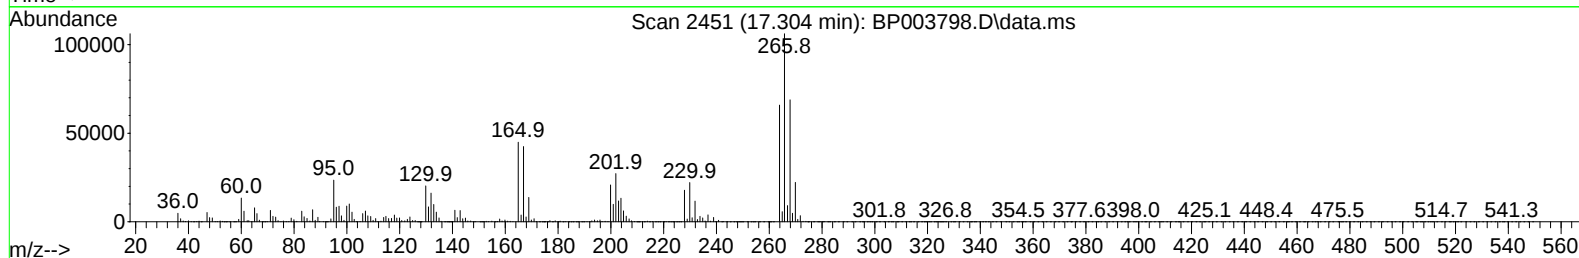


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110420\
Data File : BP003798.D
Acq On : 04 Nov 2020 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 02:03:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 16:37:10 2020
Response via : Initial Calibration

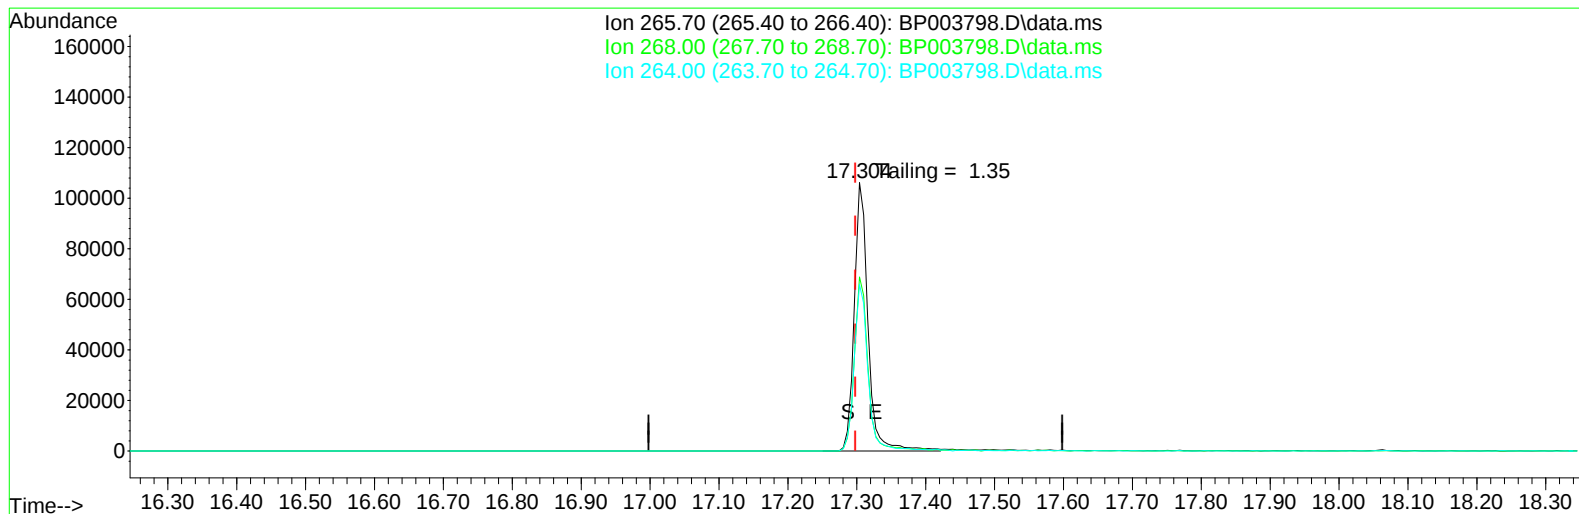

TIC: BP003798.D\data.ms

(70) Pentachlorophenol (C)




17.304min (+ 0.006) 15714.95 ng

response 108291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.88
264.00	63.30	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110420\
Data File : BP003798.D
Acq On : 04 Nov 2020 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 02:03:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 16:37:10 2020
Response via : Initial Calibration

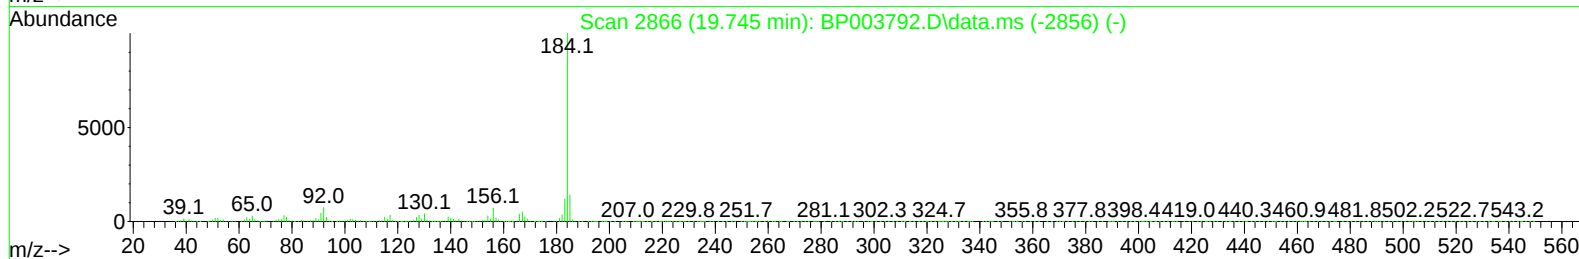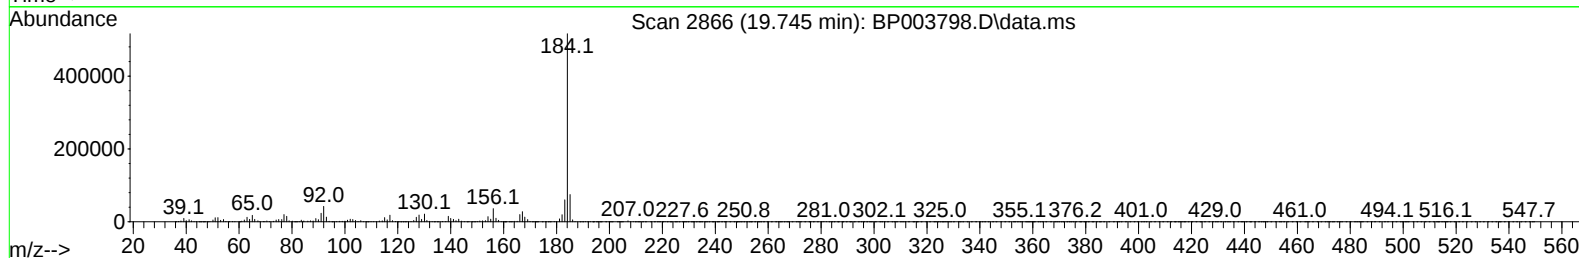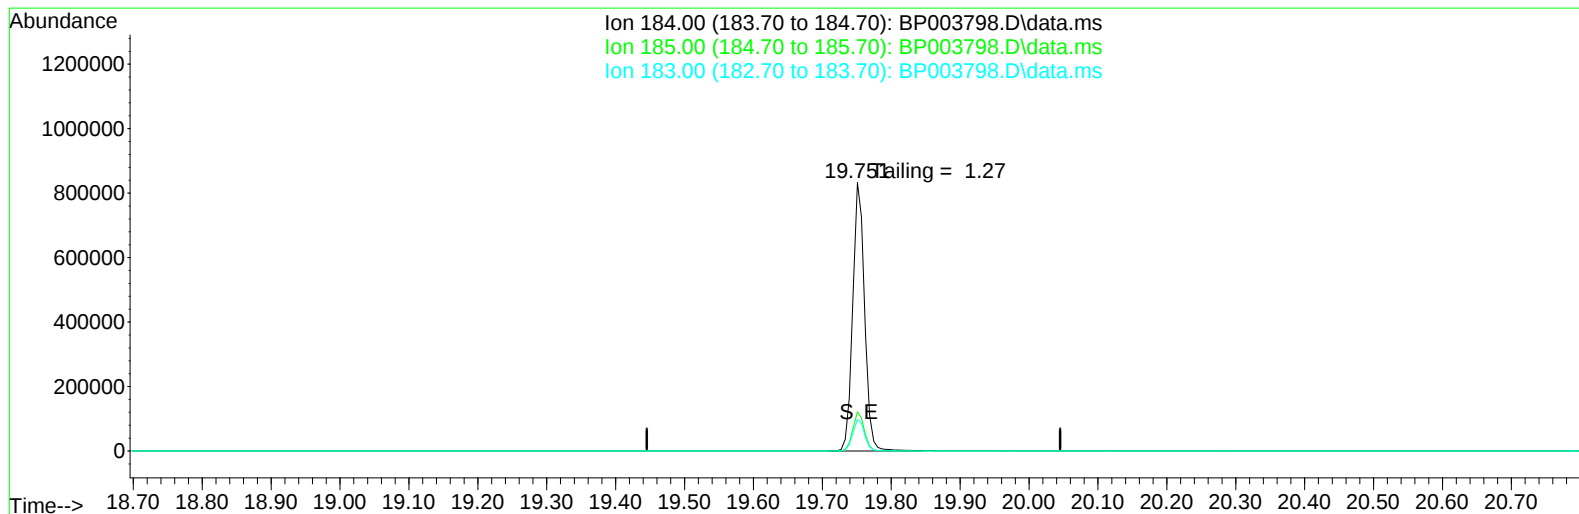

TIC: BP003798.D\data.ms

(77) Benzidine

19.745min (-19.745) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00