
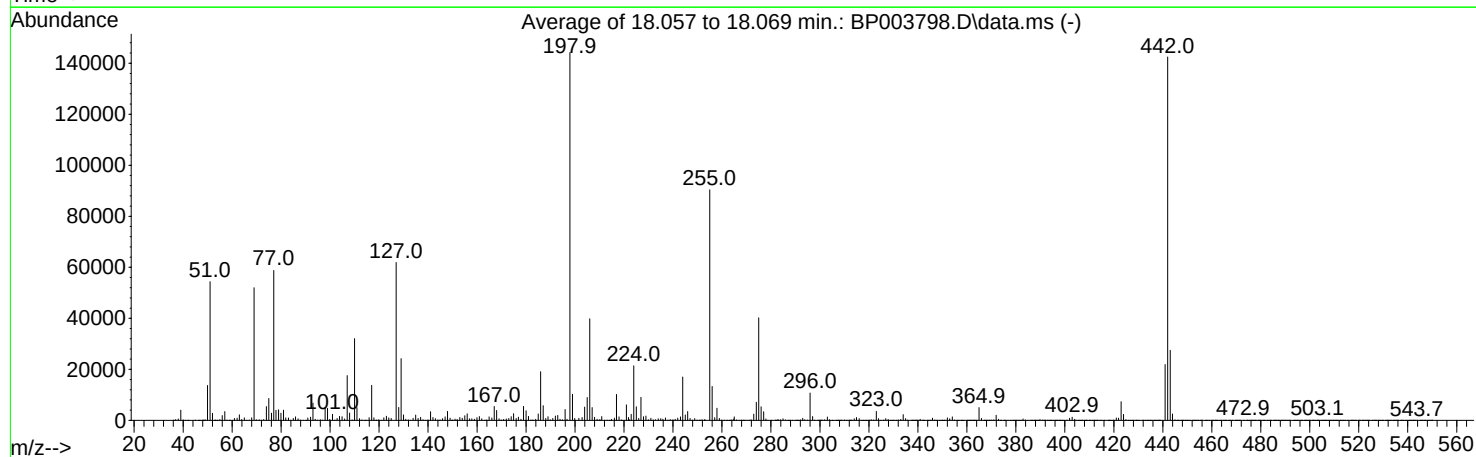


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110420\
 Data File : BP003798.D
 Acq On : 04 Nov 2020 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 12 15:22:47 2020

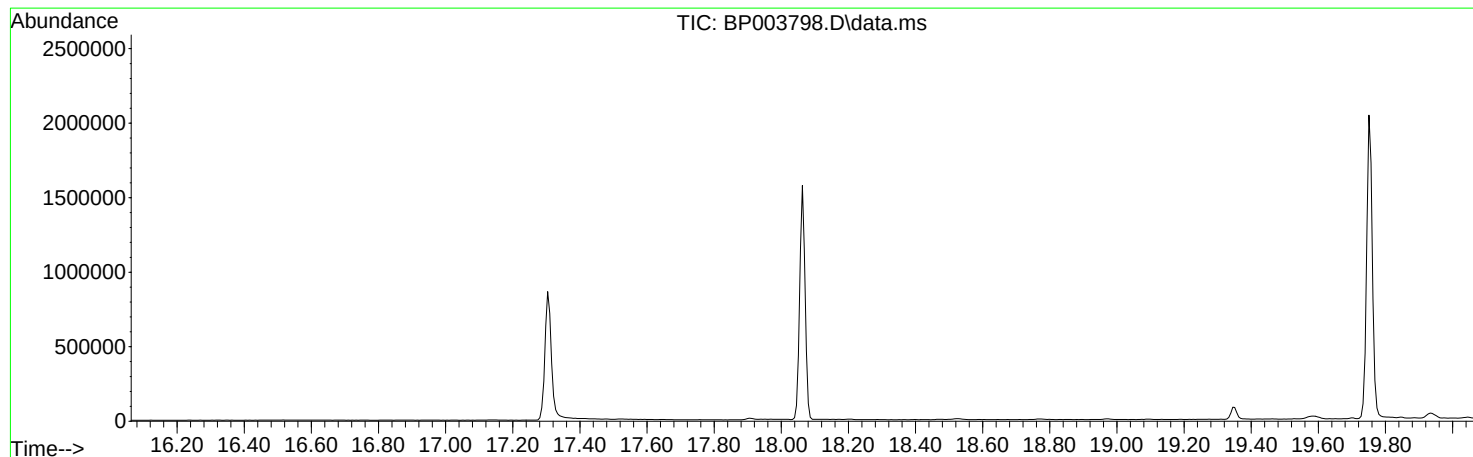

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	54380	PASS
68	69	0.00	2	2.0	1037	PASS
69	198	0.00	100	36.1	51999	PASS
70	69	0.00	2	0.5	283	PASS
127	198	10	80	42.9	61888	PASS
197	198	0.00	2	0.3	431	PASS
198	198	100	100	100.0	144205	PASS
199	198	5	9	7.1	10225	PASS
275	198	10	60	27.9	40187	PASS
365	198	1	100	3.5	5011	PASS
441	198	0.01	100	15.2	21876	PASS
442	198	50	100	98.8	142451	PASS
443	442	15	24	19.3	27460	PASS