

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
 Data File : BP007843.D
 Acq On : 04 Nov 2021 12:14
 Operator : CG/JU
 Sample : PB140389BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140389BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	367	375	387	rBV	4209973	6254938	37.61%	9.309%
2	7.087	638	646	656	rBV	3849407	6087488	36.61%	9.060%
3	7.911	779	786	794	rBV	748494	1164966	7.01%	1.734%
4	9.075	976	984	997	rBV	2253021	3785250	22.76%	5.633%
5	10.716	1255	1263	1276	rBV	961634	1639843	9.86%	2.441%
6	13.181	1674	1682	1697	rBV	6392115	9601579	57.74%	14.290%
7	14.551	1906	1915	1924	rBV	1677590	2446923	14.71%	3.642%
8	16.045	2159	2169	2191	rBV	5668955	8200813	49.32%	12.205%
9	17.310	2376	2384	2396	rBV	2175722	3166438	19.04%	4.713%
10	19.875	2814	2820	2825	rBV	12883699	16628845	100.00%	24.748%
11	21.398	3074	3079	3091	rVB	2980999	4152278	24.97%	6.180%
12	23.833	3486	3493	3504	rVB2	1924460	4062871	24.43%	6.047%




Sum of corrected areas: 67192232

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
Data File : BP007843.D
Acq On : 04 Nov 2021 12:14
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

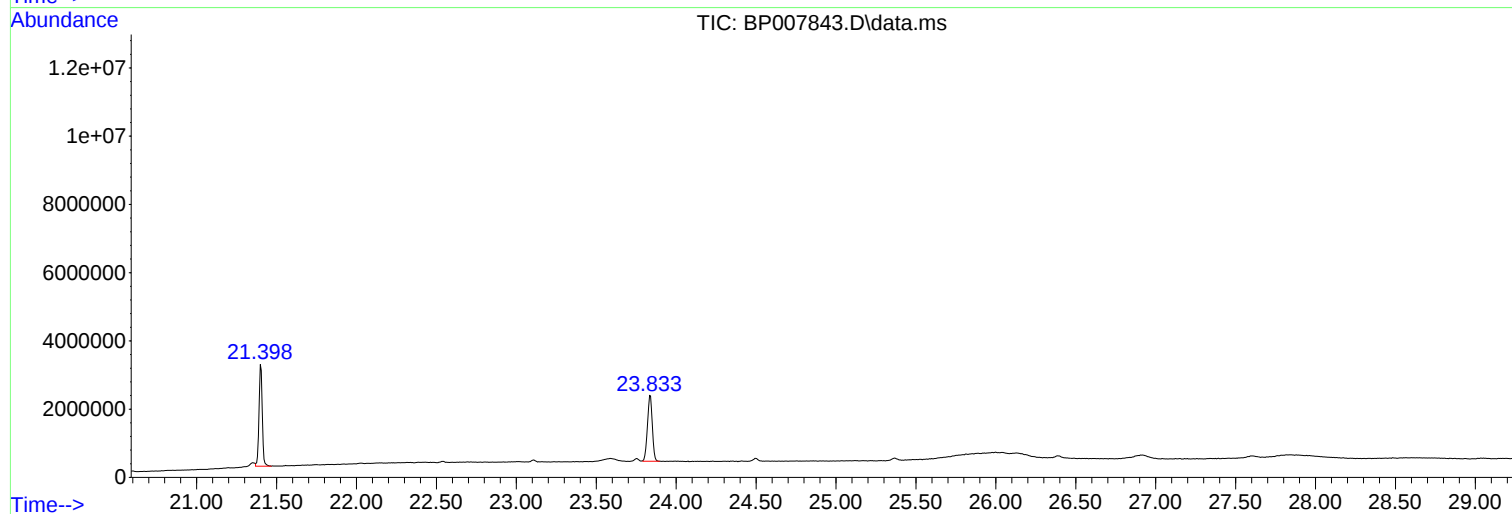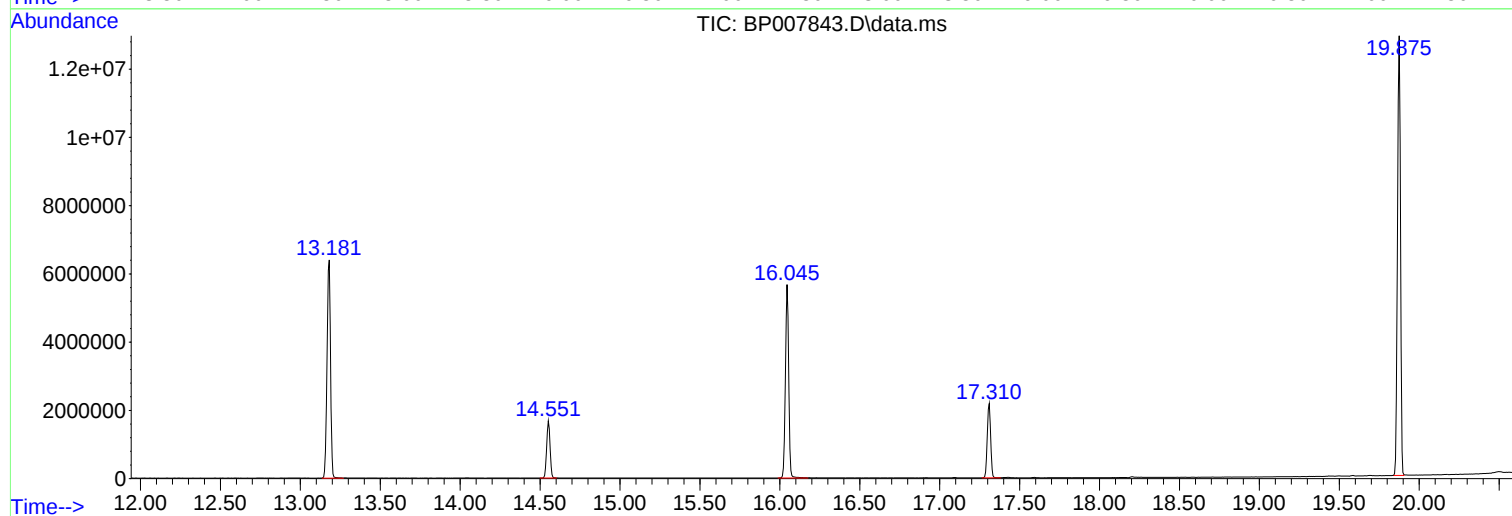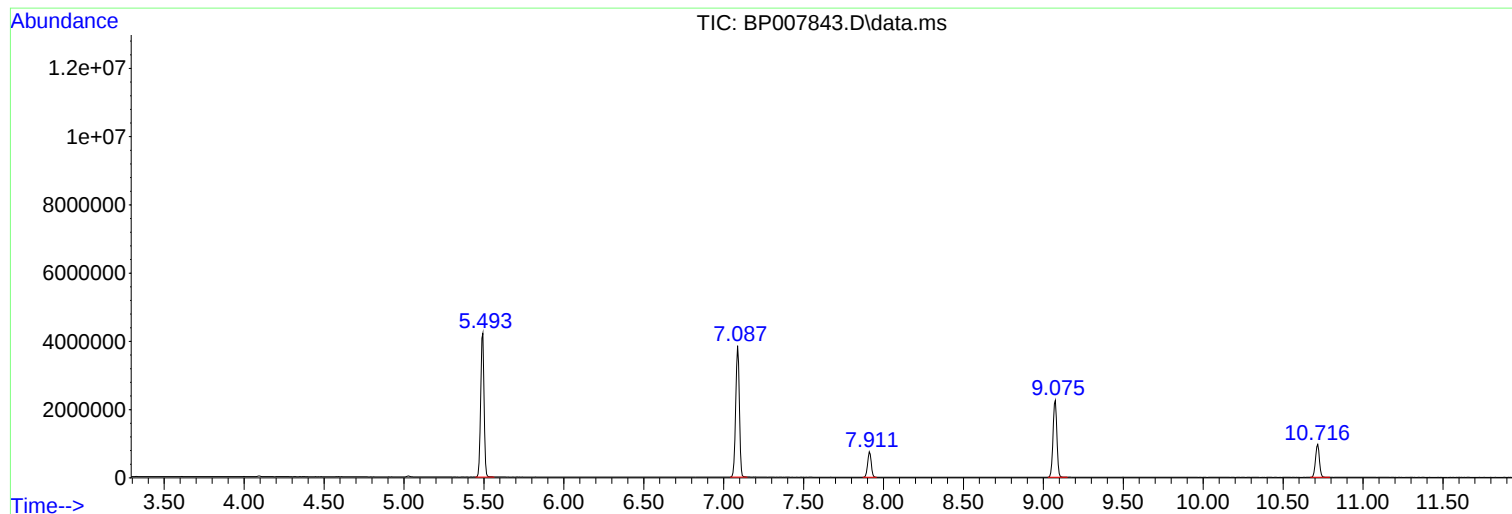

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
Data File : BP007843.D
Acq On : 04 Nov 2021 12:14
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
Data File : BP007843.D
Acq On : 04 Nov 2021 12:14
Operator : CG/JU
Sample : PB140389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------