


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
 Data File : BP007841.D
 Acq On : 04 Nov 2021 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 09 10:45:24 2021

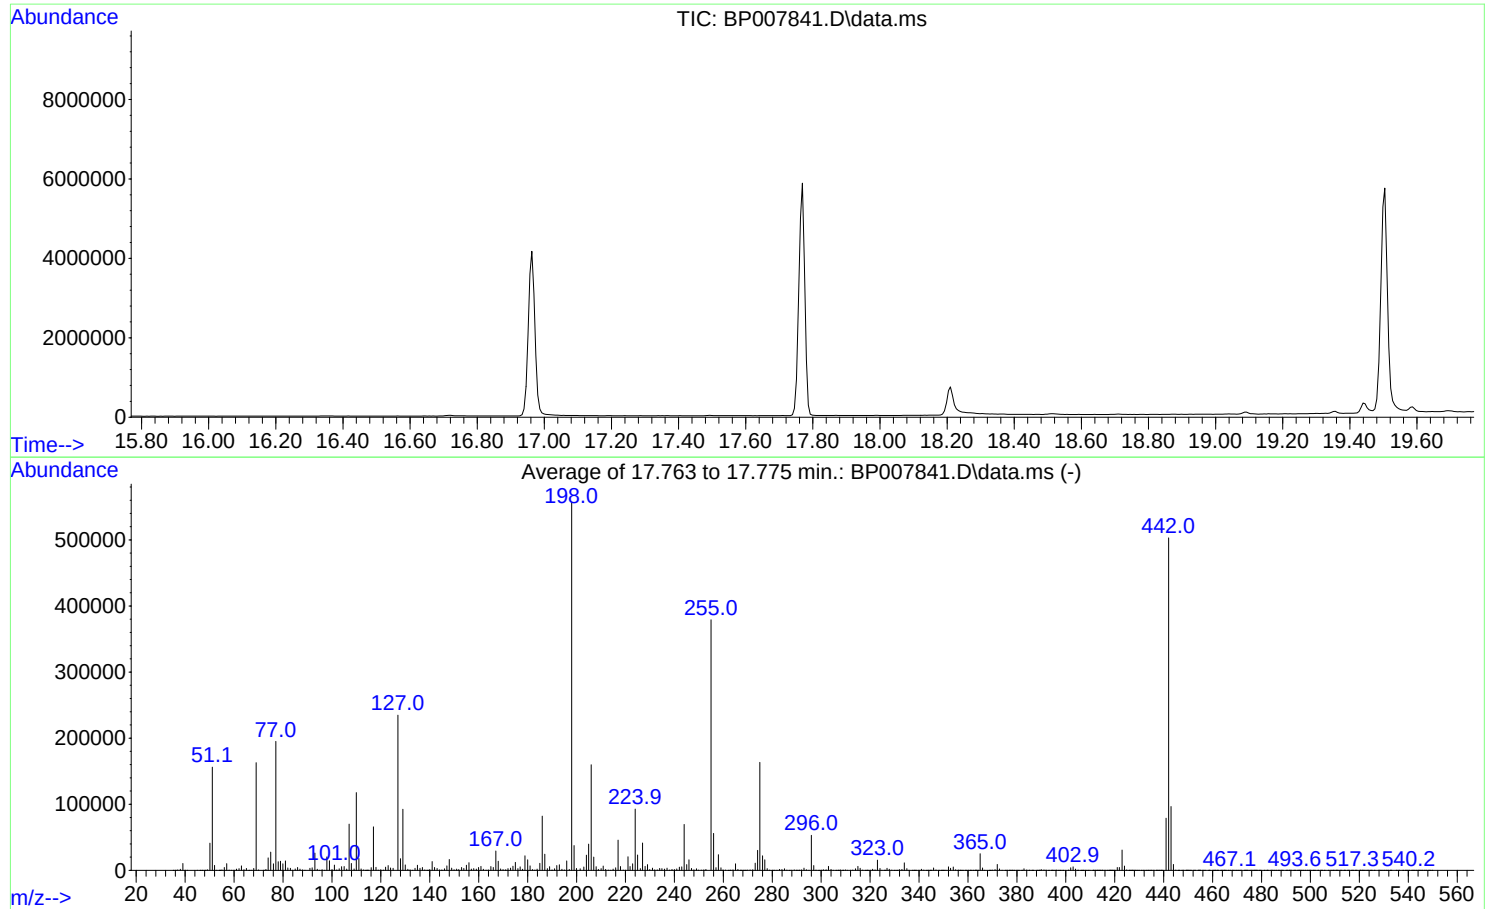




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	156177	PASS
68	69	0.00	2	1.7	2833	PASS
69	198	0.00	100	29.3	162820	PASS
70	69	0.00	2	0.5	765	PASS
127	198	10	80	42.2	234837	PASS
197	198	0.00	2	0.3	1516	PASS
198	198	100	100	100.0	556576	PASS
199	198	5	9	6.8	37572	PASS
275	198	10	60	29.3	163336	PASS
365	198	1	100	4.5	25204	PASS
441	198	0.01	100	14.2	79017	PASS
442	442	100	100	100.0	503083	PASS
443	442	15	24	19.2	96675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
Data File : BP007841.D
Acq On : 04 Nov 2021 11:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 07 11:28:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 19:18:55 2021
Response via : Initial Calibration

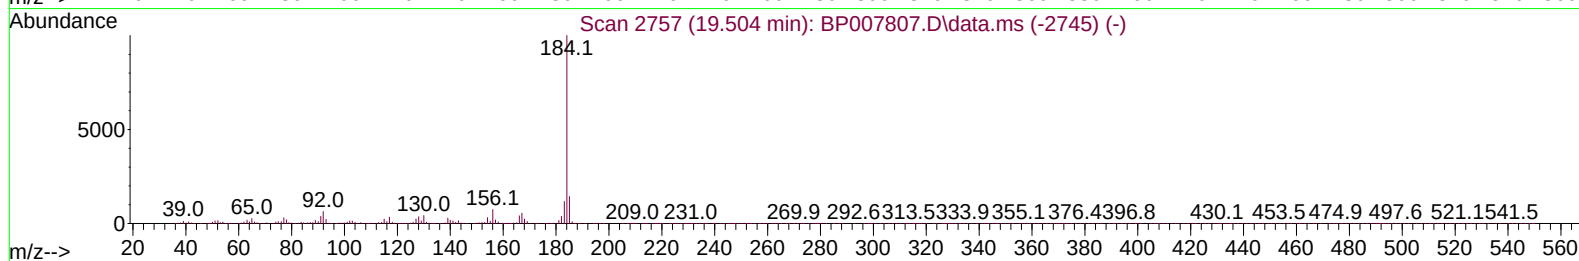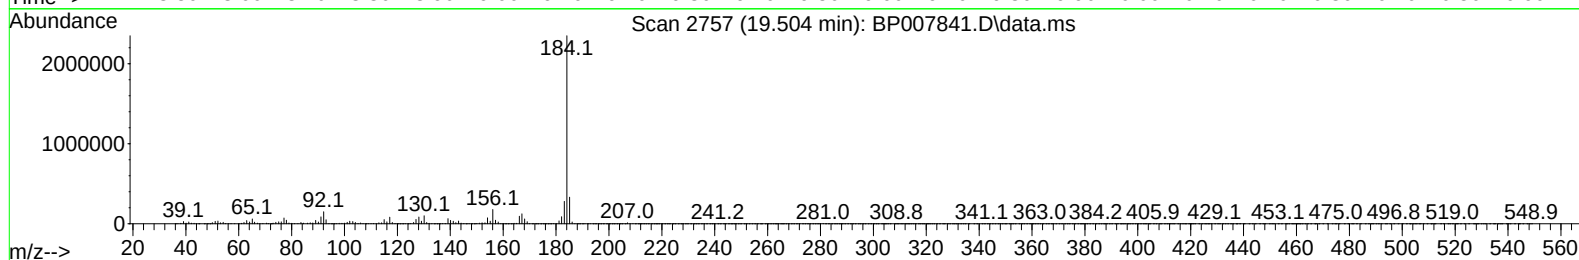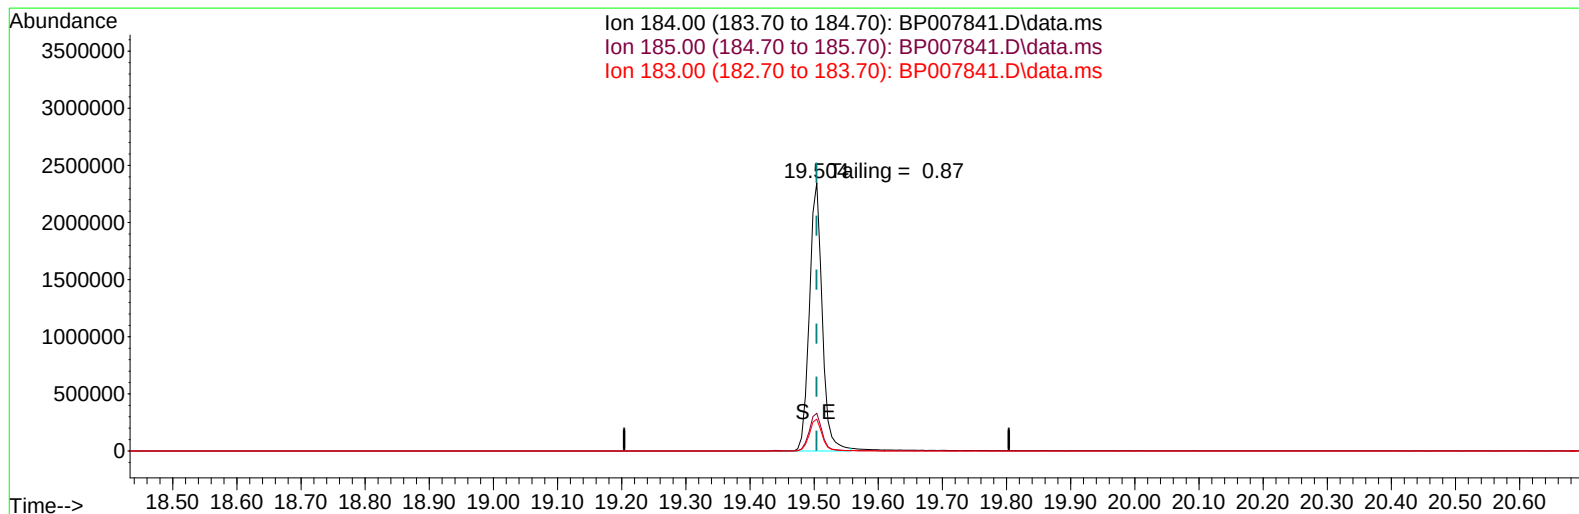

TIC: BP007841.D\data.ms

(77) Benzidine

19.504min (+ 0.000) 438551.39 ng




response 3337937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.11
183.00	11.40	11.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110421\
Data File : BP007841.D
Acq On : 04 Nov 2021 11:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 07 11:28:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 19:18:55 2021
Response via : Initial Calibration

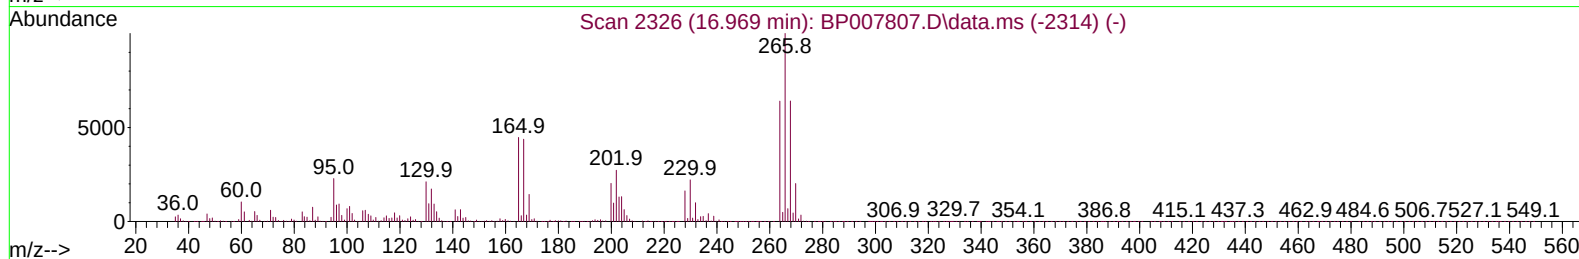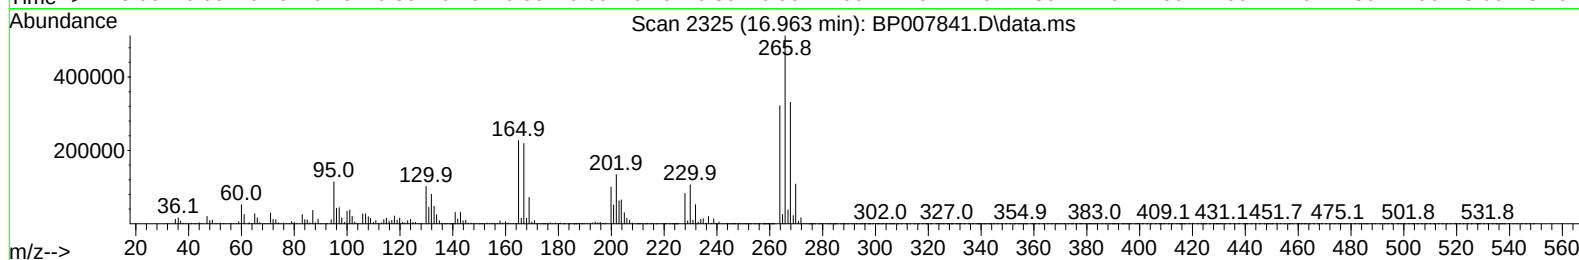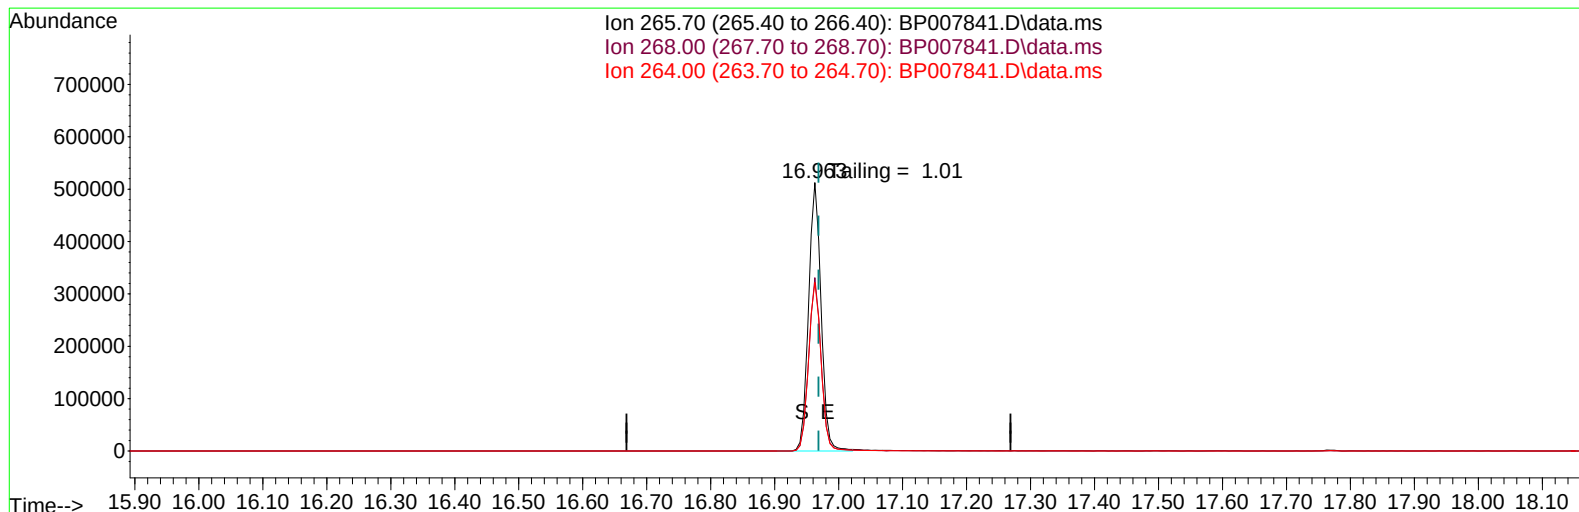

TIC: BP007841.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.006) 1089114.19 ng

response 709563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.56
264.00	60.90	62.77
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
11/4/2021	BNA_P	BP007841.D
Compound Name	Response	Retention Time
DDT	2170219	20.71
DDD	34691	20.28
DDE	1539	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36230	2206449	1.64