




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022900.D
Acq On : 06 Nov 2024 19:17
Operator : RC/JU
Sample : P4622-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6M7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 07 00:55:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

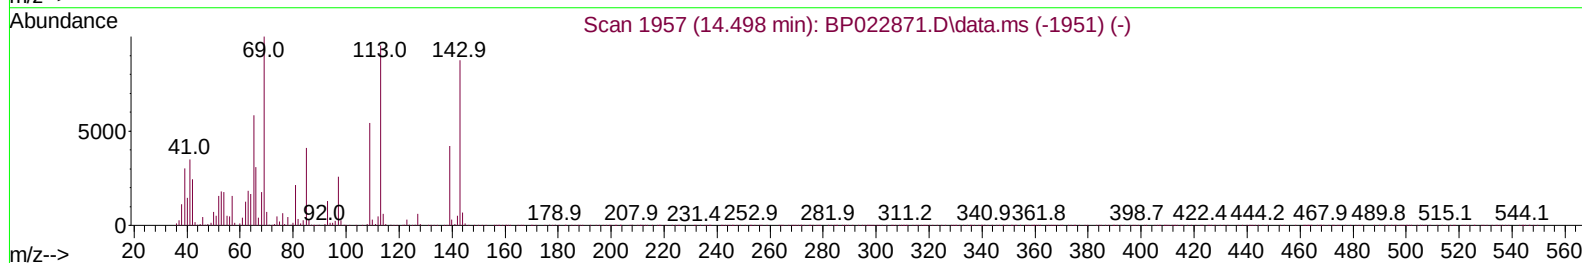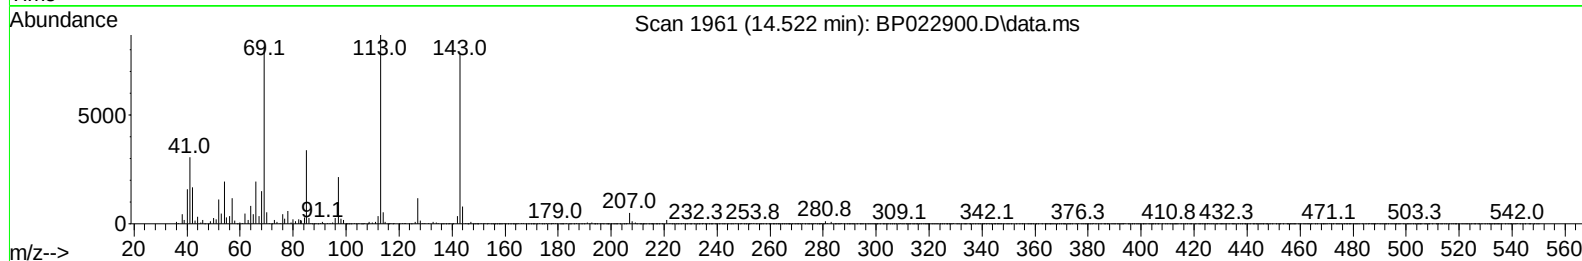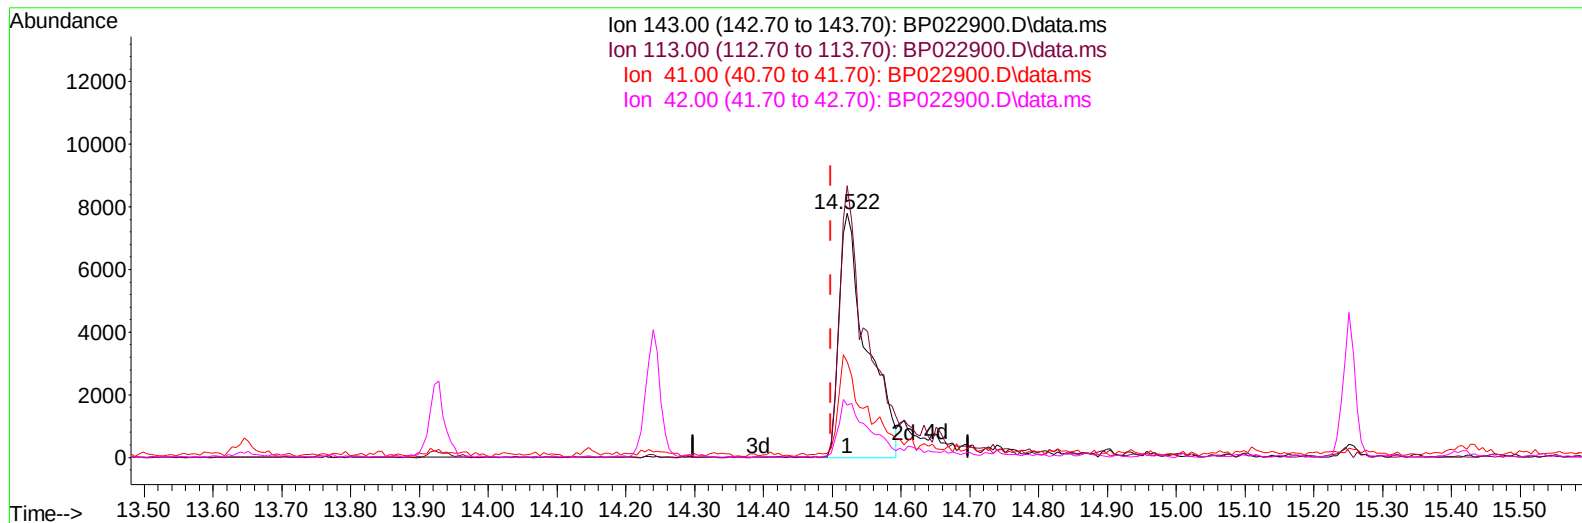

TIC: BP022900.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.024) 8.00 ng/ul

response 21644

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	111.31
41.00	35.90	39.14
42.00	23.70	21.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022900.D
Acq On : 06 Nov 2024 19:17
Operator : RC/JU
Sample : P4622-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6M7

Manual IntegrationsAPPROVED

Quant Time: Nov 07 00:55:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

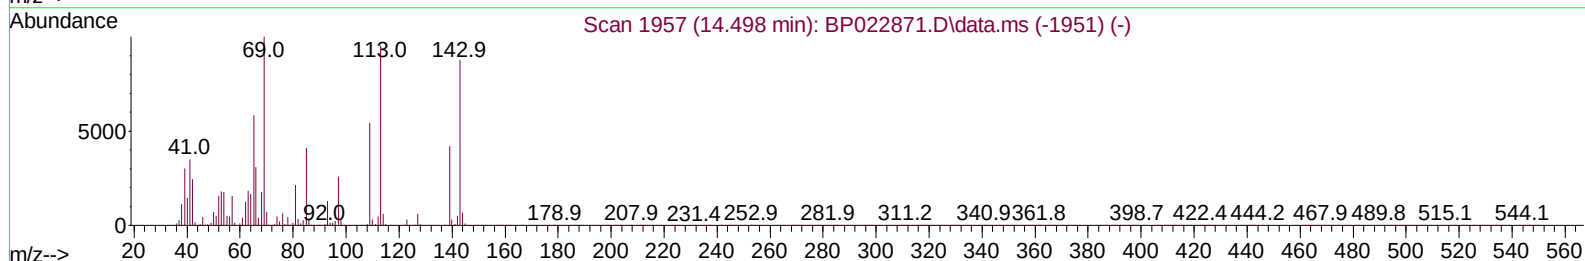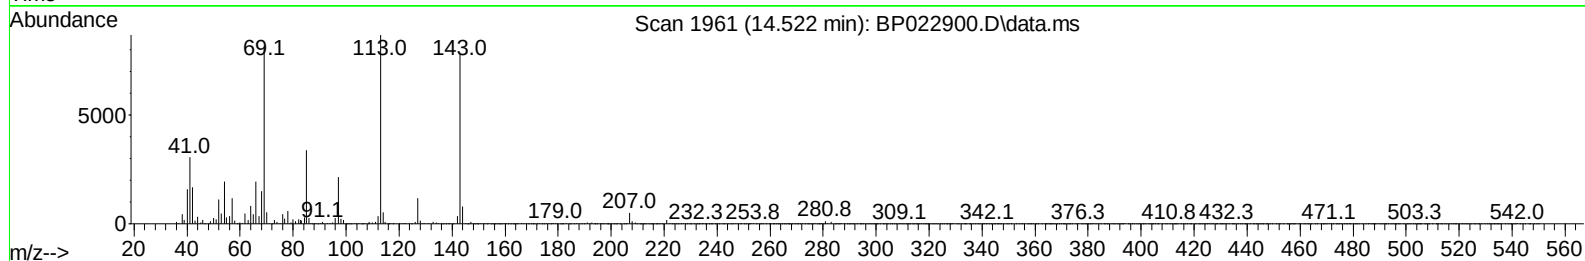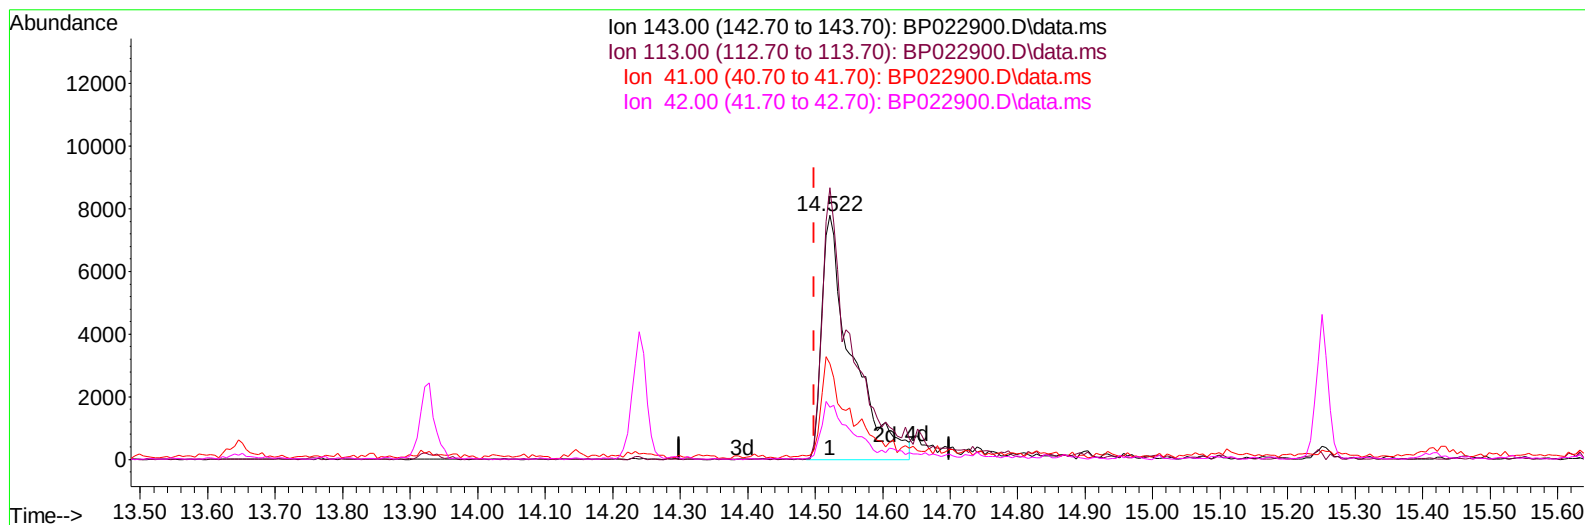

TIC: BP022900.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.024) 8.84 ng/ul m

response 23906

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.60	111.31
41.00	35.90	39.14
42.00	23.70	21.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022900.D
 Acq On : 06 Nov 2024 19:17
 Operator : RC/JU
 Sample : P4622-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6M7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/07/2024
 Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 07 00:56:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 00:31:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	69493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	262352	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.240	164	202918	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.033	188	475141	20.000	ng/ul	-0.02
79) Chrysene-d12	21.492	240	478950	20.000	ng/ul	0.00
88) Perylene-d12	24.745	264	565559	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	3294	1.842	ng/uL	0.00
4) Pyridine-d5	3.611	84	5327	1.085	ng/ul	0.02
7) Phenol-d5	6.822	99	78031	13.339	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.963	67	44885	13.055	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	58973	14.208	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	67754	14.513	ng/ul	0.00
21) Nitrobenzene-d5	8.763	128	30048	14.896	ng/ul	0.00
24) 2-Nitrophenol-d4	9.475	143	35967	15.401	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	71610	14.427	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	80929	13.798	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166	247954	15.380	ng/ul	-0.02
49) Acenaphthylene-d8	13.928	160	290371	16.957	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	23906m	8.839	ng/ul	0.02
60) Fluorene-d10	15.251	176	247770	17.718	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	14652	4.689	ng/ul	0.00
73) Anthracene-d10	17.151	188	386104	17.274	ng/ul	-0.01
81) Pyrene-d10	19.527	212	491085	19.389	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.504	264	548441	18.158	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022900.D
Acq On : 06 Nov 2024 19:17
Operator : RC/JU
Sample : P4622-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6M7

Manual IntegrationsAPPROVED

Quant Time: Nov 07 00:56:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

