




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022903.D
 Acq On : 06 Nov 2024 21:20
 Operator : RC/JU
 Sample : P4622-04
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N0

Manual IntegrationsAPPROVED

Quant Time: Nov 07 01:07:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 00:31:03 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
 Supervised By :mohammad ahmed 11/08/2024

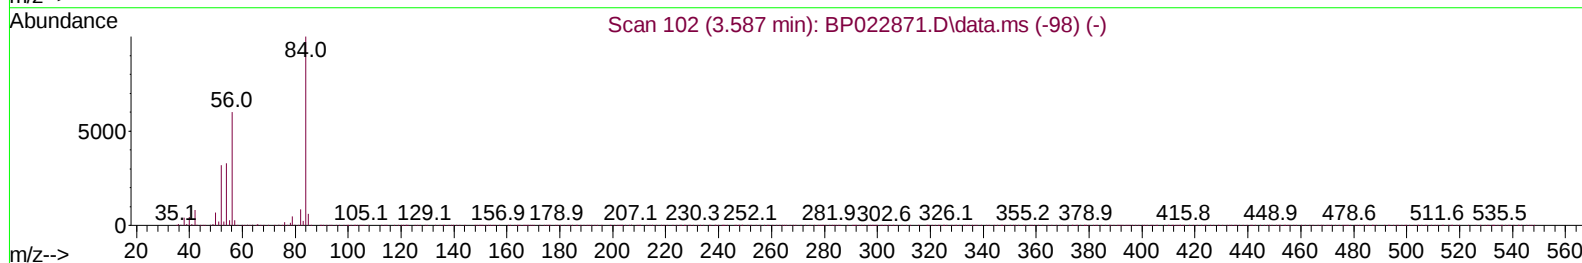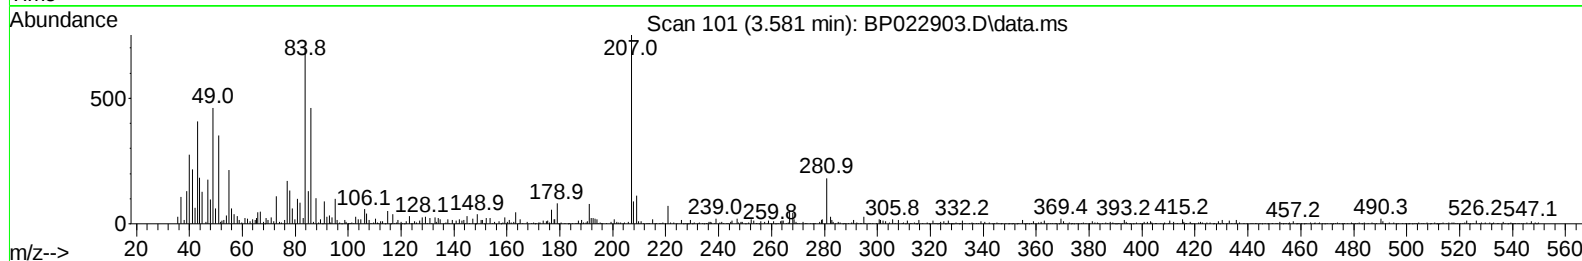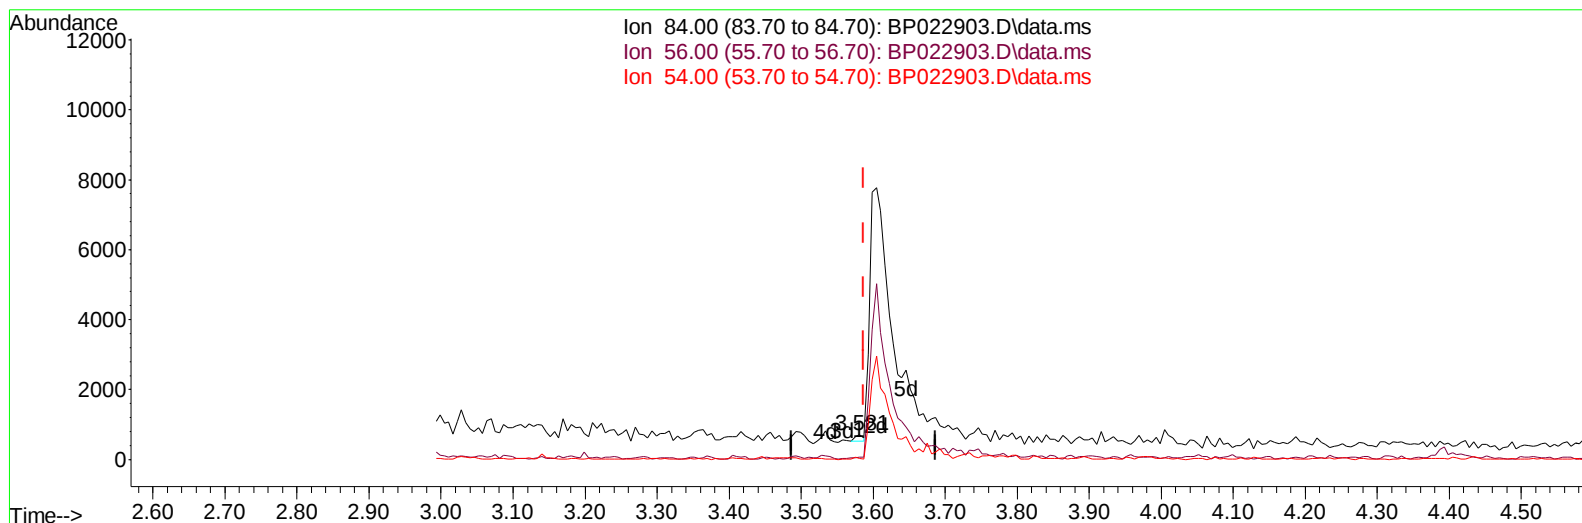

TIC: BP022903.D\data.ms

(4) Pyridine-d5 (S)

3.581min (-0.006) 0.02 ng/u1

response 147

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.10	8.53#
54.00	30.90	4.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022903.D
Acq On : 06 Nov 2024 21:20
Operator : RC/JU
Sample : P4622-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N0

Manual IntegrationsAPPROVED

Quant Time: Nov 07 01:07:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

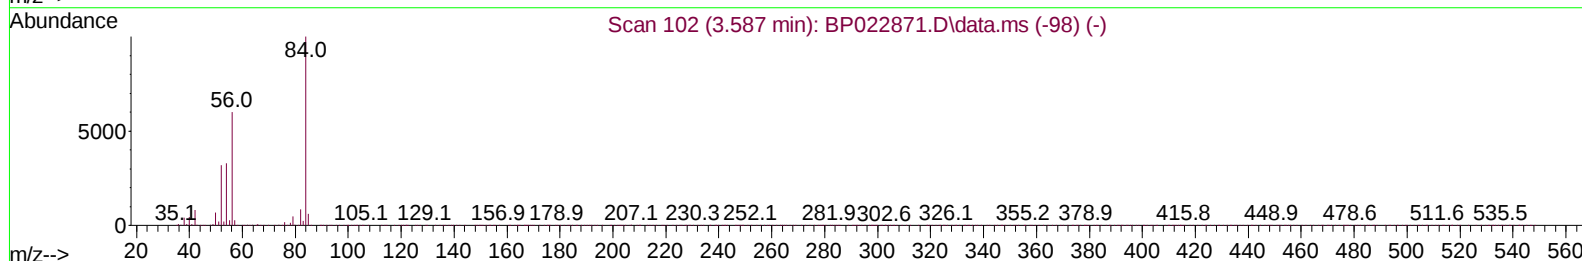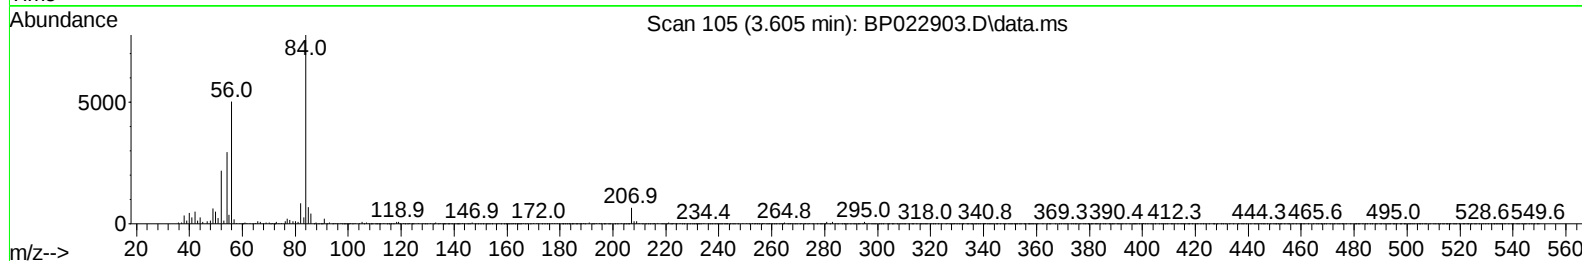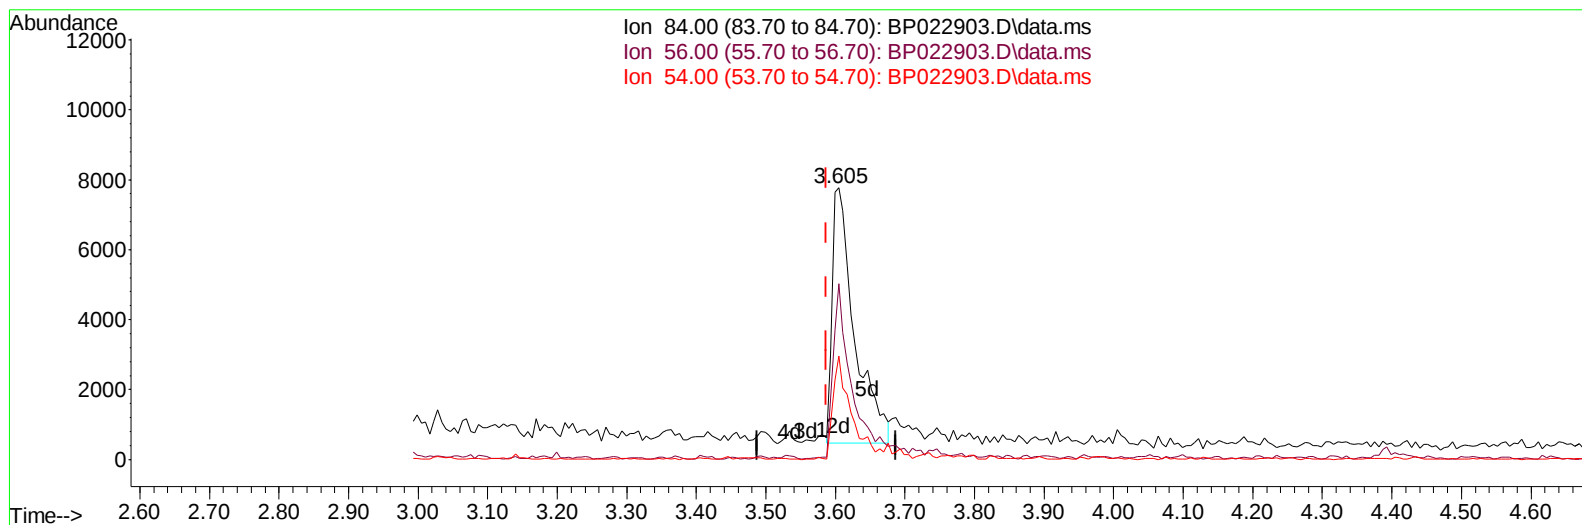

TIC: BP022903.D\data.ms

(4) Pyridine-d5 (S)

3.605min (+ 0.018) 2.58 ng/u1 m

response 16269

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.10	64.70
54.00	30.90	37.99#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022903.D
 Acq On : 06 Nov 2024 21:20
 Operator : RC/JU
 Sample : P4622-04
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/07/2024
 Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 07 01:08:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 00:31:03 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.616	152		89263	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.375	136		338076	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.251	164		262741	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.051	188		637968	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.486	240		682476	20.000	ng/ul	0.00
88) Perylene-d12	24.733	264		809633	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.175	96		4705	2.048	ng/uL	0.00
4) Pyridine-d5	3.605	84		16269m	2.580	ng/ul	0.02
7) Phenol-d5	6.822	99		113499	15.105	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.963	67		62819	14.225	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132		83995	15.754	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113		97308	16.228	ng/ul	-0.01
21) Nitrobenzene-d5	8.763	128		44823	17.243	ng/ul	0.00
24) 2-Nitrophenol-d4	9.475	143		51331	17.056	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.016	165		112923	17.654	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131		117734	15.577	ng/ul	0.00
46) Dimethylphthalate-d6	13.645	166		368022	17.629	ng/ul	-0.02
49) Acenaphthylene-d8	13.934	160		418855	18.891	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143		42602	12.165	ng/ul	0.02
60) Fluorene-d10	15.263	176		364089	20.108	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200		23723	5.654	ng/ul	0.00
73) Anthracene-d10	17.151	188		571543	19.044	ng/ul	-0.01
81) Pyrene-d10	19.539	212		760597	21.075	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.509	264		856332	19.805	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022903.D
Acq On : 06 Nov 2024 21:20
Operator : RC/JU
Sample : P4622-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N0

Manual IntegrationsAPPROVED

Quant Time: Nov 07 01:08:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

