




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022907.D
Acq On : 07 Nov 2024 00:03
Operator : RC/JU
Sample : P4622-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N4

Manual IntegrationsAPPROVED

Quant Time: Nov 07 01:17:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

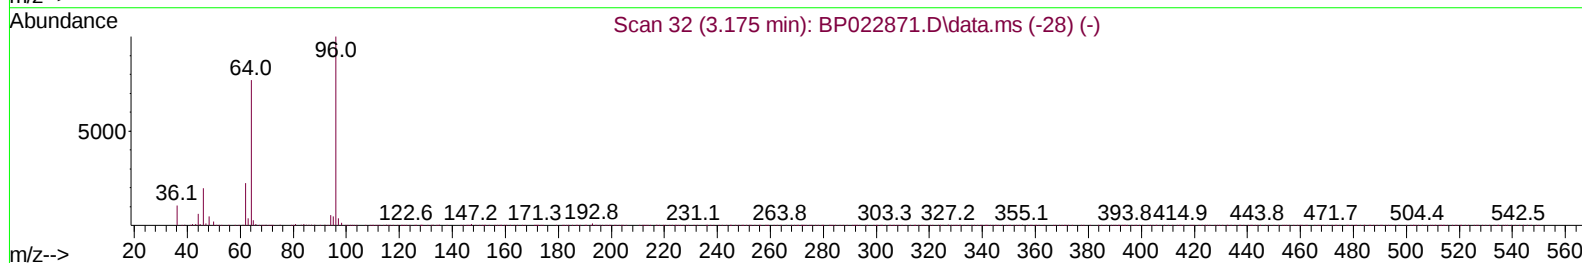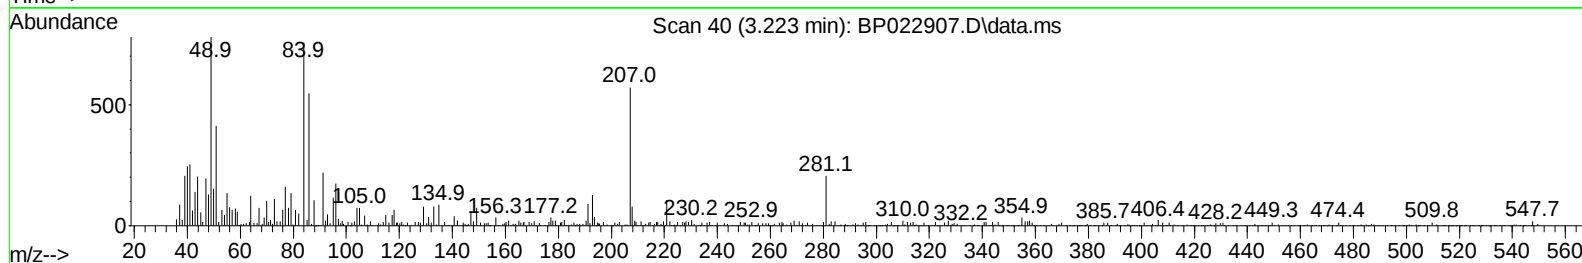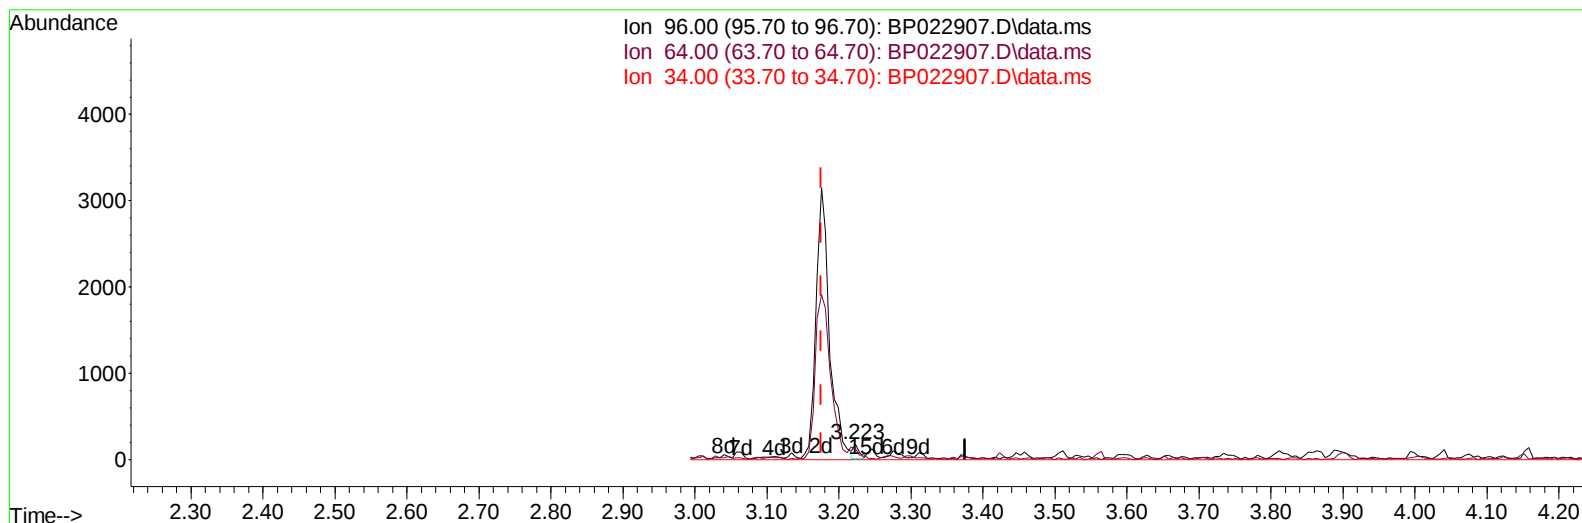

TIC: BP022907.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.223min (+ 0.047) 0.03 ng/uL

response 86

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	70.29
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022907.D
Acq On : 07 Nov 2024 00:03
Operator : RC/JU
Sample : P4622-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 07 01:17:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

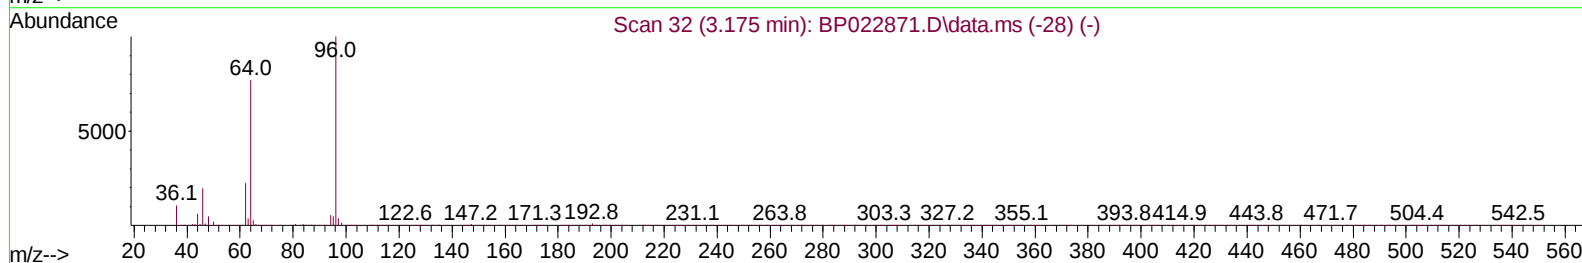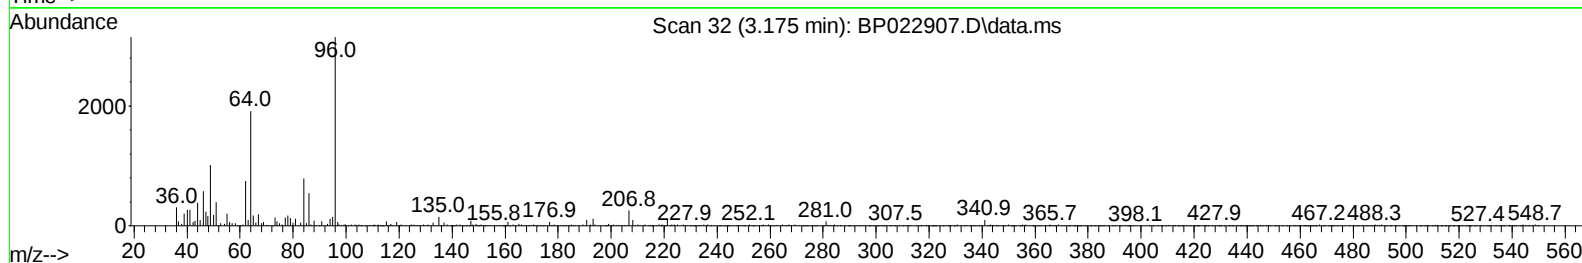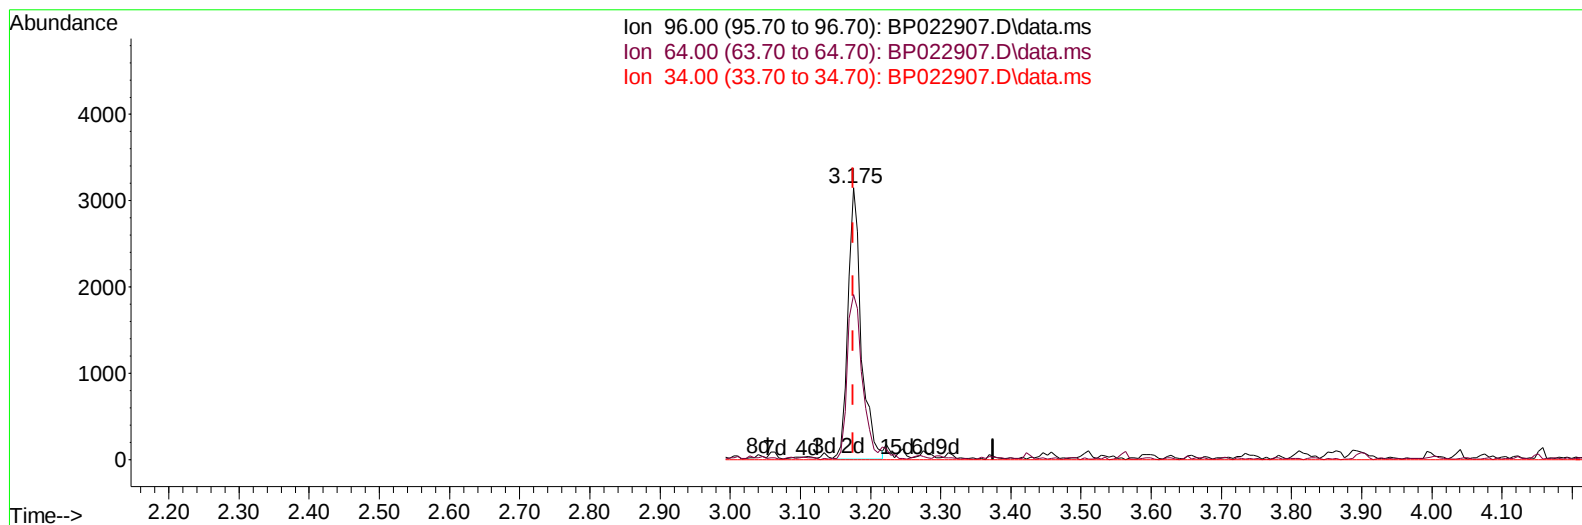

TIC: BP022907.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.175min (+ 0.000) 1.69 ng/uL m

response 4161

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	60.74#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022907.D
 Acq On : 07 Nov 2024 00:03
 Operator : RC/JU
 Sample : P4622-08
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH6N4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/07/2024
 Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 07 01:19:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 00:31:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	95710	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	363475	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.240	164	277376	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.051	188	664326	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	688970	20.000	ng/ul	0.00
88) Perylene-d12	24.745	264	827121	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	4161m	1.689	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.822	99	118681	14.731	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	67836	14.326	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	88103	15.411	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	101790	15.832	ng/ul	0.00
21) Nitrobenzene-d5	8.763	128	46571	16.664	ng/ul	0.00
24) 2-Nitrophenol-d4	9.475	143	53300	16.473	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	119199	17.333	ng/ul	0.00
31) 4-Chloroaniline-d4	10.528	131	112237	13.812	ng/ul	0.00
46) Dimethylphthalate-d6	13.640	166	308261	13.988	ng/ul	-0.02
49) Acenaphthylene-d8	13.928	160	459452	19.629	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	41029	11.097	ng/ul	0.02
60) Fluorene-d10	15.263	176	387958	20.296	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	12256	2.805	ng/ul	0.00
73) Anthracene-d10	17.145	188	632892	20.252	ng/ul	-0.02
81) Pyrene-d10	19.545	212	795787	21.842	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.527	264	916909	20.757	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022907.D
Acq On : 07 Nov 2024 00:03
Operator : RC/JU
Sample : P4622-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH6N4

Manual IntegrationsAPPROVED

Quant Time: Nov 07 01:19:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 00:31:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/07/2024
Supervised By :mohammad ahmed 11/08/2024

