

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022834.D
 Acq On : 04 Nov 2024 19:42
 Operator : RC/JU
 Sample : P4568-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EE6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/06/2024
 Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 04 21:43:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 30 10:56:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	74727	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.387	136	286093	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	222359	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	549177m	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	556580	20.000	ng/ul	-0.02
88) Perylene-d12	24.727	264	701282	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	2018	1.049	ng/uL	0.00
4) Pyridine-d5	3.623	84	4393m	0.832	ng/ul	0.03
7) Phenol-d5	6.834	99	37522	5.965	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	21778	5.891	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	28878	6.470	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	24953	4.971	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	14314	6.507	ng/ul	0.00
24) 2-Nitrophenol-d4	9.487	143	16294	6.398	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.040	165	35352	6.531	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	12893m	2.016	ng/ul	0.01
46) Dimethylphthalate-d6	13.651	166	132964	7.526	ng/ul	-0.01
49) Acenaphthylene-d8	13.940	160	129353	6.894	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.546	143	10994m	3.709	ng/ul	0.04
60) Fluorene-d10	15.263	176	120921	7.891	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.416	200	10904m	3.019	ng/ul	0.01
73) Anthracene-d10	17.151	188	183987	7.122	ng/ul	-0.02
81) Pyrene-d10	19.534	212	186227	6.327	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.510	264	152063	4.060	ng/ul	-0.01
Target Compounds					Qvalue	
8) Phenol	6.858	94	16868m	2.577	ng/ul	
16) Acetophenone	8.446	105	59306	7.156	ng/ul	93
72) Phenanthrene	17.098	178	109355m	3.722	ng/ul	
80) Fluoranthene	19.192	202	174629	5.161	ng/ul#	96
82) Pyrene	19.563	202	100334	2.767	ng/ul	99
85) Benzo(a)anthracene	21.463	228	71826	1.841	ng/ul	98
87) Chrysene	21.528	228	77344	2.138	ng/ul	97
90) Benzo(b)fluoranthene	23.716	252	98615	2.234	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022834.D
Acq On : 04 Nov 2024 19:42
Operator : RC/JU
Sample : P4568-16
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4EE6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/06/2024
Supervised By :mohammad ahmed 11/08/2024

Quant Time: Nov 04 21:43:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 30 10:56:39 2024
Response via : Initial Calibration

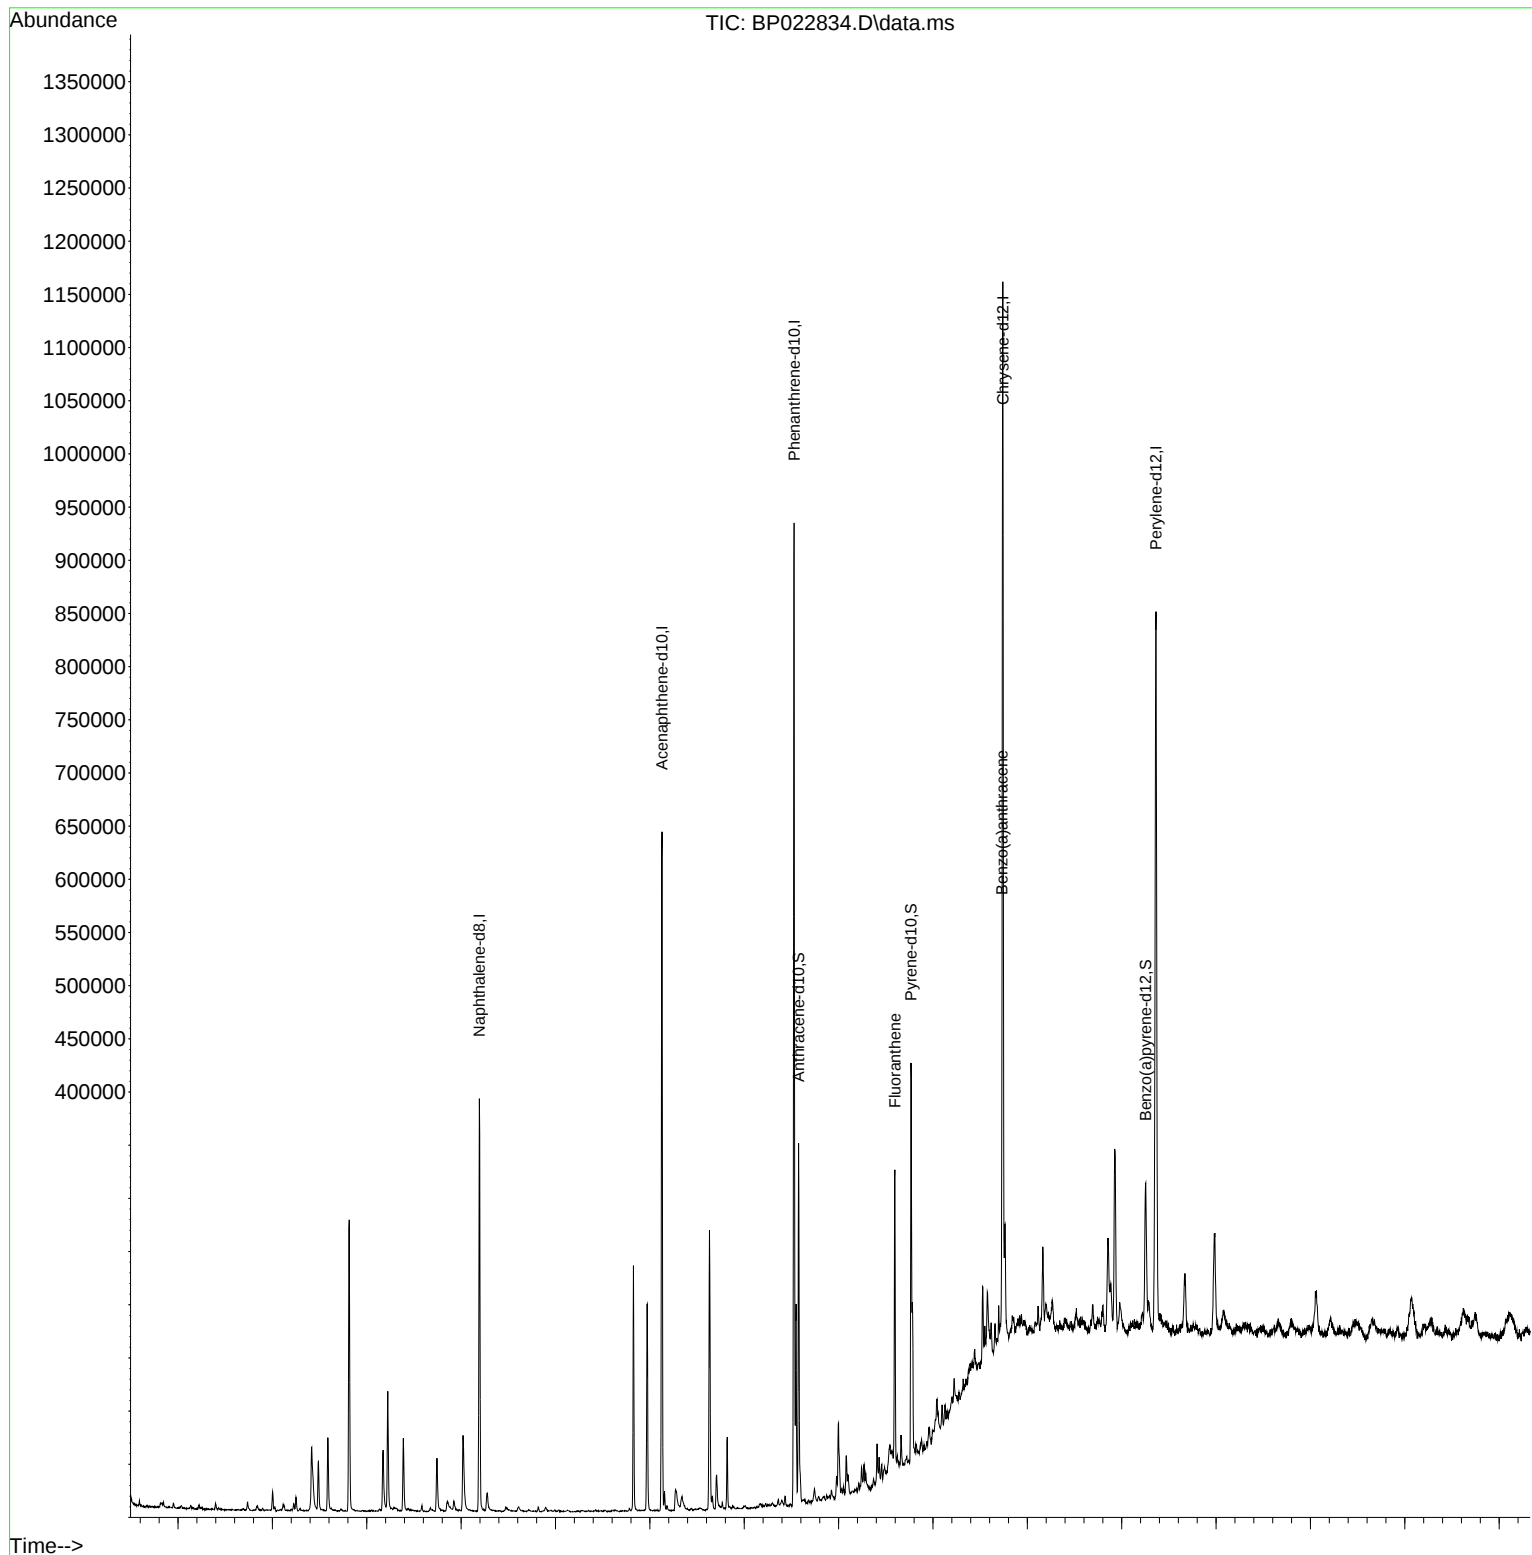

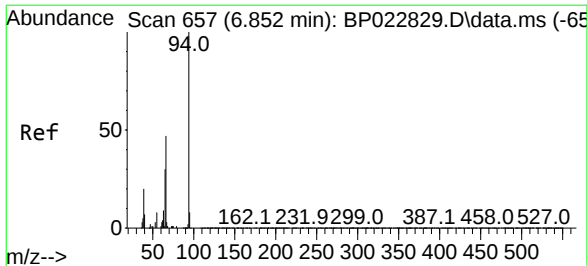





#8
Phenol
Concen: 2.577 ng/u1 m
RT: 6.858 min Scan# 65
Delta R.T. 0.000 min
Lab File: BP022834.D
Acq: 04 Nov 2024 19:42

Instrument :
BNA_P
ClientSampleId :
A4EE6

Tgt Ion:	94	Resp:	16868
Ion	Ratio	Lower	Upper
94	100		
65	36.7	25.9	38.9
66	54.0	37.6	56.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/06/2024
Supervised By :mohammad ahmed 11/08/2024

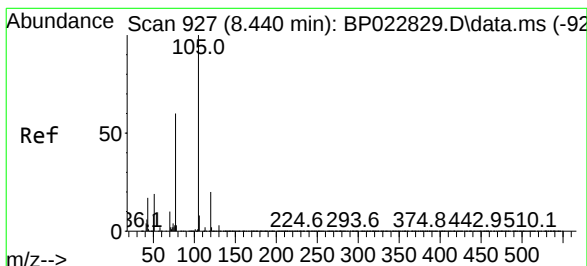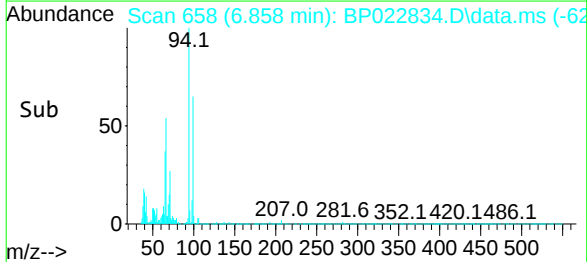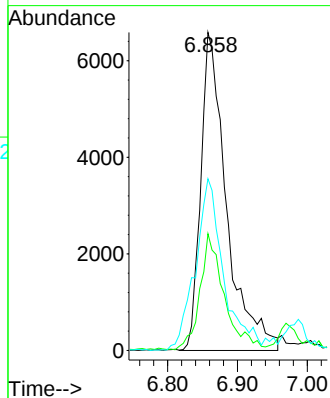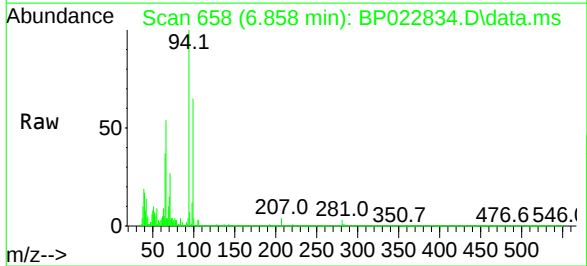

#16
Acetophenone
Concen: 7.156 ng/u1
RT: 8.446 min Scan# 928
Delta R.T. -0.006 min
Lab File: BP022834.D
Acq: 04 Nov 2024 19:42


Tgt Ion:	105	Resp:	59306
Ion	Ratio	Lower	Upper
105	100		
77	78.7	69.0	103.4
51	27.3	22.6	33.8

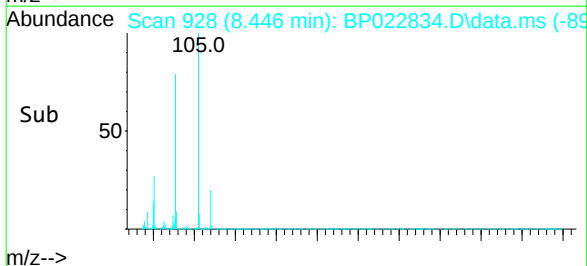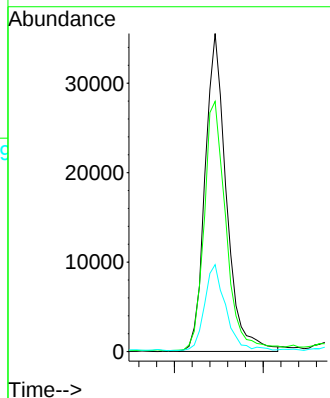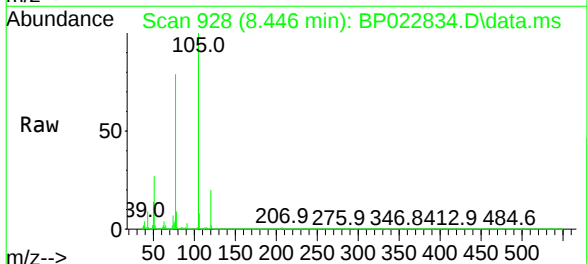

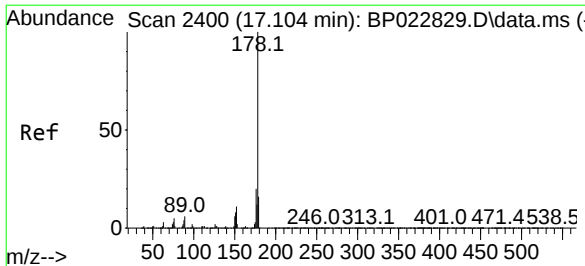

#72
Phenanthrene
Concen: 3.722 ng/u1 m
RT: 17.098 min Scan# 2399
Delta R.T. -0.006 min
Lab File: BP022834.D
Acq: 04 Nov 2024 19:42




Instrument :
BNA_P
ClientSampleId :
A4EE6

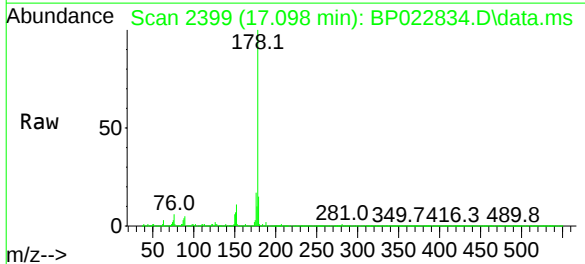

Tgt Ion:178 Resp: 109355
Ion Ratio Lower Upper
178 100
179 15.0 12.2 18.4
176 17.4 15.7 23.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/06/2024
Supervised By :mohammad ahmed 11/08/2024

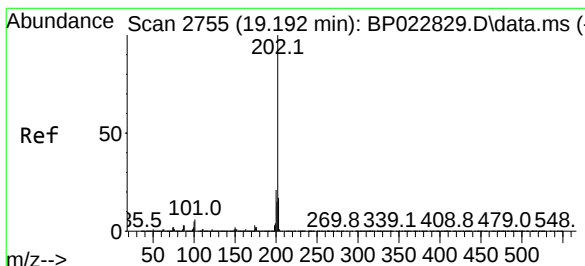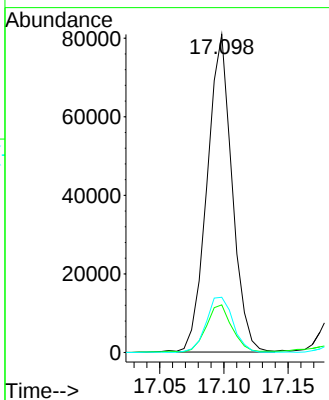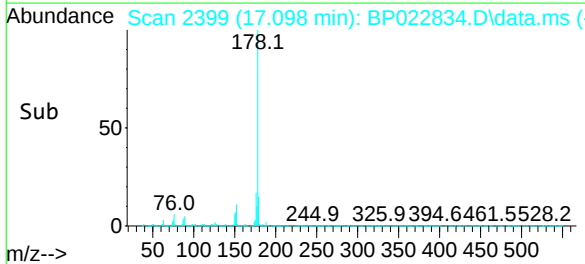

#80
Fluoranthene
Concen: 5.161 ng/u1
RT: 19.192 min Scan# 2755
Delta R.T. 0.000 min
Lab File: BP022834.D
Acq: 04 Nov 2024 19:42

Tgt Ion:202 Resp: 174629
Ion Ratio Lower Upper
202 100
101 5.4 5.8 8.8#
100 4.6 4.5 6.7

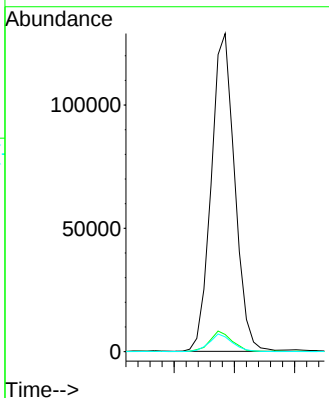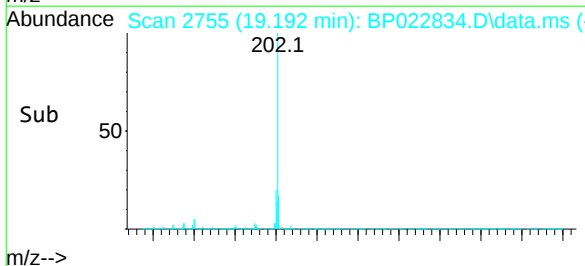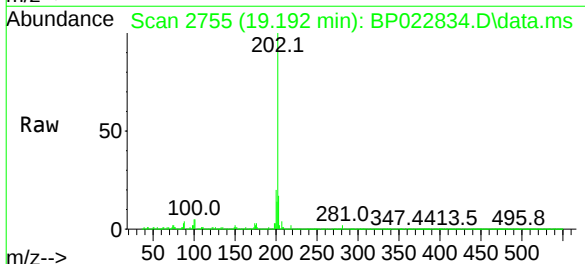

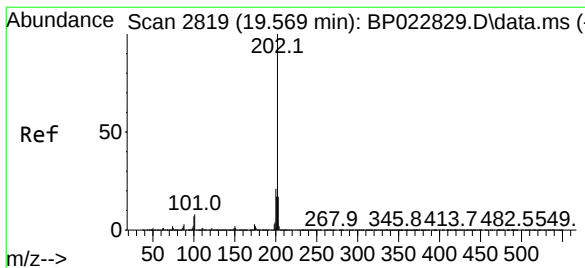

#82

Pyrene

Concen: 2.767 ng/u1

RT: 19.563 min Scan# 2819

Delta R.T. -0.012 min

Lab File: BP022834.D

Acq: 04 Nov 2024 19:42

Instrument :

BNA_P

ClientSampleId :

A4EE6





Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.2	6.7	10.1
100	6.4	5.8	8.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/06/2024

Supervised By :mohammad ahmed 11/08/2024

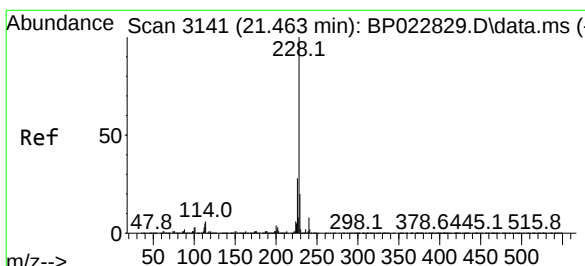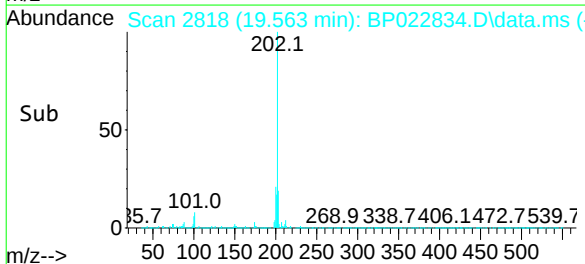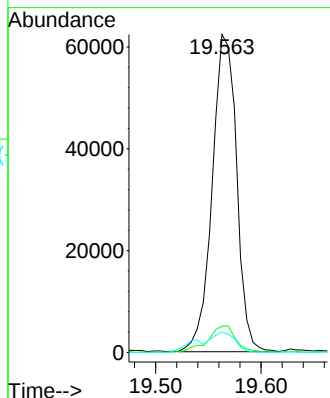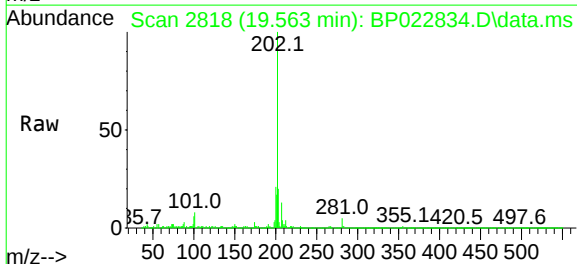

#85

Benzo(a)anthracene

Concen: 1.841 ng/u1




RT: 21.463 min Scan# 3141


Delta R.T. -0.012 min

Lab File: BP022834.D

Acq: 04 Nov 2024 19:42

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.8	15.4	23.0
226	26.9	21.5	32.3

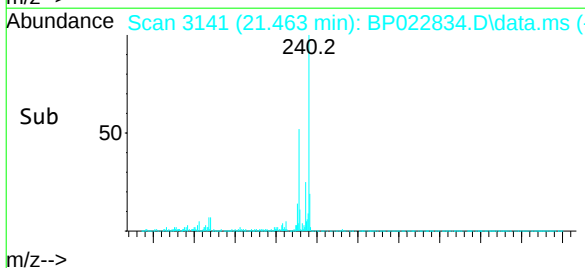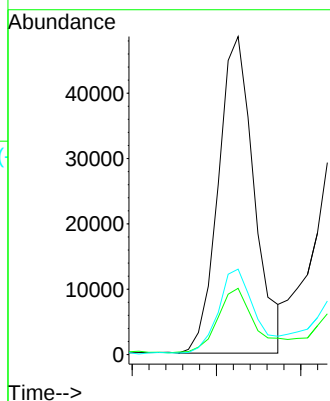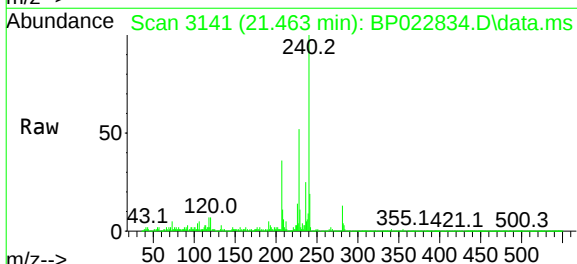

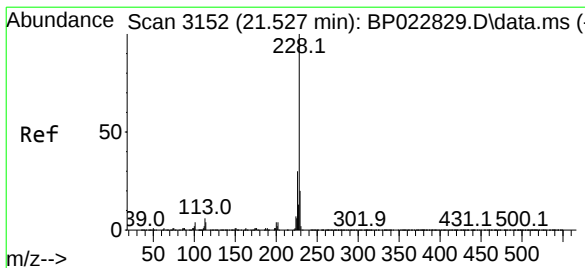

#87

Chrysene

Concen: 2.138 ng/u1

RT: 21.528 min Scan# 31

Delta R.T. -0.023 min

Lab File: BP022834.D

Acq: 04 Nov 2024 19:42

Instrument :

BNA_P

ClientSampleId :

A4EE6





Tgt	Ion:228	Resp:	77344
Ion	Ratio	Lower	Upper
228	100		
226	30.9	23.8	35.8
229	21.1	15.5	23.3

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/06/2024

Supervised By :mohammad ahmed 11/08/2024

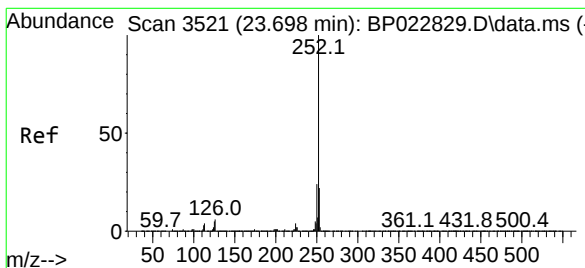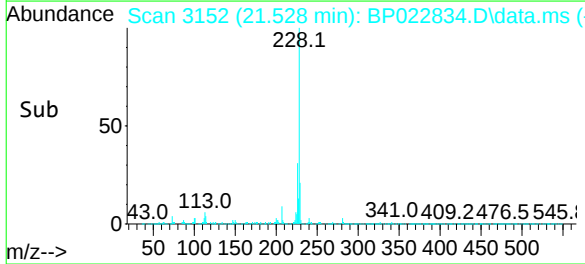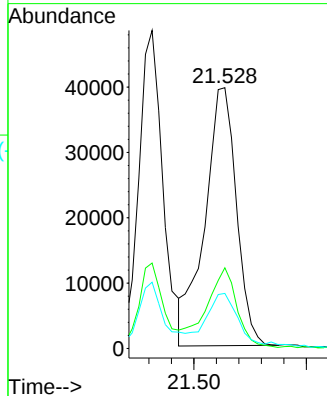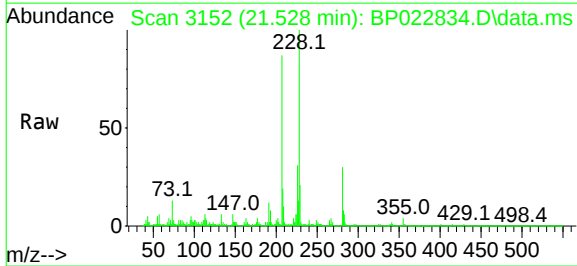

#90

Benzo(b)fluoranthene

Concen: 2.234 ng/u1

RT: 23.716 min Scan# 3524

Delta R.T. -0.006 min

Lab File: BP022834.D

Acq: 04 Nov 2024 19:42

Tgt	Ion:252	Resp:	98615
Ion	Ratio	Lower	Upper
252	100		
253	21.6	17.8	26.8
125	5.5	5.0	7.4

