

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022822.D
 Acq On : 04 Nov 2024 10:56
 Operator : RC/JU
 Sample : PB164462BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	39	rVB	15860	19832	1.10%	0.113%
2	3.593	99	103	121	rBV	156607	268941	14.94%	1.530%
3	3.899	150	155	164	rBV	35795	51372	2.85%	0.292%
4	6.763	639	642	646	rBV5	1574	1840	0.10%	0.010%
5	6.822	646	652	672	rVV	183184	353278	19.62%	2.010%
6	6.975	672	678	690	rBV	156561	261090	14.50%	1.486%
7	7.175	705	712	727	rBV	205513	356936	19.83%	2.031%
8	7.628	780	789	801	rBV	225947	374264	20.79%	2.130%
9	8.339	901	910	926	rBV	257771	458535	25.47%	2.609%
10	8.763	975	982	995	rBV	203866	370594	20.58%	2.109%
11	9.163	1044	1050	1057	rBV5	3865	5359	0.30%	0.030%
12	9.481	1095	1104	1120	rBV	174349	322119	17.89%	1.833%
13	10.028	1190	1197	1227	rBV	239274	515204	28.62%	2.932%
14	10.386	1250	1258	1270	rVB	288605	504677	28.03%	2.872%
15	10.533	1274	1283	1301	rBV	225760	468085	26.00%	2.663%
16	11.645	1468	1472	1479	rVB7	2339	4717	0.26%	0.027%
17	12.004	1526	1533	1535	rBV2	3136	5682	0.32%	0.032%
18	13.651	1807	1813	1825	rBV	684964	881727	48.97%	5.017%
19	13.945	1856	1863	1872	rBV	721885	922140	51.22%	5.247%
20	14.251	1909	1915	1924	rBV	571990	799414	44.40%	4.549%
21	14.522	1955	1961	1975	rBV2	95922	305943	16.99%	1.741%
22	14.963	2032	2036	2040	rBV6	1675	2501	0.14%	0.014%
23	15.269	2079	2088	2102	rVV	876132	1434107	79.65%	8.160%
24	15.410	2103	2112	2125	rBV	184032	361686	20.09%	2.058%
25	15.504	2125	2128	2136	rVB8	4874	11699	0.65%	0.067%
26	15.916	2193	2198	2203	rBV5	2783	4497	0.25%	0.026%
27	15.986	2205	2210	2216	rVB3	5725	8132	0.45%	0.046%
28	16.045	2216	2220	2226	rBV8	1536	2837	0.16%	0.016%
29	16.321	2264	2267	2270	rBV4	4054	4237	0.24%	0.024%
30	16.380	2273	2277	2280	rVV4	7093	8996	0.50%	0.051%
31	16.421	2280	2284	2289	rVB4	5054	7836	0.44%	0.045%
32	16.527	2298	2302	2309	rBV9	2148	4420	0.25%	0.025%
33	16.716	2332	2334	2340	rVB7	1801	2836	0.16%	0.016%
34	16.839	2351	2355	2361	rVB8	2391	3492	0.19%	0.020%
35	17.057	2385	2392	2401	rBV	773996	1067256	59.28%	6.073%
36	17.151	2401	2408	2423	rVV	996710	1449980	80.54%	8.250%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022822.D
Acq On : 04 Nov 2024 10:56
Operator : RC/JU
Sample : PB164462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK462

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	17.998	2550	2552	2556	rVB5	1843	2069	0.11%	0.012%
38	18.486	2633	2635	2637	rBV3	2639	2737	0.15%	0.016%
39	19.086	2733	2737	2742	rBV3	12404	17514	0.97%	0.100%
40	19.162	2746	2750	2758	rVB	12770	20422	1.13%	0.116%
41	19.533	2807	2813	2828	rBV2	1202028	1800412	100.00%	10.244%
42	21.486	3139	3145	3158	rBV2	606102	1242946	69.04%	7.072%
43	24.515	3652	3660	3678	rVB	639940	1706653	94.79%	9.711%
44	24.727	3690	3696	3714	rVB	366618	1155522	64.18%	6.575%




Sum of corrected areas: 17574536

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022822.D
Acq On : 04 Nov 2024 10:56
Operator : RC/JU
Sample : PB164462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

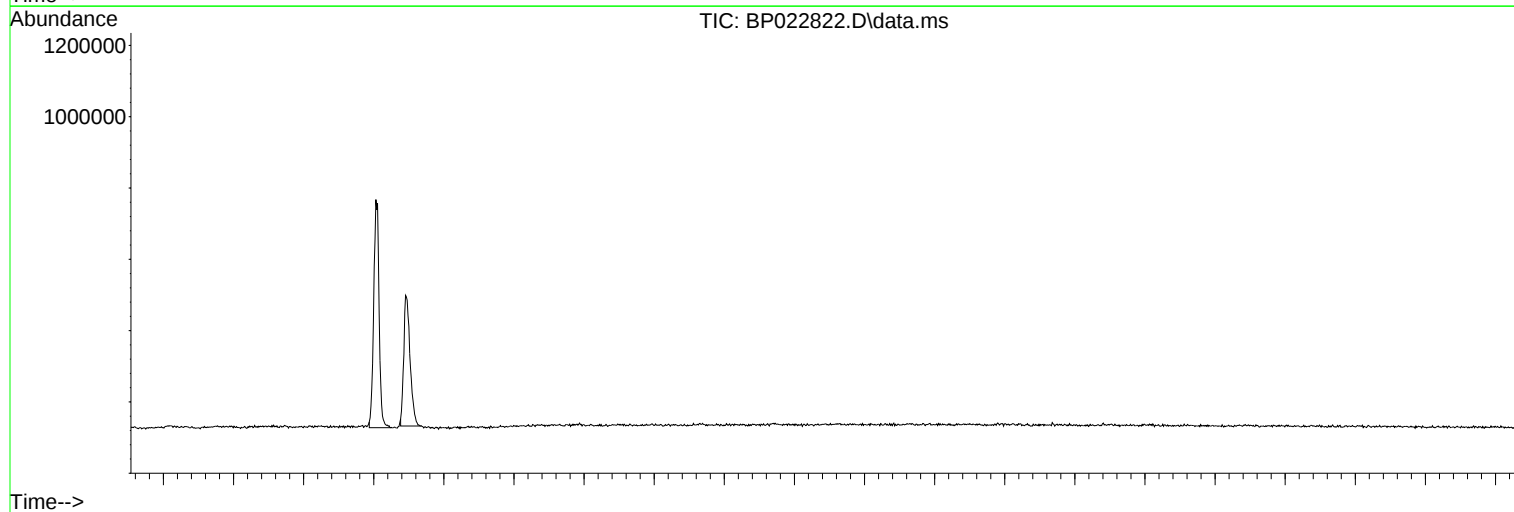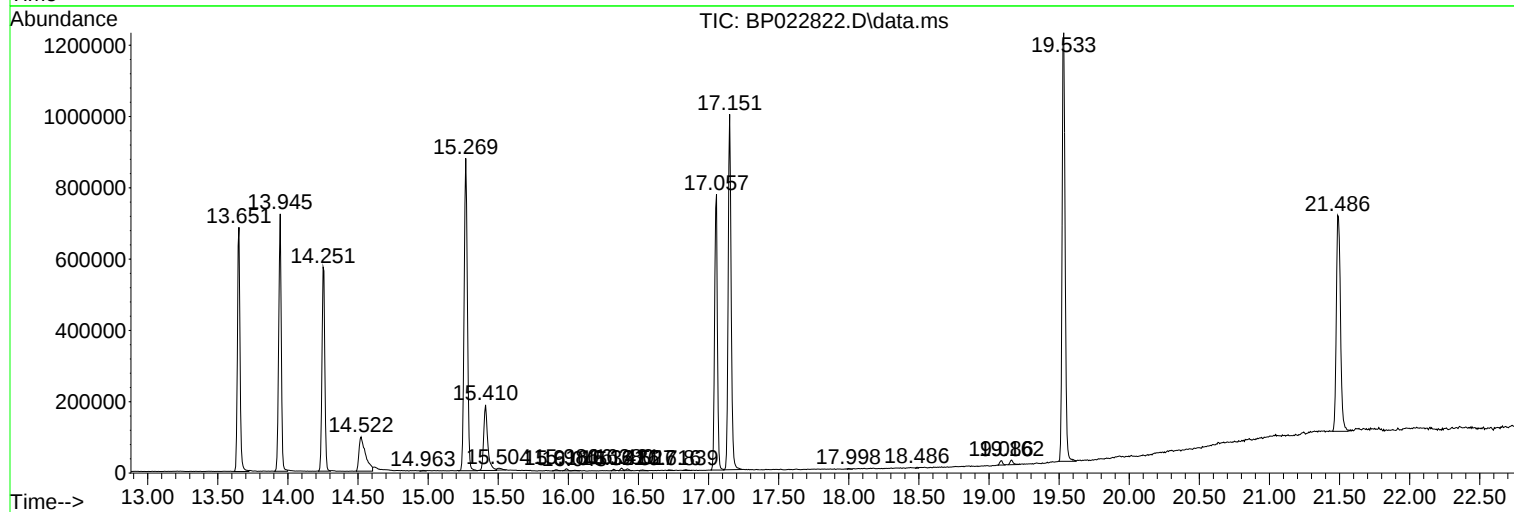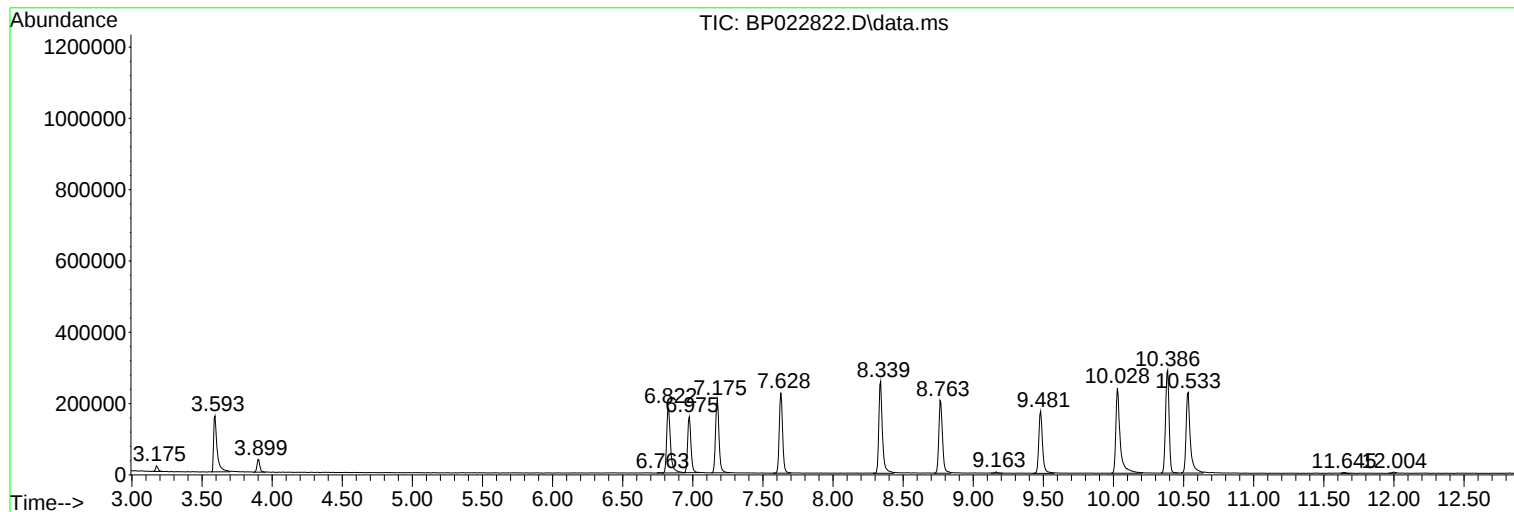

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022822.D
Acq On : 04 Nov 2024 10:56
Operator : RC/JU
Sample : PB164462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022822.D
Acq On : 04 Nov 2024 10:56
Operator : RC/JU
Sample : PB164462BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc