

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022824.D
 Acq On : 04 Nov 2024 12:57
 Operator : RC/JU
 Sample : P4568-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	38	rVB3	5462	7019	0.35%	0.054%
2	3.622	105	108	112	rBV4	5125	9200	0.46%	0.071%
3	3.687	116	119	124	rVB5	2852	4725	0.24%	0.036%
4	3.811	135	140	143	rVB6	1853	3327	0.17%	0.026%
5	3.905	152	156	160	rBV2	5329	7508	0.38%	0.058%
6	4.069	179	184	190	rBV7	3432	5199	0.26%	0.040%
7	4.269	215	218	223	rVB7	3513	5019	0.25%	0.039%
8	4.446	243	248	255	rBV8	4787	7752	0.39%	0.060%
9	4.799	303	308	313	rBV2	7202	11219	0.56%	0.086%
10	5.475	417	423	426	rBV3	8200	13887	0.69%	0.107%
11	5.663	451	455	458	rBV5	4123	7454	0.37%	0.057%
12	5.793	475	477	482	rVB5	2445	3633	0.18%	0.028%
13	6.005	507	513	518	rBV3	20031	31809	1.59%	0.244%
14	6.052	518	521	527	rVB8	3805	5884	0.29%	0.045%
15	6.169	539	541	544	rBV4	1723	2072	0.10%	0.016%
16	6.228	544	551	552	rBV6	5170	7361	0.37%	0.057%
17	6.458	585	590	593	rVV	10059	14676	0.73%	0.113%
18	6.499	593	597	607	rVB2	14620	23814	1.19%	0.183%
19	6.581	607	611	615	rBV6	2909	4106	0.21%	0.032%
20	6.775	640	644	646	rBV4	1447	2211	0.11%	0.017%
21	6.834	646	654	671	rVV4	58799	172445	8.62%	1.324%
22	6.975	673	678	688	rVB	50861	87180	4.36%	0.669%
23	7.175	706	712	722	rBV2	67162	117107	5.86%	0.899%
24	7.246	722	724	728	rVB5	1931	2700	0.13%	0.021%
25	7.628	781	789	802	rBV	337878	561299	28.06%	4.310%
26	8.275	895	899	903	rBV6	1861	2757	0.14%	0.021%
27	8.346	903	911	922	rBV	55752	120592	6.03%	0.926%
28	8.446	922	928	941	rVB	125002	220218	11.01%	1.691%
29	8.775	978	984	997	rBV	68488	123387	6.17%	0.947%
30	9.169	1044	1051	1058	rBV2	6718	10633	0.53%	0.082%
31	9.351	1077	1082	1095	rVB9	4085	11136	0.56%	0.086%
32	9.487	1098	1105	1117	rBV	48532	101778	5.09%	0.782%
33	9.704	1136	1142	1147	rBV3	12184	28483	1.42%	0.219%
34	9.857	1161	1168	1174	rBV3	8879	21920	1.10%	0.168%
35	10.040	1193	1199	1211	rBV2	70023	157540	7.88%	1.210%
36	10.381	1249	1257	1270	rBV	434815	781553	39.08%	6.001%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022824.D
 Acq On : 04 Nov 2024 12:57
 Operator : RC/JU
 Sample : P4568-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	10.557	1281	1287	1304	rBV2	18139	44157	2.21%	0.339%
38	10.963	1350	1356	1360	rBV8	3912	9690	0.48%	0.074%
39	11.216	1394	1399	1400	rBV3	3219	3956	0.20%	0.030%
40	11.428	1432	1435	1446	rVB3	2306	6544	0.33%	0.050%
41	11.651	1466	1473	1479	rBV4	5702	10242	0.51%	0.079%
42	11.793	1491	1497	1505	rVB7	4318	9977	0.50%	0.077%
43	11.910	1512	1517	1520	rBV6	1742	2533	0.13%	0.019%
44	11.987	1525	1530	1535	rVB7	2035	3729	0.19%	0.029%
45	12.051	1535	1541	1546	rBV10	1325	3298	0.16%	0.025%
46	13.557	1790	1797	1800	rBV9	1744	3579	0.18%	0.027%
47	13.663	1808	1815	1828	rBV	189566	308454	15.42%	2.369%
48	13.934	1854	1861	1873	rBV2	190966	312000	15.60%	2.396%
49	14.245	1907	1914	1923	rBV	840936	1247946	62.40%	9.583%
50	14.316	1923	1926	1932	rVV5	5415	9233	0.46%	0.071%
51	14.392	1934	1939	1942	rBV7	1398	2525	0.13%	0.019%
52	14.539	1957	1964	1977	rBV3	17296	60781	3.04%	0.467%
53	14.698	1984	1991	1994	rBV8	8772	19829	0.99%	0.152%
54	15.092	2056	2058	2061	rVV4	2469	2071	0.10%	0.016%
55	15.128	2061	2064	2066	rVB4	1758	2002	0.10%	0.015%
56	15.257	2080	2086	2092	rBV	313613	465401	23.27%	3.574%
57	15.422	2108	2114	2123	rBV	38690	76114	3.81%	0.584%
58	15.516	2128	2130	2136	rVB6	4408	6766	0.34%	0.052%
59	15.639	2143	2151	2158	rBV	30499	54919	2.75%	0.422%
60	16.010	2209	2214	2221	rVV	3703	9141	0.46%	0.070%
61	16.128	2229	2234	2238	rBV2	4606	7946	0.40%	0.061%
62	16.186	2240	2244	2249	rVB8	4973	9016	0.45%	0.069%
63	16.245	2249	2254	2256	rBV6	2457	4319	0.22%	0.033%
64	16.398	2277	2280	2285	rBV7	2212	3130	0.16%	0.024%
65	16.457	2285	2290	2295	rBV7	7121	12275	0.61%	0.094%
66	16.528	2296	2302	2306	rBV2	11286	21041	1.05%	0.162%
67	16.686	2327	2329	2331	rBV3	2237	2067	0.10%	0.016%
68	16.716	2331	2334	2341	rVB9	3366	5470	0.27%	0.042%
69	16.816	2347	2351	2352	rBV4	1966	2226	0.11%	0.017%
70	16.839	2352	2355	2357	rBV3	2247	2678	0.13%	0.021%
71	17.051	2384	2391	2396	rBV	1132918	1712689	85.63%	13.152%
72	17.098	2396	2399	2404	rVV	85133	121298	6.06%	0.931%
73	17.163	2404	2410	2421	rVV2	273752	499336	24.97%	3.834%
74	17.239	2421	2423	2426	rVB4	3897	4556	0.23%	0.035%
75	17.498	2460	2467	2470	rBV8	5423	12088	0.60%	0.093%
76	17.575	2478	2480	2483	rBV4	3849	4925	0.25%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022824.D
 Acq On : 04 Nov 2024 12:57
 Operator : RC/JU
 Sample : P4568-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

77	17.633	2487	2490	2493	rBV3	5882	8451	0.42%	0.065%
78	17.663	2493	2495	2497	rBV3	2838	2926	0.15%	0.022%
79	17.751	2506	2510	2513	rBV5	4240	5393	0.27%	0.041%
80	17.863	2524	2529	2534	rBV3	14353	22729	1.14%	0.175%
81	17.980	2543	2549	2553	rBV2	95071	139711	6.99%	1.073%
82	18.022	2553	2556	2559	rVB	16239	23092	1.15%	0.177%
83	18.086	2566	2567	2568	rBV	3750	2421	0.12%	0.019%
84	18.157	2574	2579	2583	rBV3	19497	34103	1.71%	0.262%
85	18.192	2583	2585	2586	rBV2	3497	2652	0.13%	0.020%
86	18.445	2624	2628	2630	rBV5	10416	12503	0.63%	0.096%
87	18.475	2630	2633	2637	rVB3	8726	11243	0.56%	0.086%
88	18.580	2648	2651	2655	rBV4	12614	15968	0.80%	0.123%
89	18.810	2687	2690	2695	rVB	32914	41884	2.09%	0.322%
90	18.863	2696	2699	2704	rVB	16415	19845	0.99%	0.152%
91	18.916	2705	2708	2710	rBV3	7319	8722	0.44%	0.067%
92	19.086	2734	2737	2743	rBV8	21911	32544	1.63%	0.250%
93	19.186	2749	2754	2759	rVB	184839	252729	12.64%	1.941%
94	19.316	2772	2776	2785	rVB5	46159	74433	3.72%	0.572%
95	19.451	2797	2799	2803	rBV4	9446	10929	0.55%	0.084%
96	19.539	2809	2814	2817	rBV	371113	518774	25.94%	3.984%
97	20.192	2921	2925	2930	rBV6	24381	50589	2.53%	0.388%
98	21.492	3139	3146	3151	rBV	1202792	2000025	100.00%	15.358%
99	24.751	3689	3700	3710	rBV	648401	1932509	96.62%	14.840%

Sum of corrected areas: 13022725




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022824.D
Acq On : 04 Nov 2024 12:57
Operator : RC/JU
Sample : P4568-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

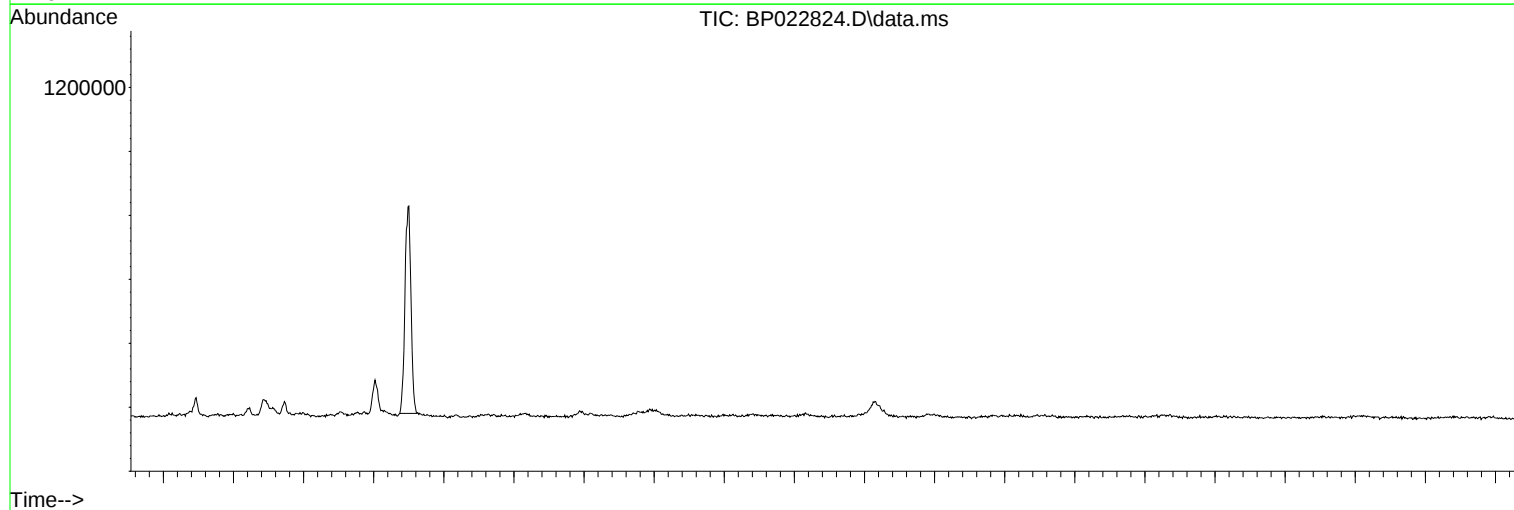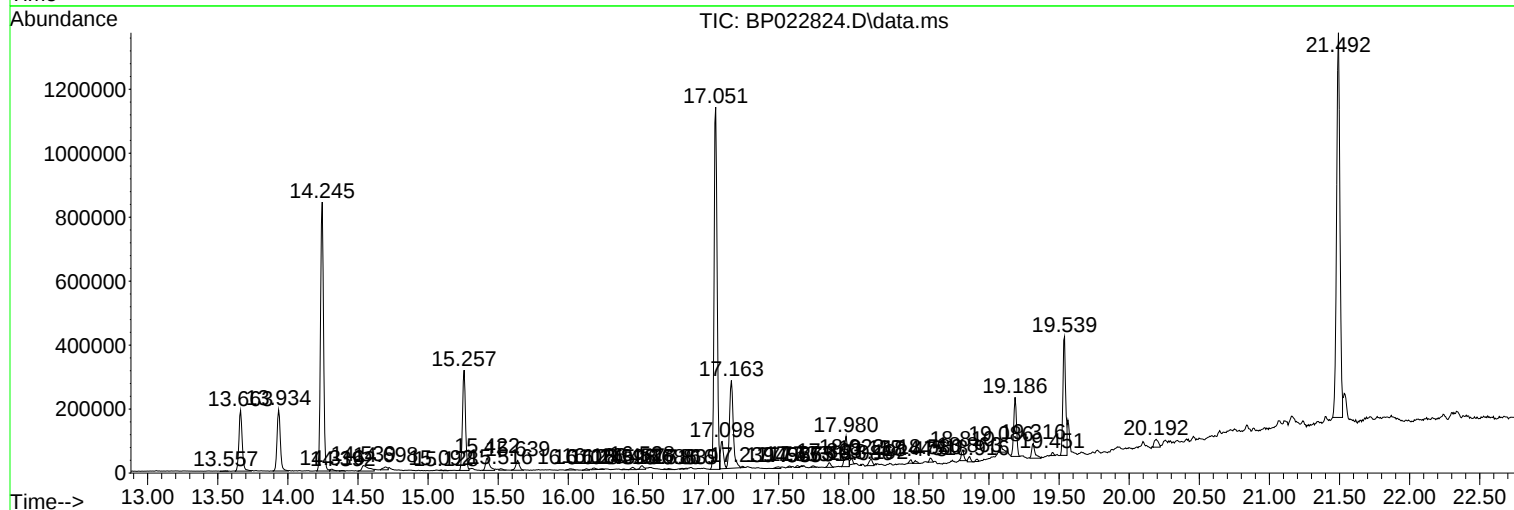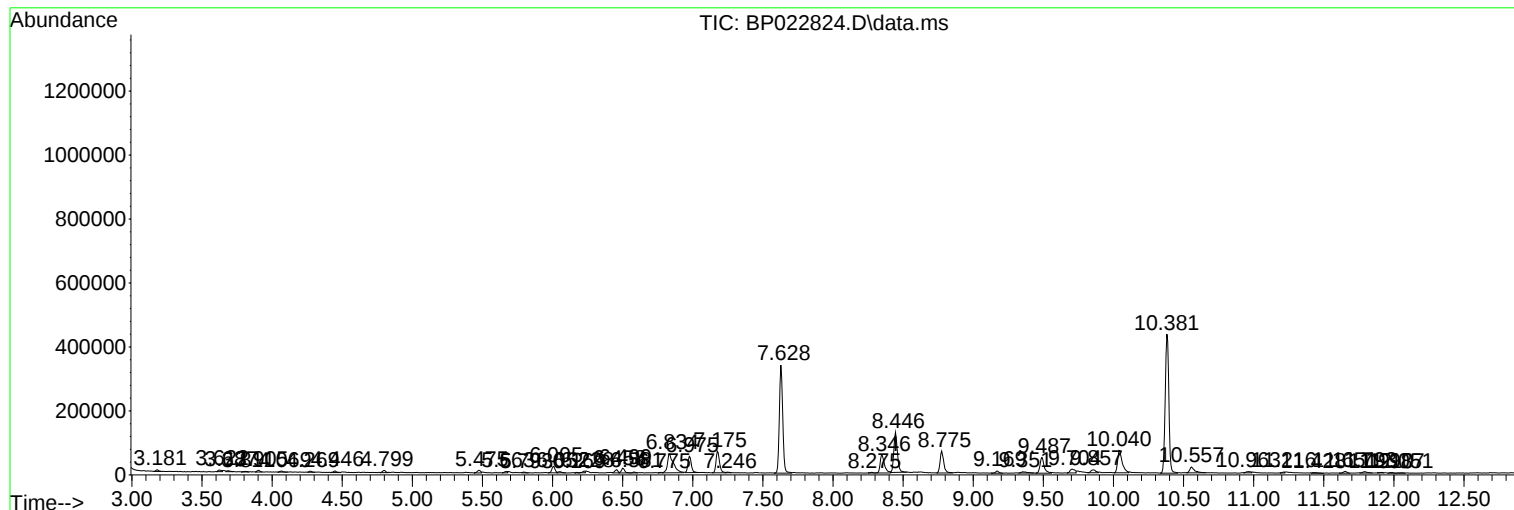

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022824.D
Acq On : 04 Nov 2024 12:57
Operator : RC/JU
Sample : P4568-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022824.D
Acq On : 04 Nov 2024 12:57
Operator : RC/JU
Sample : P4568-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc