

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
 Data File : BP022827.D
 Acq On : 04 Nov 2024 14:58
 Operator : RC/JU
 Sample : P4568-02DL 5X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.904	151	156	163	rVB2	6607	9932	0.29%	0.024%
2	4.428	239	245	249	rBV5	8394	12942	0.38%	0.031%
3	6.769	640	643	648	rBV5	2629	3620	0.11%	0.009%
4	6.857	648	658	671	rVV2	70990	188654	5.55%	0.454%
5	6.975	673	678	687	rVB	30289	49358	1.45%	0.119%
6	7.069	687	694	704	rBV	300318	463199	13.63%	1.114%
7	7.210	713	718	734	rVB	176185	322224	9.48%	0.775%
8	7.628	781	789	792	rBV	313393	543121	15.98%	1.306%
9	7.663	792	795	807	rVB	523970	805544	23.70%	1.937%
10	7.975	839	848	857	rBV	547012	869476	25.58%	2.091%
11	8.351	905	912	918	rBV	40967	81143	2.39%	0.195%
12	8.422	918	924	937	rVB	368164	593022	17.45%	1.426%
13	8.687	961	969	977	rVB	293395	478595	14.08%	1.151%
14	8.775	978	984	987	rVV	43720	68838	2.03%	0.166%
15	8.816	987	991	1005	rVB	72089	135391	3.98%	0.326%
16	9.175	1046	1052	1058	rVB6	5925	11560	0.34%	0.028%
17	9.328	1071	1078	1088	rBV	445672	758463	22.31%	1.824%
18	9.486	1097	1105	1106	rBV	37750	46507	1.37%	0.112%
19	9.516	1106	1110	1122	rVV2	77491	145996	4.30%	0.351%
20	9.634	1125	1130	1138	rVB	16620	28999	0.85%	0.070%
21	9.804	1150	1159	1172	rBV	375615	600501	17.67%	1.444%
22	10.057	1189	1202	1219	rBV2	243763	605819	17.82%	1.457%
23	10.381	1246	1257	1265	rBV	416334	704204	20.72%	1.693%
24	10.539	1280	1284	1296	rBV	28026	57873	1.70%	0.139%
25	10.704	1303	1312	1321	rVB	499821	841295	24.75%	2.023%
26	11.639	1465	1471	1474	rBV6	3414	6210	0.18%	0.015%
27	11.692	1474	1480	1496	rVB	98827	185453	5.46%	0.446%
28	11.933	1516	1521	1527	rBV3	4320	8485	0.25%	0.020%
29	12.045	1532	1540	1556	rBV	246320	420482	12.37%	1.011%
30	12.469	1607	1612	1618	rBV5	3581	6845	0.20%	0.016%
31	12.669	1638	1646	1657	rBV	545658	984061	28.95%	2.367%
32	12.763	1657	1662	1677	rVB	116069	214806	6.32%	0.517%
33	13.292	1748	1752	1759	rVB9	2063	3441	0.10%	0.008%
34	13.651	1806	1813	1826	rVB	95086	175470	5.16%	0.422%
35	13.833	1836	1844	1851	rBV	737776	989925	29.12%	2.381%
36	13.933	1855	1861	1864	rVV	142783	226412	6.66%	0.544%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022827.D
Acq On : 04 Nov 2024 14:58
Operator : RC/JU
Sample : P4568-02DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	13.963	1864	1866	1872	rVB	104764	128985	3.79%	0.310%
38	14.151	1891	1898	1901	rBV8	1704	3810	0.11%	0.009%
39	14.245	1908	1914	1919	rBV	861456	1075779	31.65%	2.587%
40	14.304	1919	1924	1932	rVV	823803	1064441	31.31%	2.560%

41	14.380	1932	1937	1943	rVB5	6278	10719	0.32%	0.026%
42	14.516	1953	1960	1968	rBV3	104882	256023	7.53%	0.616%
43	14.633	1974	1980	1994	rVB	419080	678302	19.95%	1.631%
44	14.904	2021	2026	2032	rVB4	8542	14330	0.42%	0.034%
45	15.257	2080	2086	2089	rBV	221895	274440	8.07%	0.660%

46	15.304	2089	2094	2108	rVB2	1516445	2189281	64.41%	5.265%
47	15.421	2108	2114	2121	rBV3	19904	40297	1.19%	0.097%
48	15.574	2135	2140	2145	rBV	16842	23267	0.68%	0.056%
49	15.627	2145	2149	2156	rVV	44866	62110	1.83%	0.149%
50	15.916	2195	2198	2202	rBV6	3089	4192	0.12%	0.010%

51	16.004	2207	2213	2223	rVB6	5846	14325	0.42%	0.034%
52	16.227	2242	2251	2263	rBV	243202	329405	9.69%	0.792%
53	16.339	2263	2270	2280	rVV	1520388	2037176	59.93%	4.899%
54	16.586	2309	2312	2316	rVB5	3088	3758	0.11%	0.009%
55	16.704	2324	2332	2350	rBV	758053	1266752	37.27%	3.046%

56	17.045	2384	2390	2395	rBV	929922	1401184	41.22%	3.370%
57	17.092	2395	2398	2404	rVV	300761	469398	13.81%	1.129%
58	17.157	2404	2409	2412	rVV2	176430	283870	8.35%	0.683%
59	17.198	2412	2416	2424	rVV	313276	470354	13.84%	1.131%
60	17.686	2495	2499	2505	rBV8	10279	14890	0.44%	0.036%

61	17.751	2506	2510	2515	rVB3	11429	15126	0.44%	0.036%
62	17.980	2546	2549	2554	rBV4	30263	37181	1.09%	0.089%
63	18.057	2556	2562	2571	rVV	1010900	1300796	38.27%	3.128%
64	18.533	2640	2643	2651	rVB4	18667	31571	0.93%	0.076%
65	19.074	2733	2735	2739	rBV5	5450	7422	0.22%	0.018%

66	19.180	2747	2753	2765	rBV	1372245	1985585	58.41%	4.775%
67	19.321	2775	2777	2782	rBV6	7481	8503	0.25%	0.020%
68	19.445	2794	2798	2803	rBV	12116	20584	0.61%	0.050%
69	19.533	2807	2813	2815	rVV	287504	418286	12.31%	1.006%
70	19.562	2815	2818	2826	rVB	595536	843363	24.81%	2.028%

71	20.509	2975	2979	2984	rBV	255160	315477	9.28%	0.759%
72	21.392	3124	3129	3135	rBV	1167594	1517784	44.65%	3.650%
73	21.480	3135	3144	3150	rVV3	1242798	3399203	100.00%	8.175%
74	21.539	3150	3154	3165	rVB	1851165	2764799	81.34%	6.649%
75	23.703	3513	3522	3537	rVB	1172279	2656972	78.16%	6.390%

76	24.503	3652	3658	3663	rBV	156972	310007	9.12%	0.746%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022827.D
Acq On : 04 Nov 2024 14:58
Operator : RC/JU
Sample : P4568-02DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EA4DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

77	24.562	3664	3668	3679	rVB	208108	492591	14.49%	1.185%
78	24.733	3687	3697	3709	rVB	548953	1692686	49.80%	4.071%

Sum of corrected areas: 41582890




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022827.D
Acq On : 04 Nov 2024 14:58
Operator : RC/JU
Sample : P4568-02DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

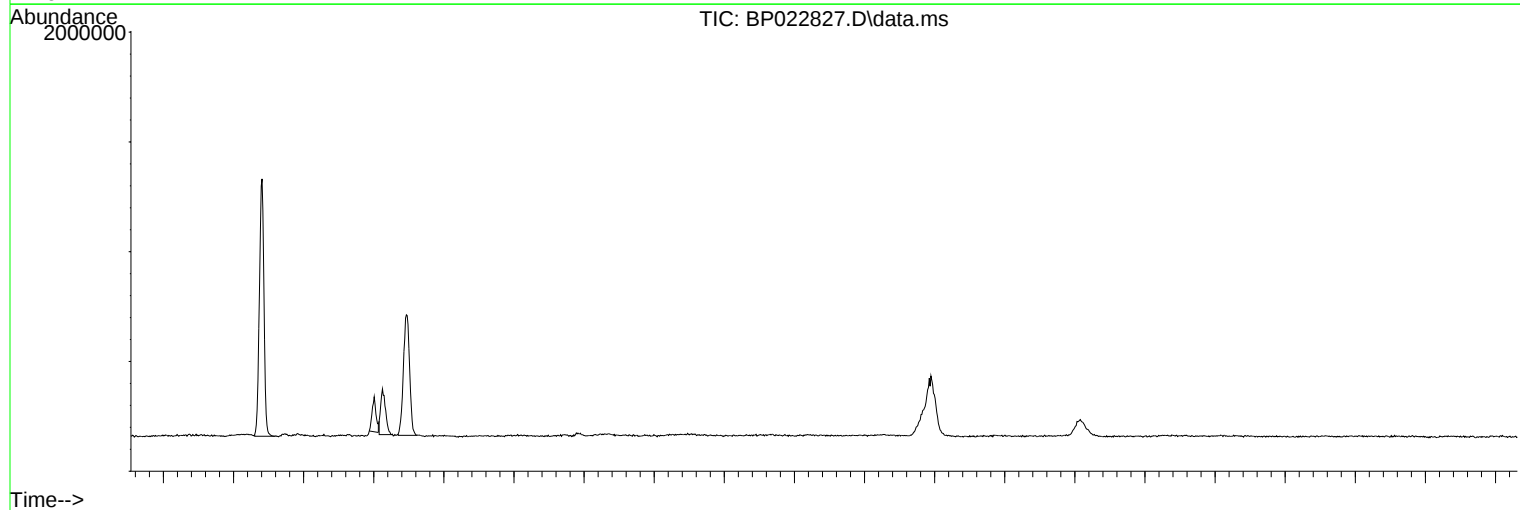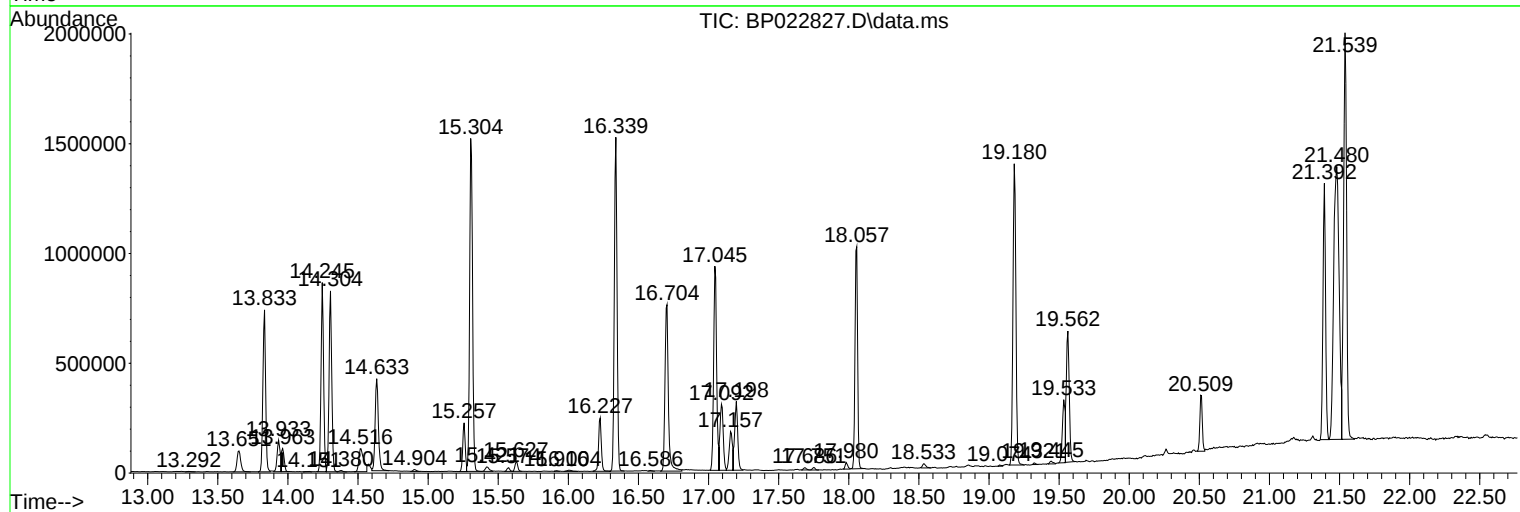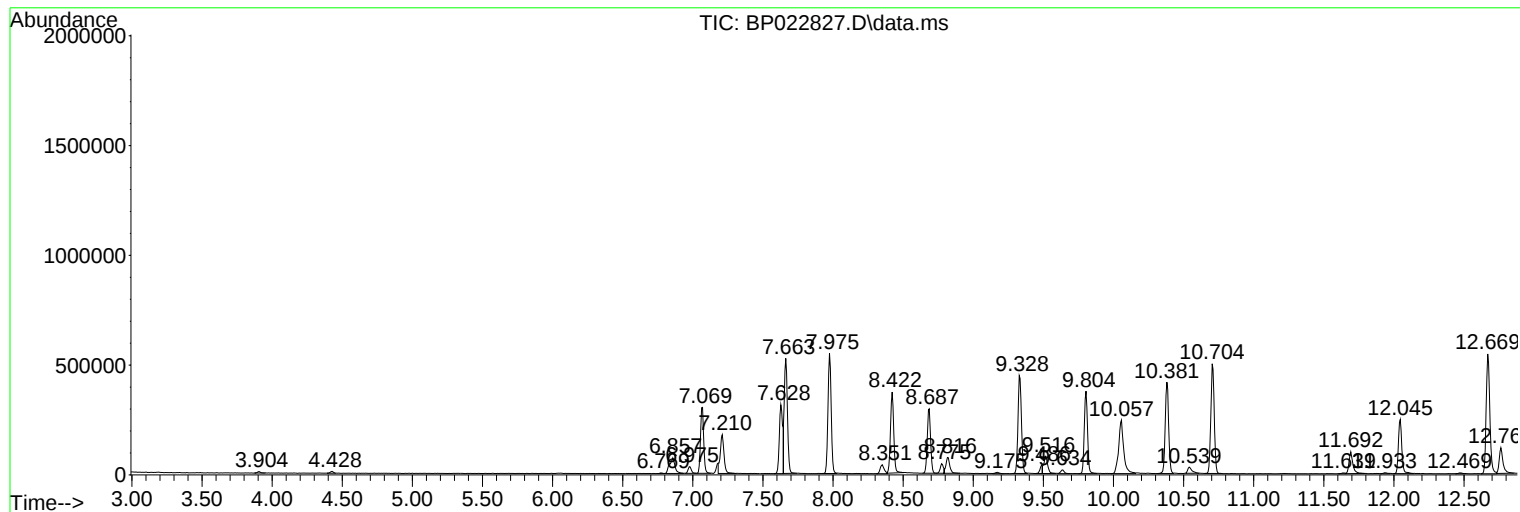

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022827.D
Acq On : 04 Nov 2024 14:58
Operator : RC/JU
Sample : P4568-02DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION










TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3-dichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.975	32.02 ng/ul	869476	1,4-Dichlorobenzene-d4	7.628

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	98
2	Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
3	Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
4	Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
5	Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97

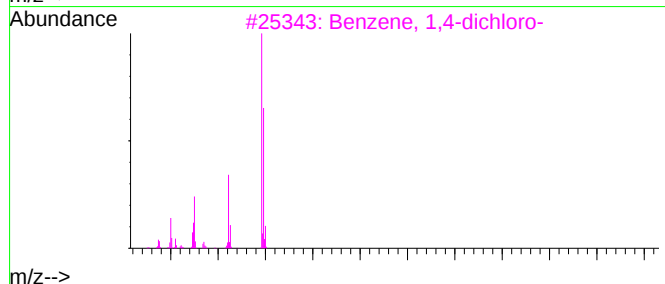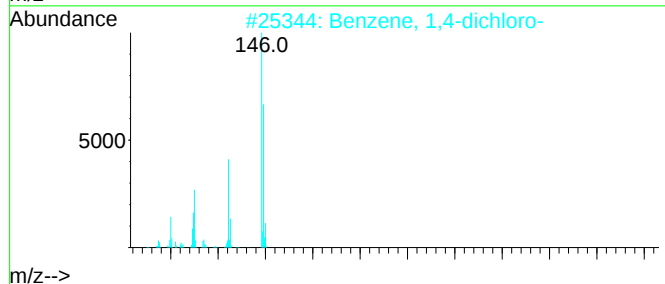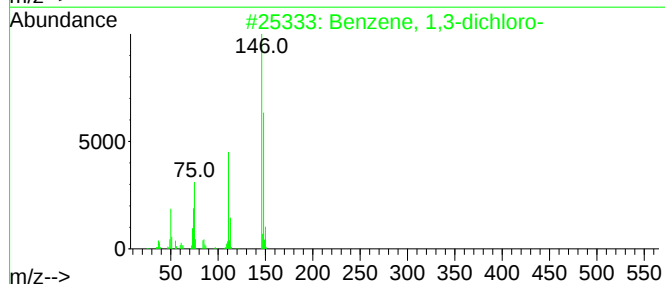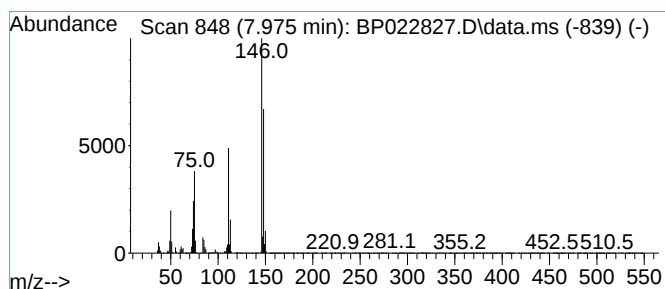

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110424\
Data File : BP022827.D
Acq On : 04 Nov 2024 14:58
Operator : RC/JU
Sample : P4568-02DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc

Benzene, 1,3-di...	7.975	32.0	ng/ul	869476	1	7.628	543121	20.0